


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070717\
 Data File : BF096549.D
 Acq On : 7 Jul 2017 10:37
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 13:02:33 2017

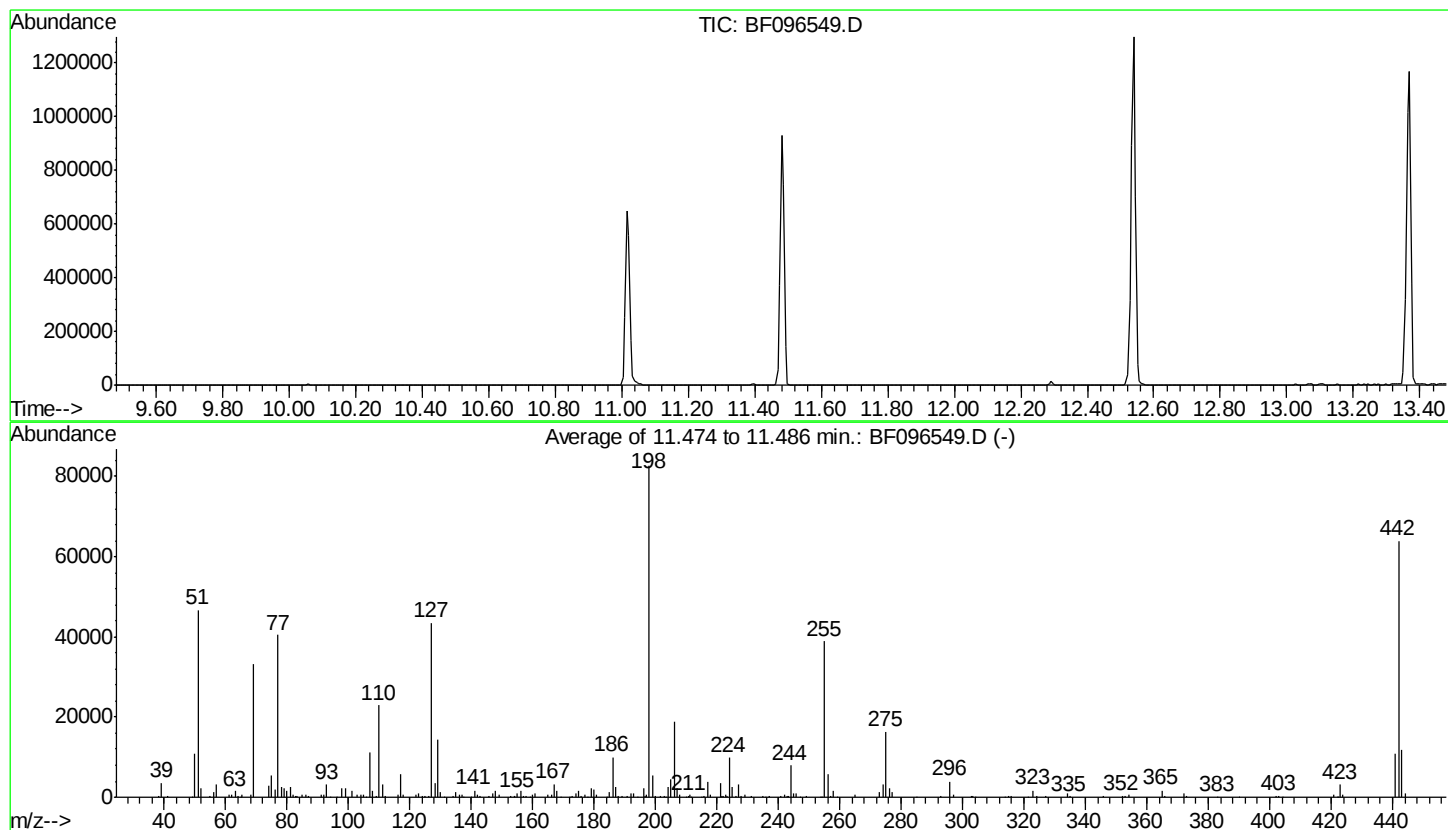

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	46704	PASS
68	69	0.00	2	1.9	638	PASS
69	198	0.00	100	40.1	33141	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	43493	PASS
197	198	0.00	2	0.9	731	PASS
198	198	100	100	100.0	82704	PASS
199	198	5	9	6.4	5289	PASS
275	198	10	60	19.7	16333	PASS
365	198	1	100	2.0	1693	PASS
441	442	0.01	24	17.0	10884	PASS
442	198	50	100	77.4	63994	PASS
443	442	15	24	18.6	11871	PASS