
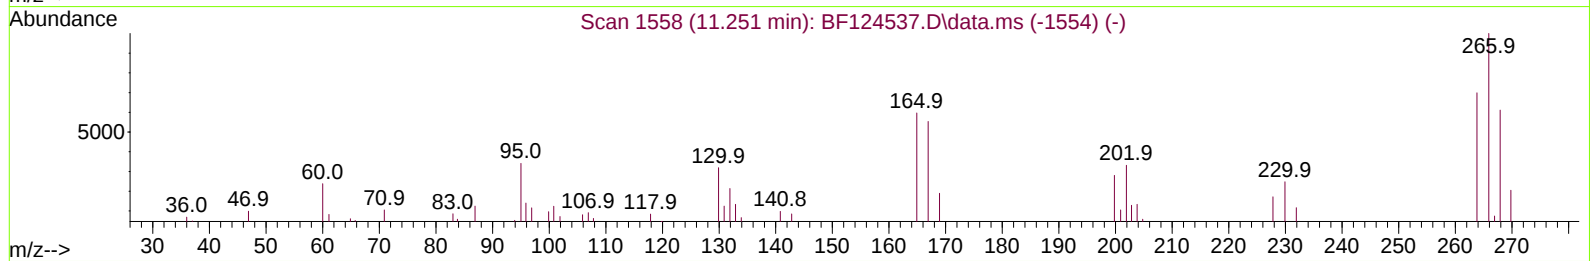
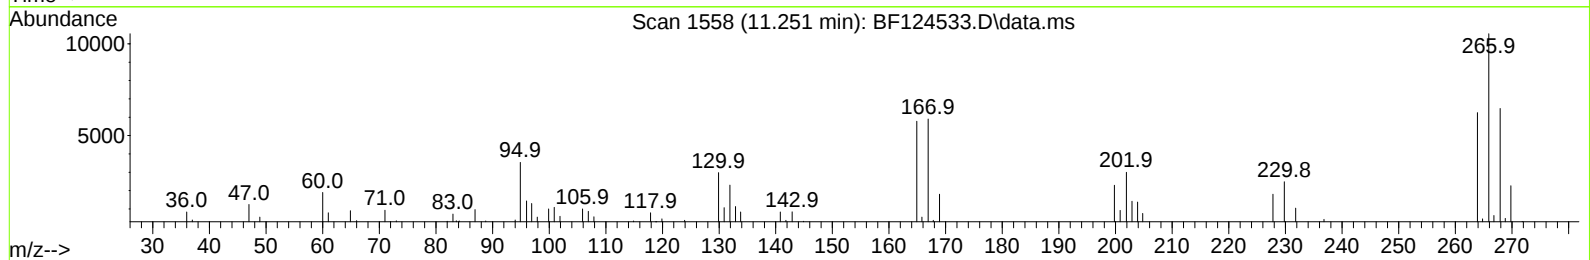


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
Data File : BF124533.D
Acq On : 7 Jul 2021 16:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 05:34:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 05:15:31 2021
Response via : Initial Calibration

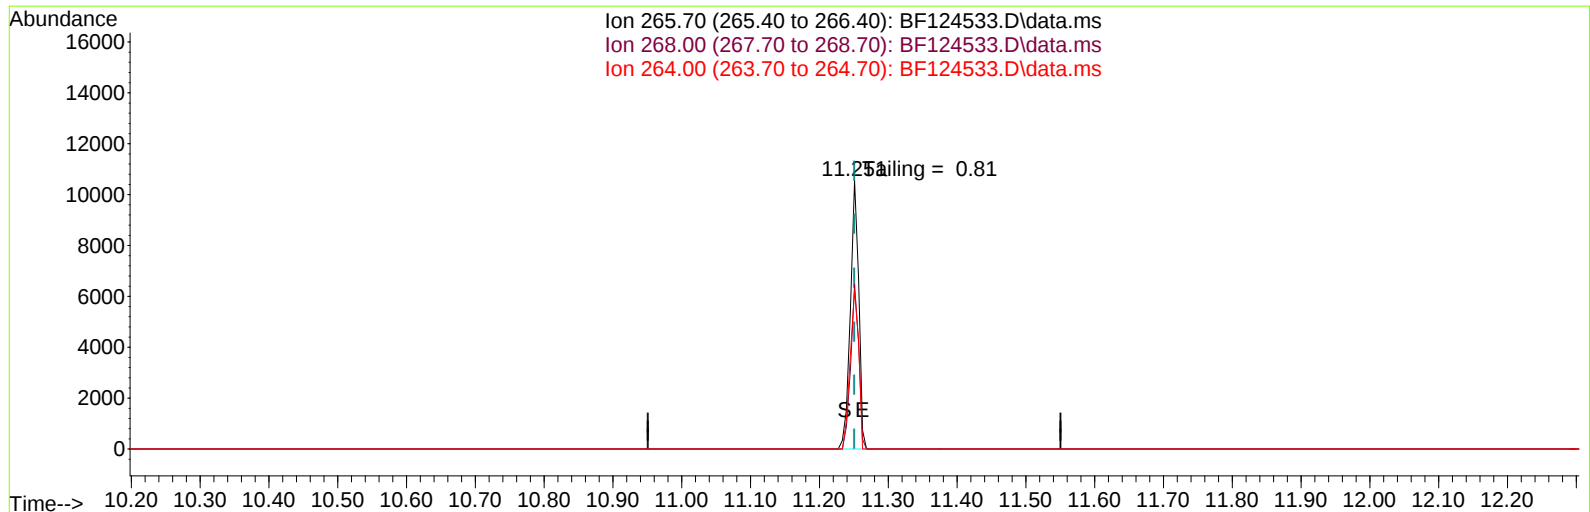

TIC: BF124533.D\data.ms




(70) Pentachlorophenol (C)

11.251min (+ 0.000) 0.00 ng

response 8938

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.36
264.00	69.90	59.29
0.00	0.00	0.00

Quant Time: Jul 08 05:34:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 05:15:31 2021
Response via : Initial Calibration

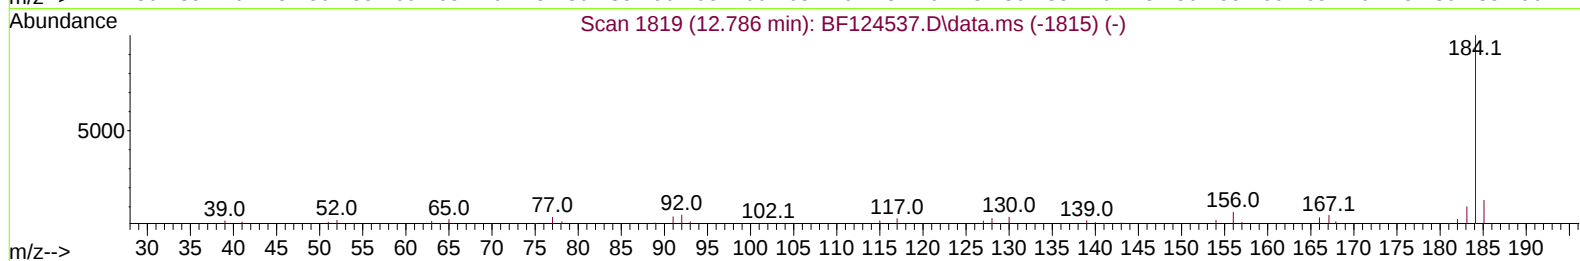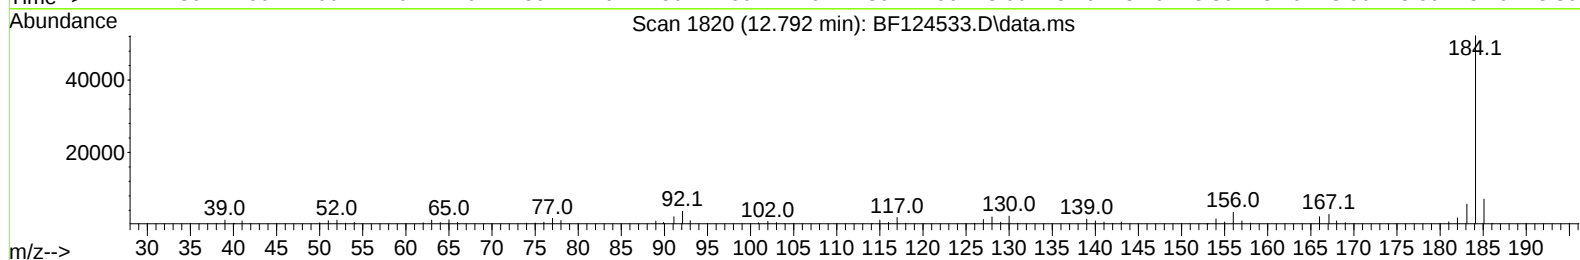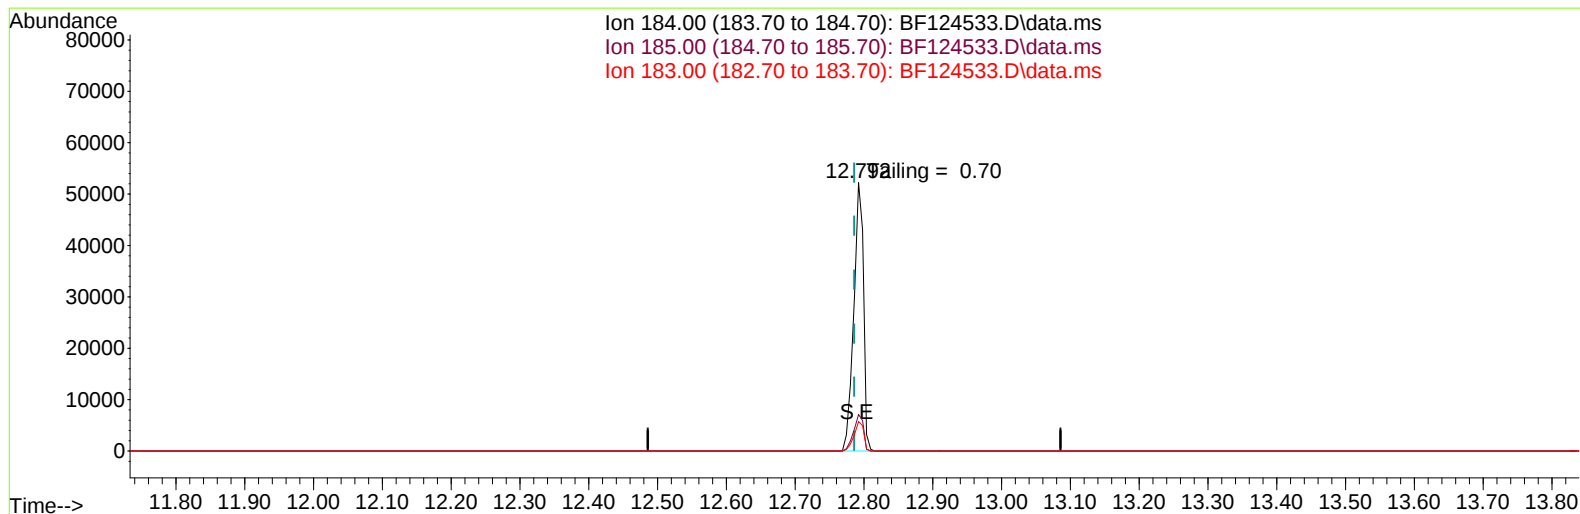

TIC: BF124533.D\data.ms

(77) Benzidine

12.792min (+ 0.006) 0.00 ng

response 51277

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.59
183.00	10.10	10.97
0.00	0.00	0.00