

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
 Data File : BF124542.D
 Acq On : 7 Jul 2021 22:58
 Operator : JU/CG
 Sample : PB137511BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137511BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	529	531	536	rBB	2612	3439	1.10%	0.204%
2	5.563	585	591	594	rBB	193140	216525	69.56%	12.819%
3	6.551	752	759	761	rBB	165950	221051	71.02%	13.087%
4	6.922	819	822	825	rBB	46781	41153	13.22%	2.436%
5	7.486	912	918	921	rBB	114119	145280	46.67%	8.601%
6	8.204	1036	1040	1043	rBB	58342	56754	18.23%	3.360%
7	9.286	1217	1224	1227	rBB	291472	296954	95.40%	17.580%
8	9.963	1334	1339	1342	rBB	78653	66801	21.46%	3.955%
9	10.757	1468	1474	1477	rBB	191931	177516	57.03%	10.509%
10	11.451	1588	1592	1595	rBV	83828	68956	22.15%	4.082%
11	13.051	1858	1864	1867	rBB	304472	311262	100.00%	18.427%
12	14.092	2037	2041	2044	rBB	60891	49497	15.90%	2.930%
13	15.586	2291	2295	2299	rBB	30166	33947	10.91%	2.010%




Sum of corrected areas: 1689135

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
Data File : BF124542.D
Acq On : 7 Jul 2021 22:58
Operator : JU/CG
Sample : PB137511BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137511BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

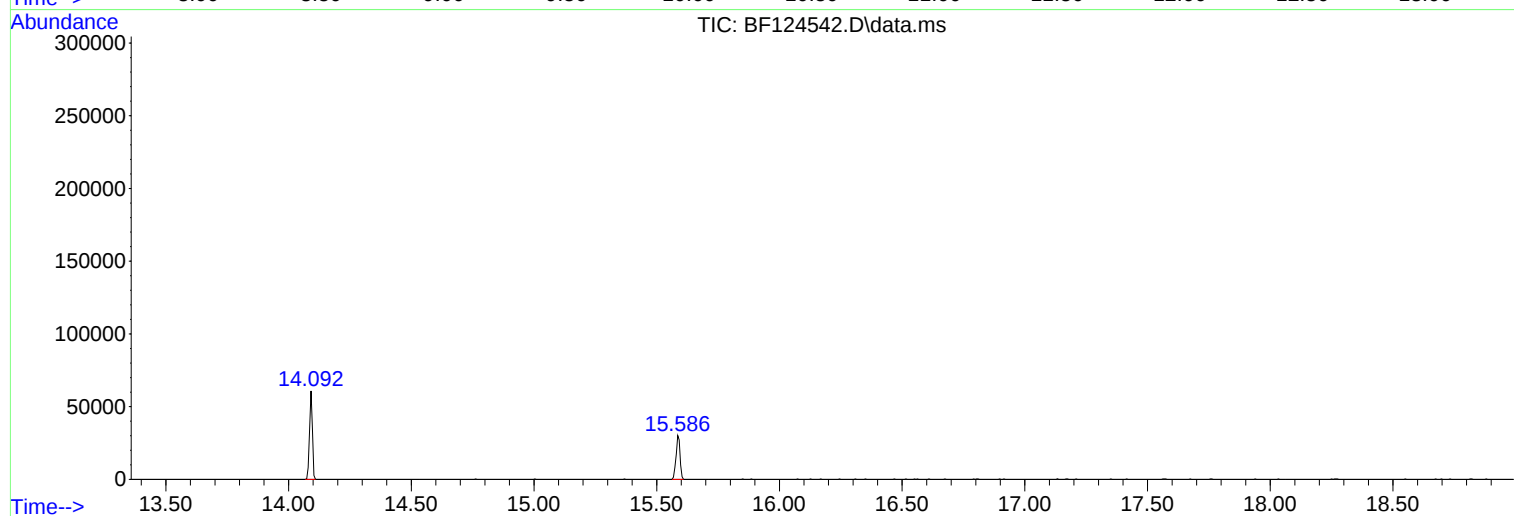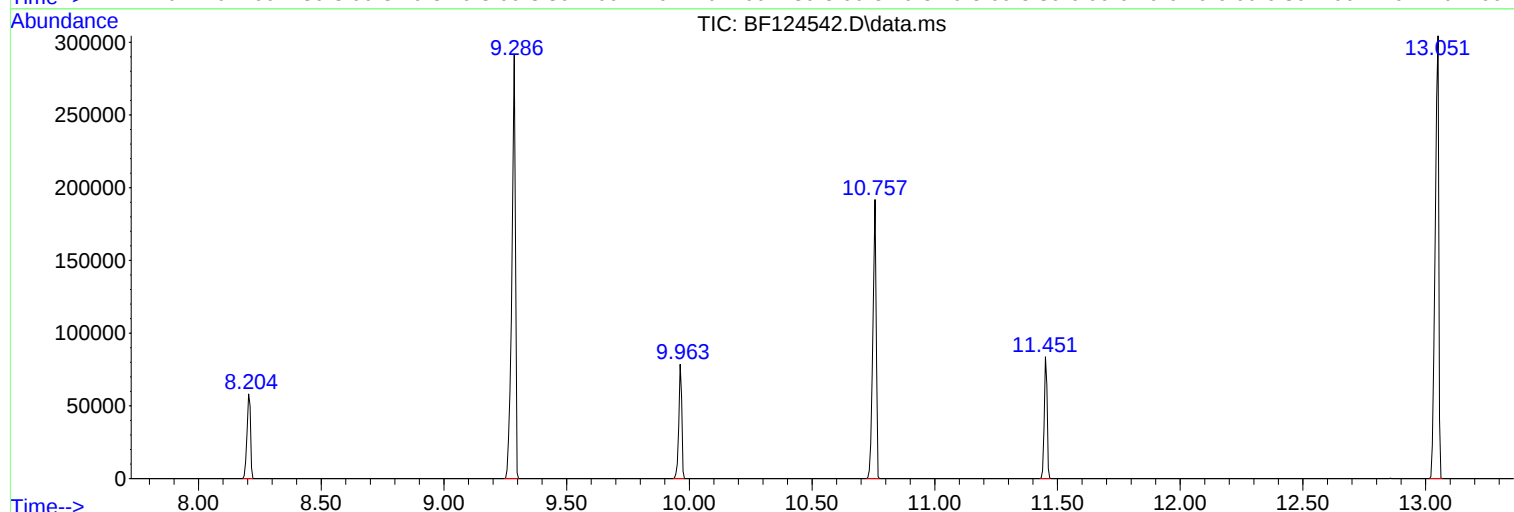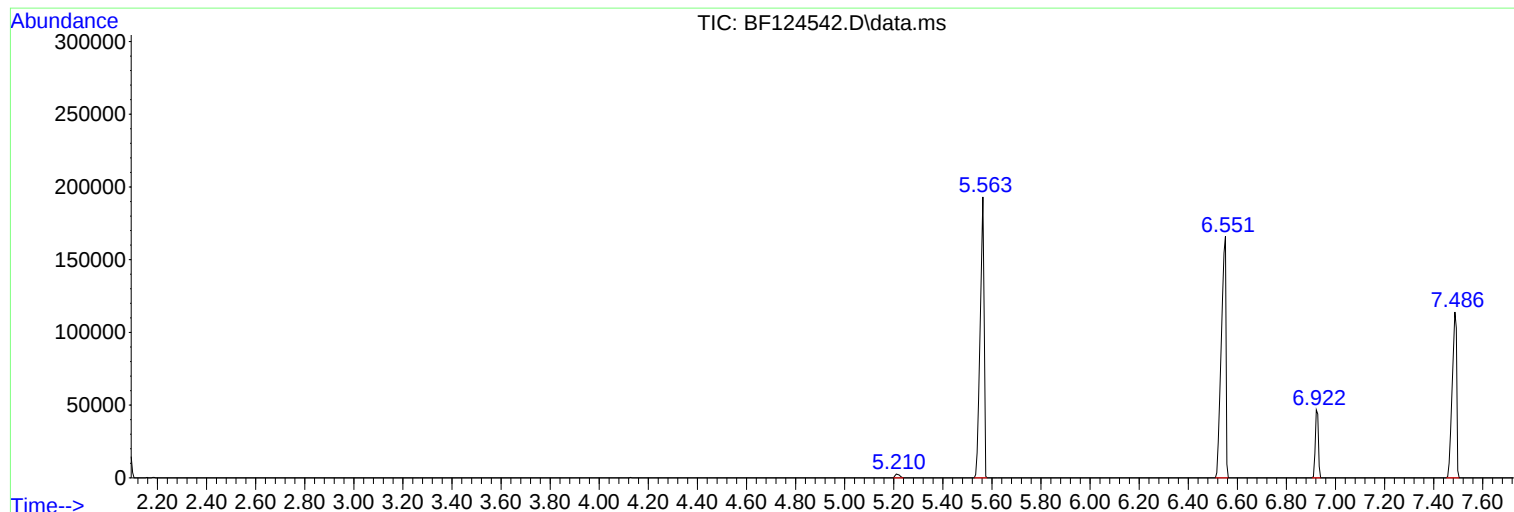

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
Data File : BF124542.D
Acq On : 7 Jul 2021 22:58
Operator : JU/CG
Sample : PB137511BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137511BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
Data File : BF124542.D
Acq On : 7 Jul 2021 22:58
Operator : JU/CG
Sample : PB137511BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137511BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------