
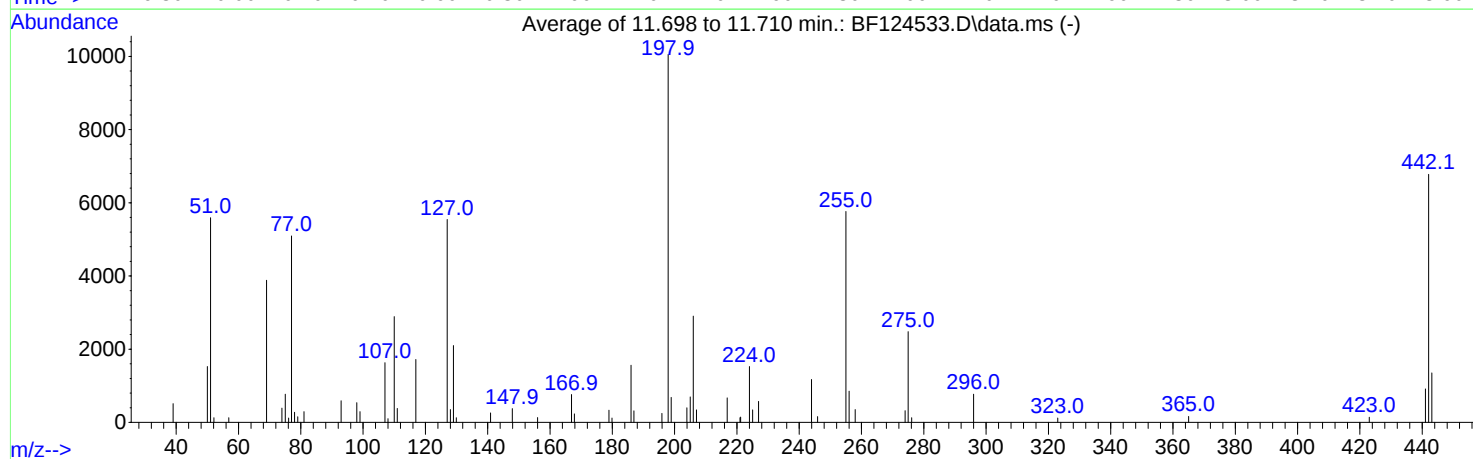


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
 Data File : BF124533.D
 Acq On : 7 Jul 2021 16:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 08 07:49:42 2021

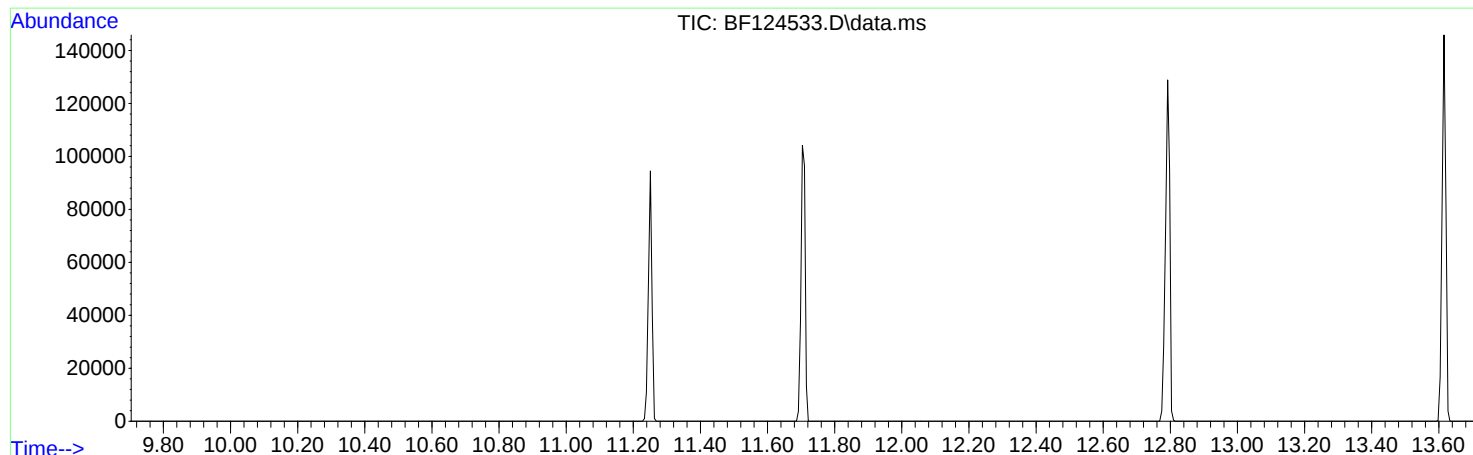




AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.6	5590	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	3883	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.2	5546	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10051	PASS
199	198	5	9	6.8	683	PASS
275	198	10	60	24.7	2480	PASS
365	198	1	100	1.6	162	PASS
441	198	0.01	100	9.1	914	PASS
442	442	50	100	100.0	6777	PASS
443	442	15	24	19.9	1350	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
Data File : BF124533.D
Acq On : 7 Jul 2021 16:57
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 08 05:34:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 05:15:31 2021
Response via : Initial Calibration

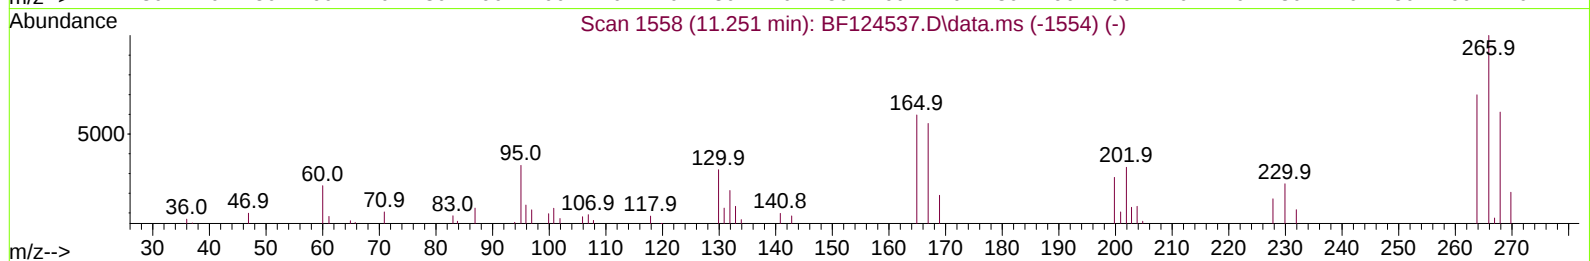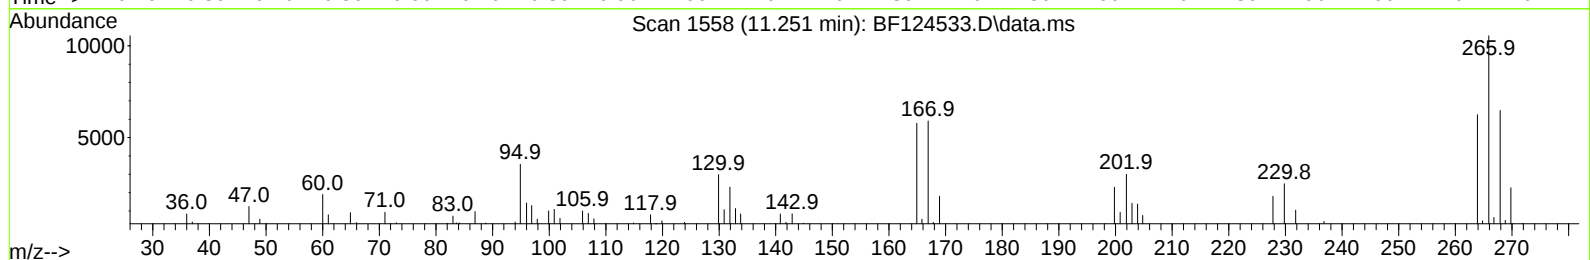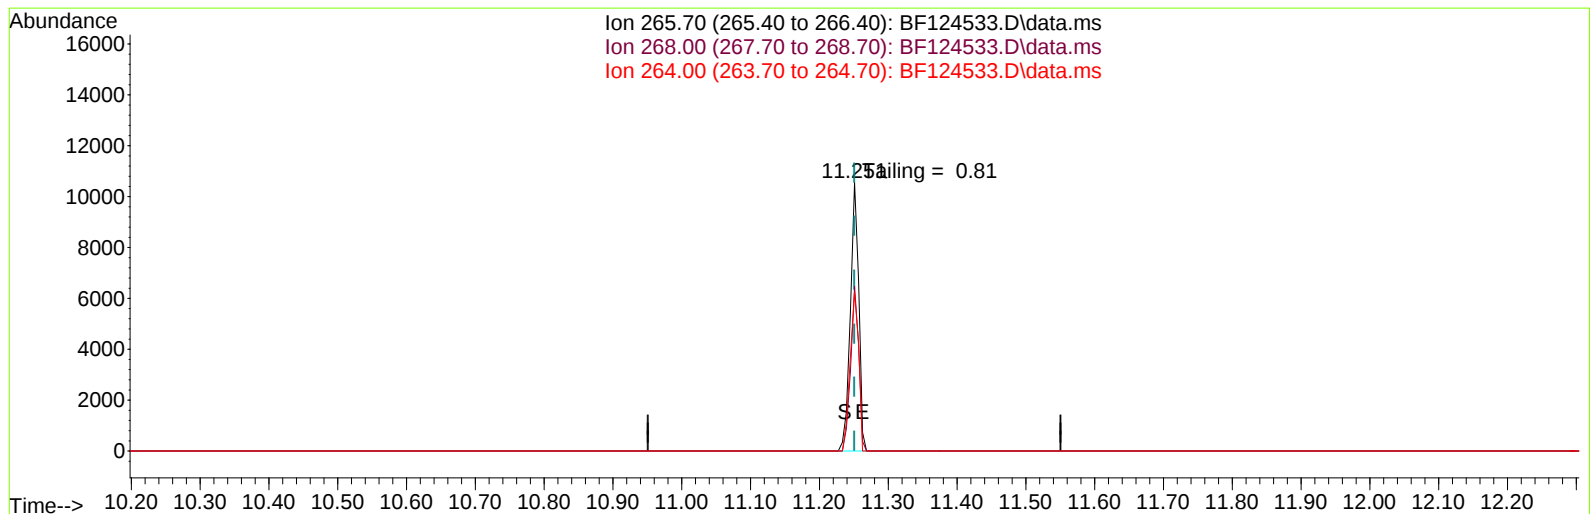

TIC: BF124533.D\data.ms

(70) Pentachlorophenol (C)

11.251min (+ 0.000) 0.00 ng




response 8938

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.36
264.00	69.90	59.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070721\
 Data File : BF124533.D
 Acq On : 7 Jul 2021 16:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 08 05:34:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 05:15:31 2021
 Response via : Initial Calibration

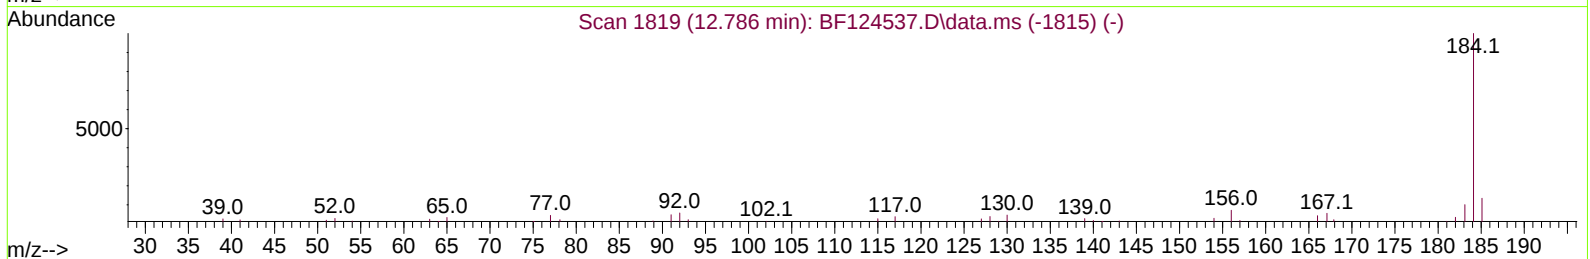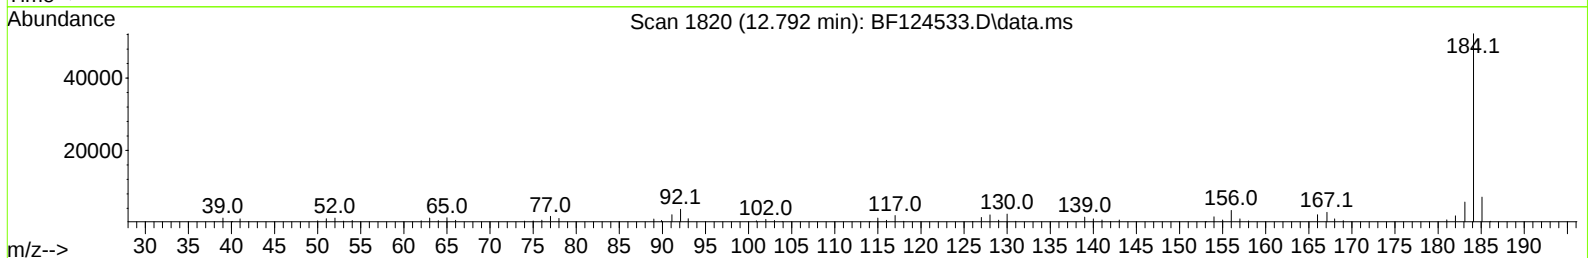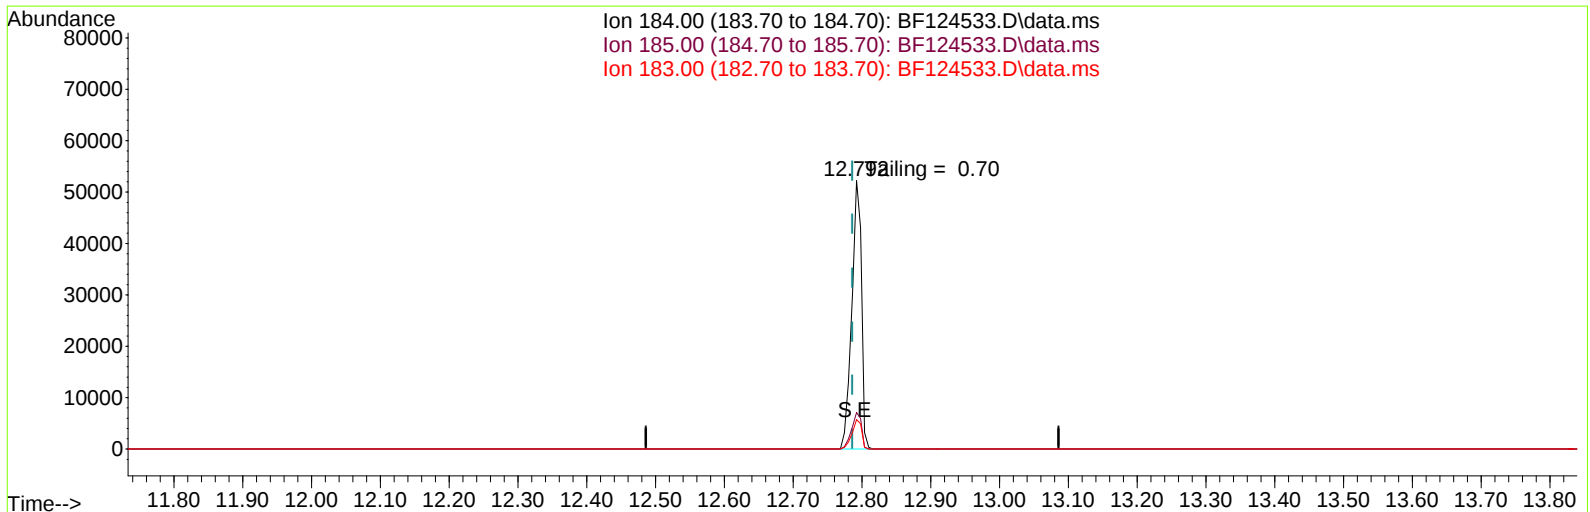

TIC: BF124533.D\data.ms

(77) Benzidine

12.792min (+ 0.006) 0.00 ng

response 51277

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.59
183.00	10.10	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/7/2021	BNA_F	<u>BF124533.D</u>
Compound Name	Response	Retention Time
DDT	22190	13.527
DDD	0	0
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	22190	0.00