
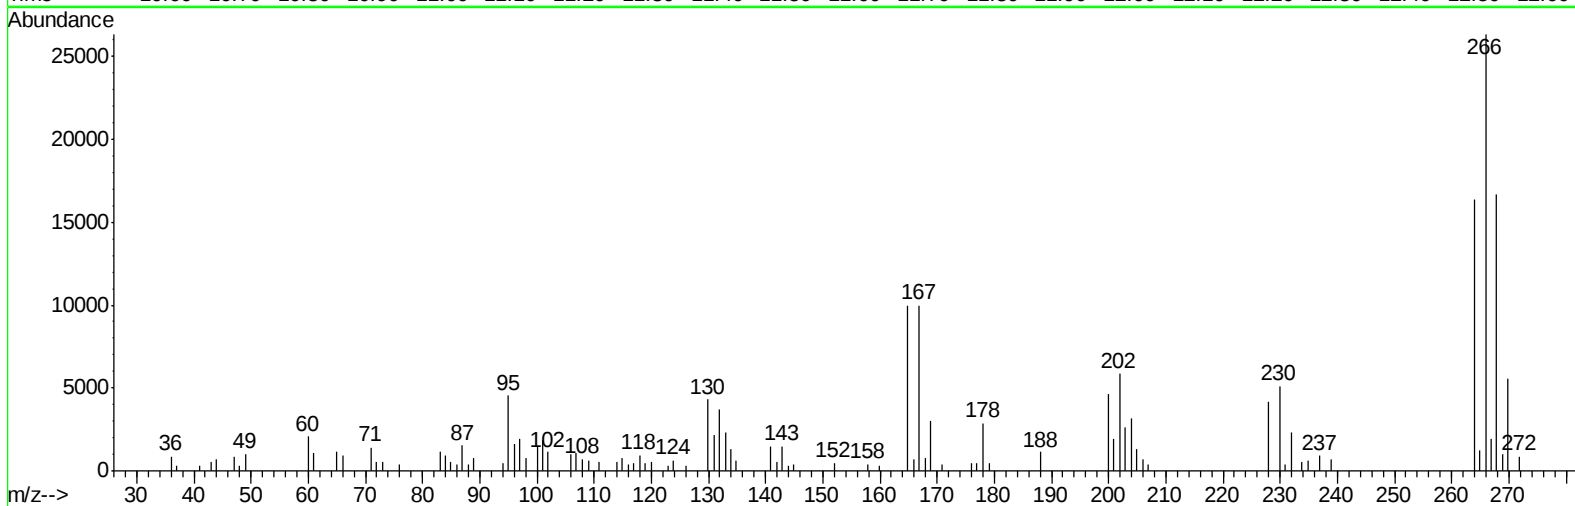


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070815\
Data File : BF080384.D
Acq On : 8 Jul 2015 12:41
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 03:58:26 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 09 01:25:24 2015
Response via : Initial Calibration

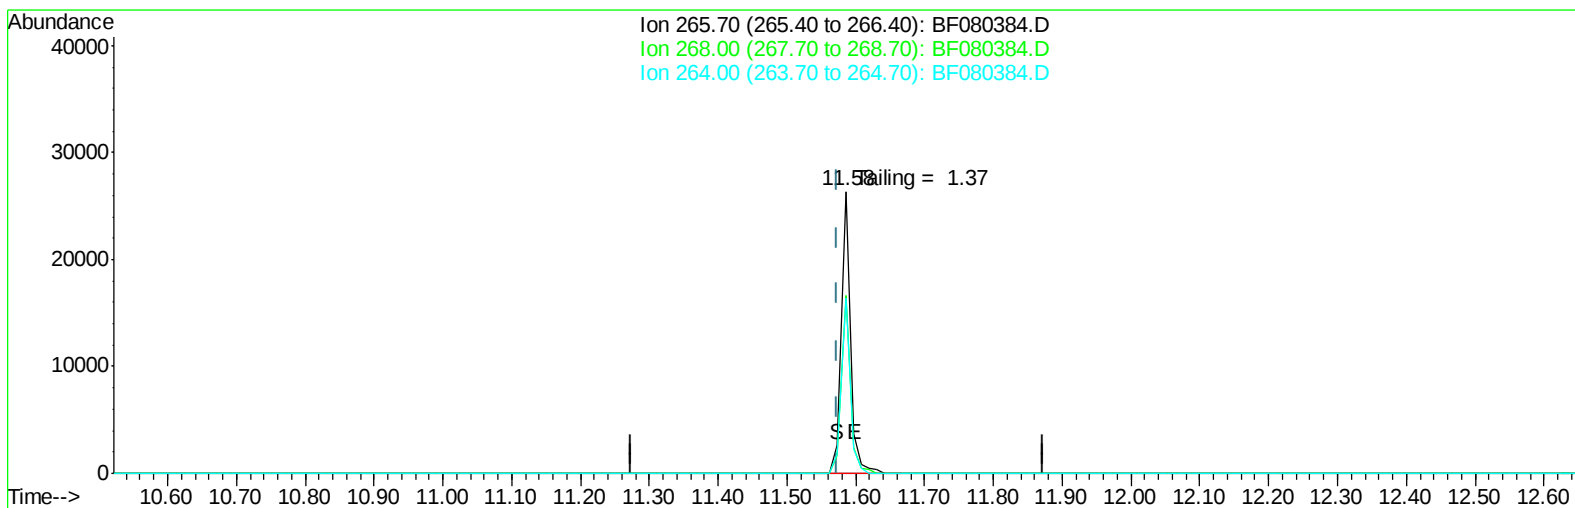

TIC: BF080384.D

(69) Pentachlorophenol (C)



11.585min (+0.011) 591.11ng

response 23519

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	63.24
264.00	68.80	62.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070815\
Data File : BF080384.D
Acq On : 8 Jul 2015 12:41
Operator : TP/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 03:58:26 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 09 01:25:24 2015
Response via : Initial Calibration

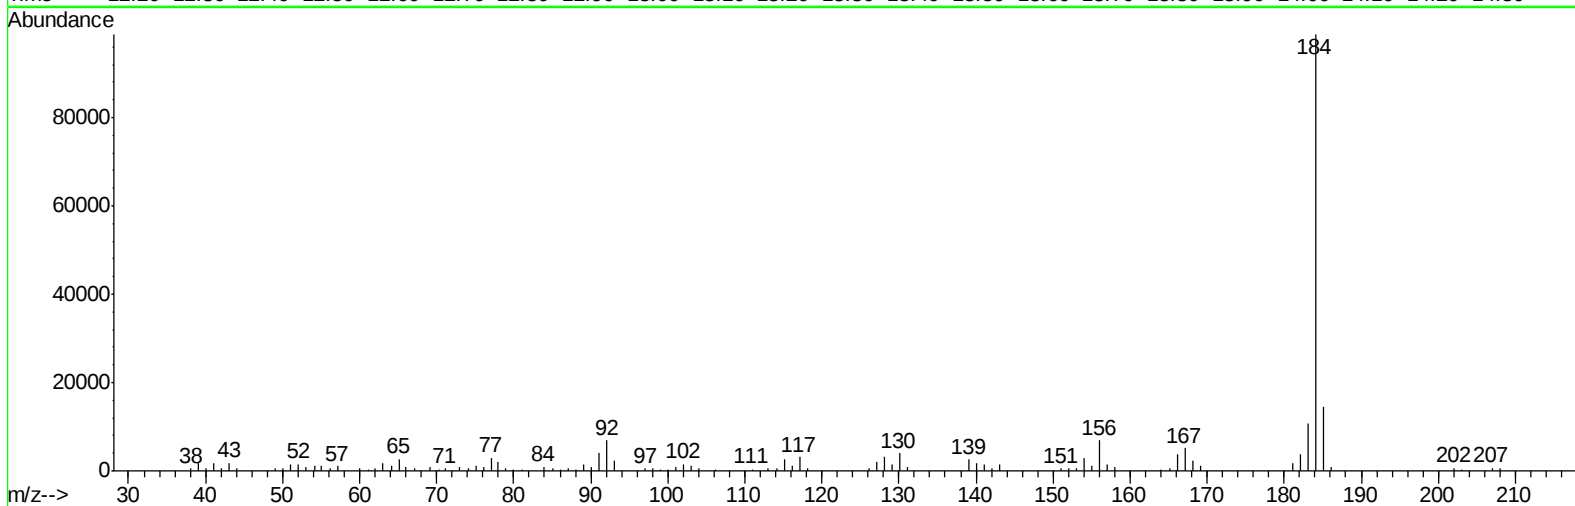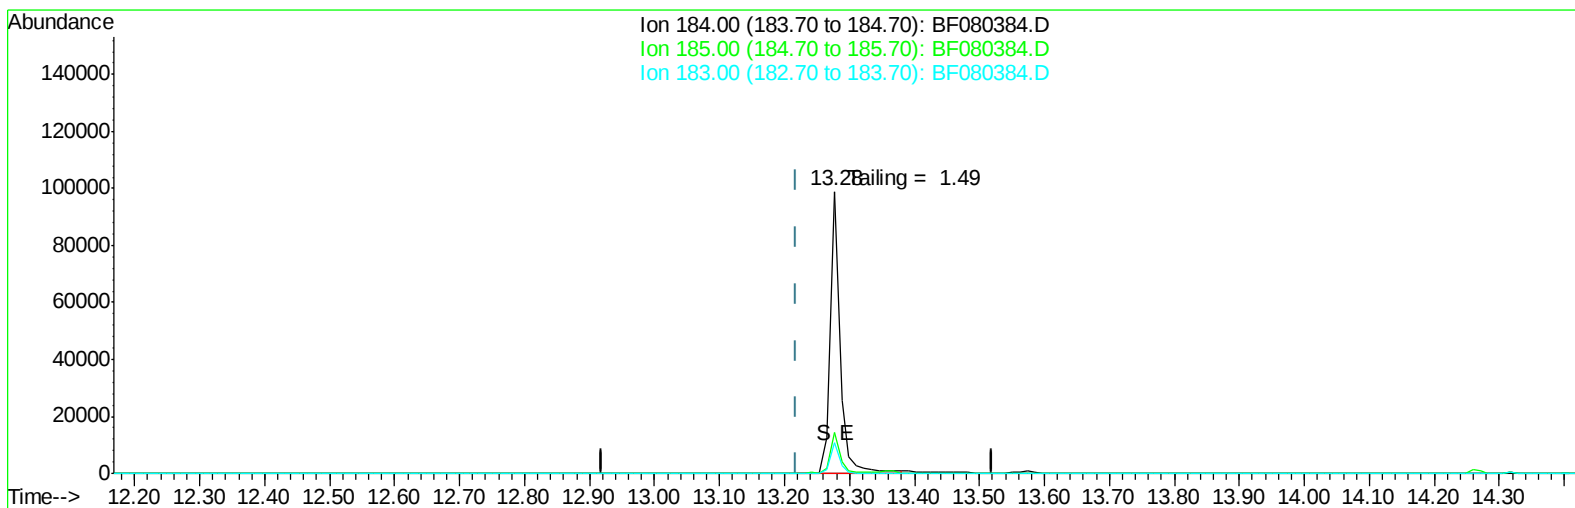

TIC: BF080384.D

(76) Benzidine

13.276min (+0.057) 101.64ng

response 105920

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.67
183.00	11.50	10.99
0.00	0.00	0.00