

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
 Data File : BF088821.D
 Acq On : 8 Jul 2016 13:04
 Operator : UM/SJ
 Sample : PB91866BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB91866BL

Quant Time: Jul 08 18:54:41 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 05 17:15:08 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	75769	20.00	ng	-0.05
21) Naphthalene-d8	8.01	136	277422	20.00	ng	-0.06
38) Acenaphthene-d10	9.76	164	138408	20.00	ng	-0.06
63) Phenanthrene-d10	11.23	188	266012	20.00	ng	-0.06
75) Chrysene-d12	13.86	240	241968	20.00	ng	-0.06
86) Perylene-d12	15.23	264	195623	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.34	112	595670	117.82	ng	-0.03
7) Phenol-d6	6.38	99	811808	124.27	ng	-0.03
23) Nitrobenzene-d5	7.29	82	420117	79.36	ng	-0.06
41) 2,4,6-Tribromophenol	10.55	330	173008	134.61	ng	-0.06
44) 2-Fluorobiphenyl	9.10	172	882510	100.72	ng	-0.05
78) Terphenyl-d14	12.82	244	810841	74.64	ng	-0.05
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.29	70	55457	12.64	ng	# 74
25) Isophorone	7.29	82	348356	35.52	ng	# 65
50) 2,6-Dinitrotoluene	9.76	165	17932	8.21	ng	# 39
56) 2,4-Dinitrotoluene	9.76	165	17929	6.27	ng	# 37
66) 4-Bromophenyl-phenylether	10.55	248	11798	4.40	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088821.D
Acq On : 8 Jul 2016 13:04
Operator : UM/SJ
Sample : PB91866BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91866BL

Quant Time: Jul 08 18:54:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

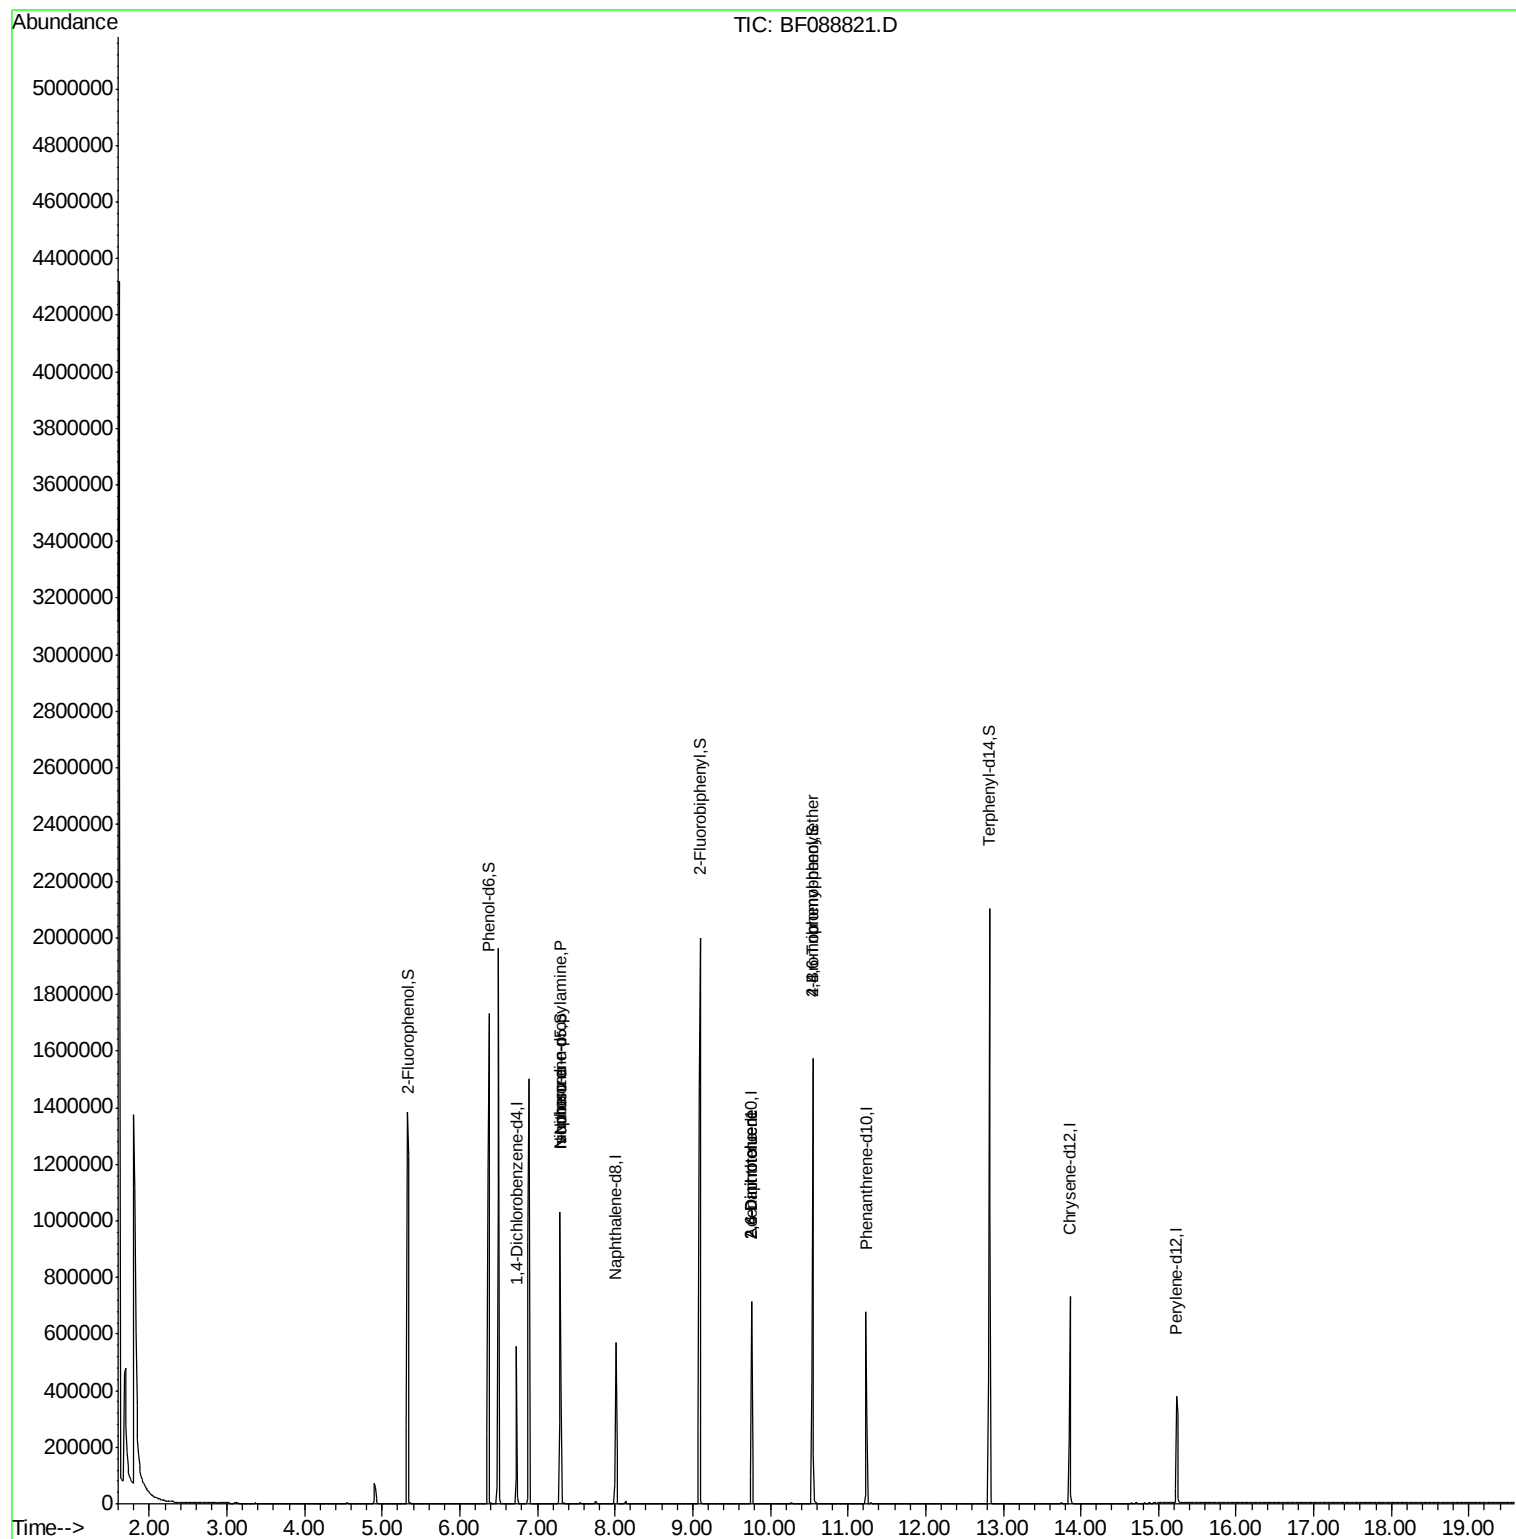



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.73 min Scan# 450

Delta R.T. -0.05 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Instrument :

BNA_F

ClientSampleId :

PB91866BL


Tgt Ion:152 Resp: 75769

Ion Ratio Lower Upper

152 100

150 157.5 123.8 185.6




115 64.9 39.6 59.4#

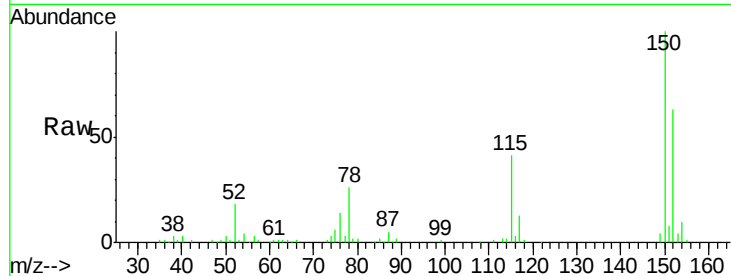

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

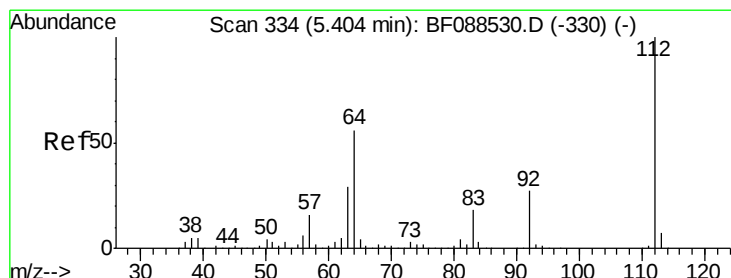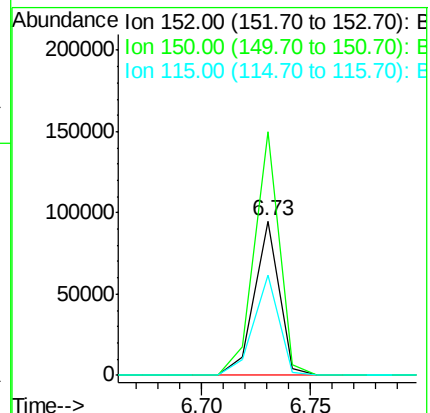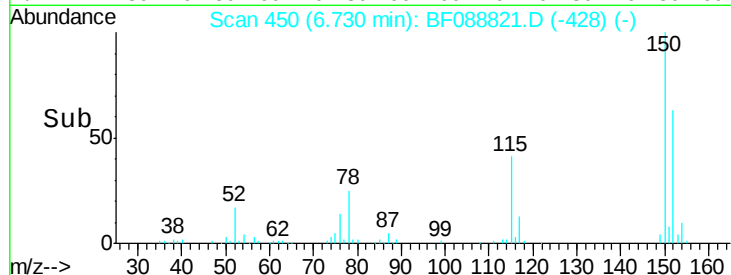

#5

2-Fluorophenol

Concen: 117.82 ng

RT: 5.34 min Scan# 328

Delta R.T. -0.03 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04


Tgt Ion:112 Resp: 595670

Ion Ratio Lower Upper

112 100

64 45.2 42.2 63.2



63 23.7 21.8 32.8

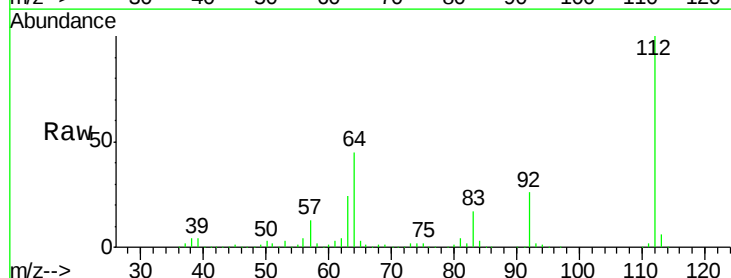

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

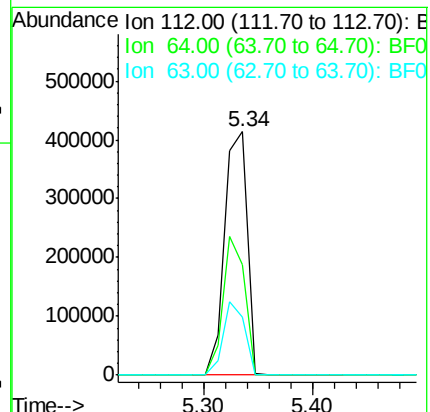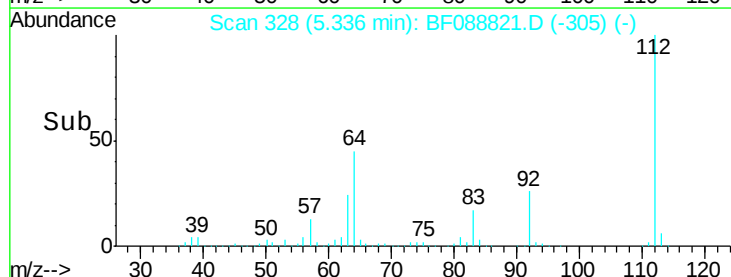



#7

Phenol-d6

Concen: 124.27 ng

RT: 6.38 min Scan# 419

Delta R.T. -0.03 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Instrument :

BNA_F

ClientSampleId :

PB91866BL




Tgt Ion: 99 Resp: 811808

Ion Ratio Lower Upper

99 100

42 14.7 12.2 18.2

71 35.0 23.4 35.0

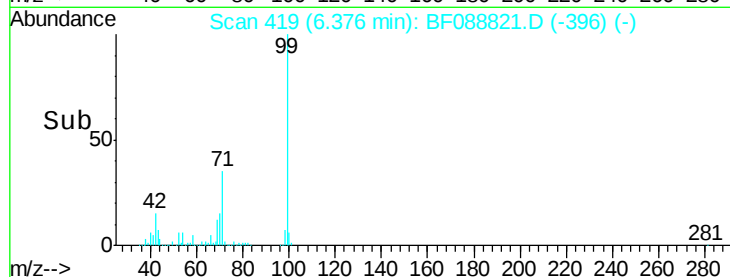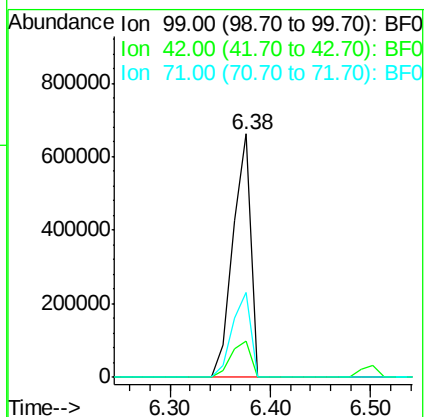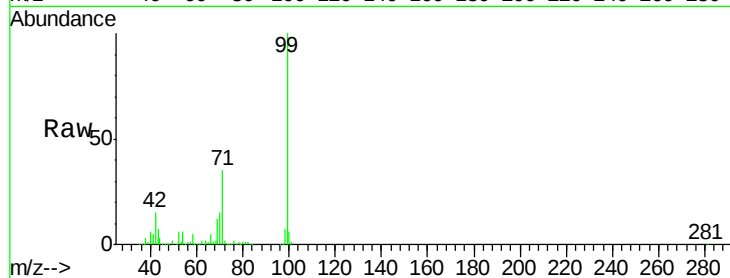

#19

n-Nitroso-di-n-propylamine

Concen: 12.64 ng

RT: 7.29 min Scan# 499

Delta R.T. 0.09 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Tgt Ion: 70 Resp: 55457




Ion Ratio Lower Upper

70 100

42 44.6 49.6 74.4#

101 0.0 7.1 10.7#

130 2.0 15.4 23.2#

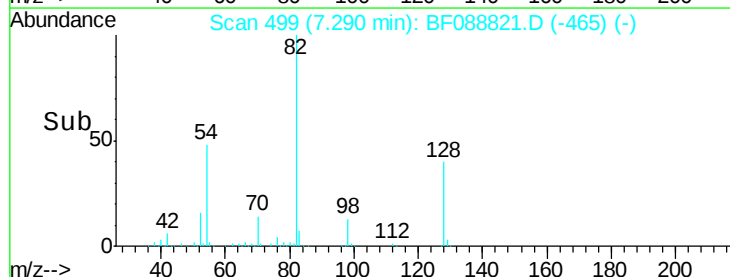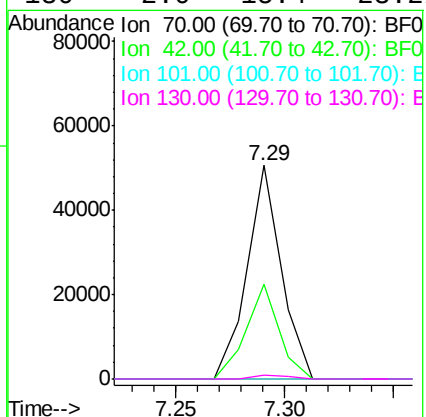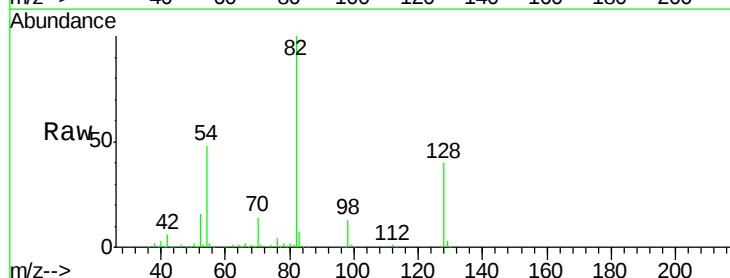



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.01 min Scan# 562

Delta R.T. -0.06 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Instrument :

BNA_F

ClientSampleId :

PB91866BL

Tgt Ion: 136 Resp: 277422



Ion Ratio Lower Upper

136 100

137 10.8 9.1 13.7

54 8.5 6.6 10.0

68 6.9 5.1 7.7

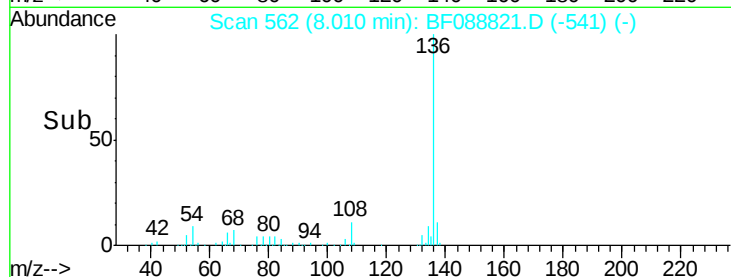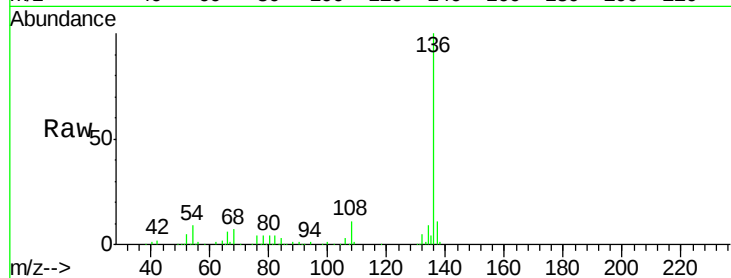


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

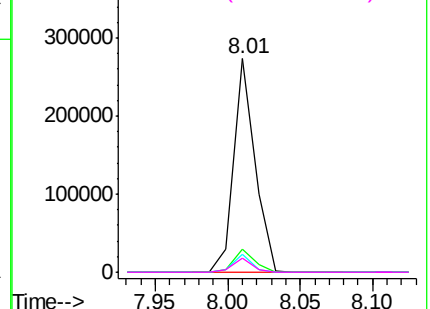

#23

Nitrobenzene-d5

Concen: 79.36 ng

RT: 7.29 min Scan# 499

Delta R.T. -0.06 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04



Tgt Ion: 82 Resp: 420117

Ion Ratio Lower Upper

82 100

128 40.4 35.9 53.9


54 48.4 40.9 61.3

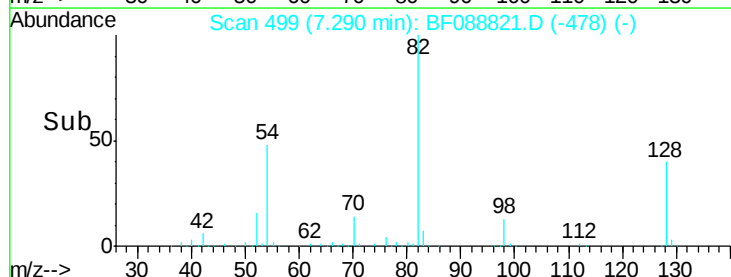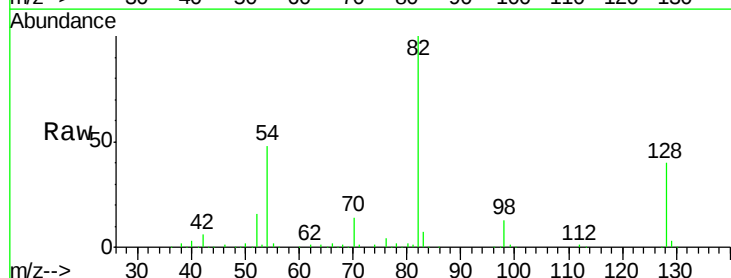


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

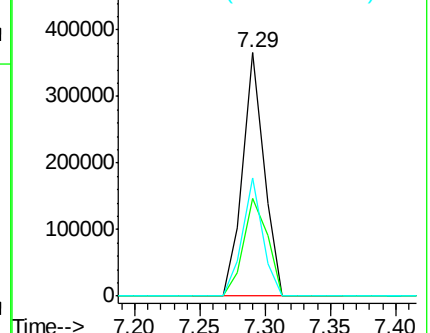

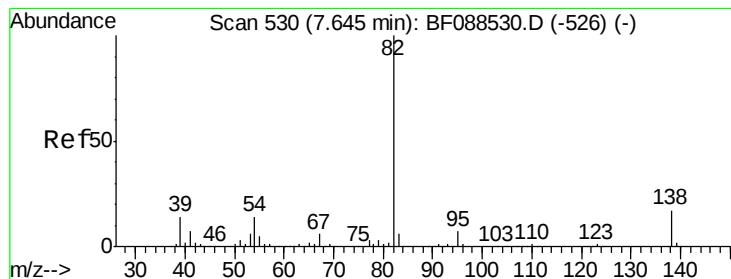

#25

Isophorone

Concen: 35.52 ng

RT: 7.29 min Scan# 499

Delta R.T. -0.32 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Instrument :

BNA_F

ClientSampleId :

PB91866BL





Tgt Ion: 82 Resp: 348356

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#

138 0.0 14.6 21.8#

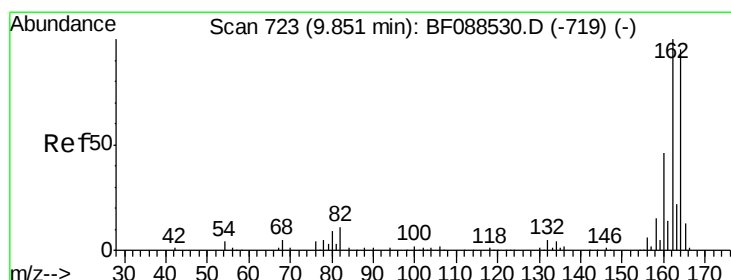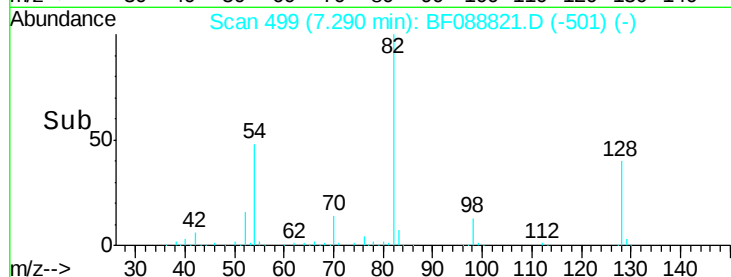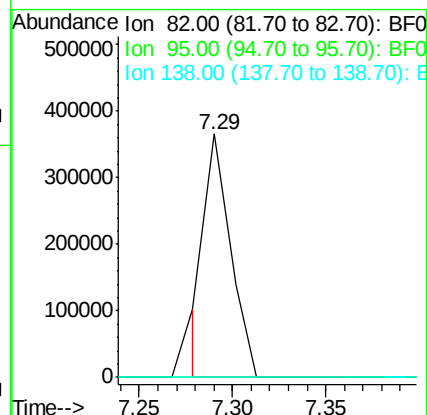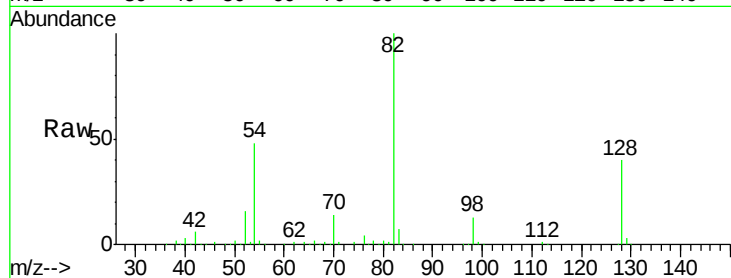

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.76 min Scan# 715

Delta R.T. -0.06 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04




Tgt Ion: 164 Resp: 138408


Ion Ratio Lower Upper

164 100

162 104.5 85.4 128.2

160 46.9 39.5 59.3


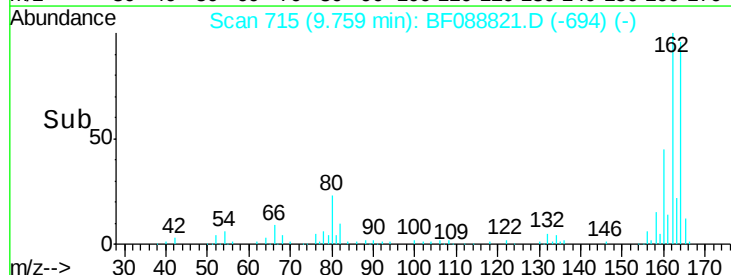
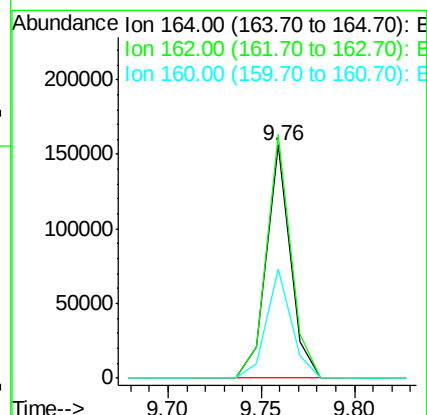
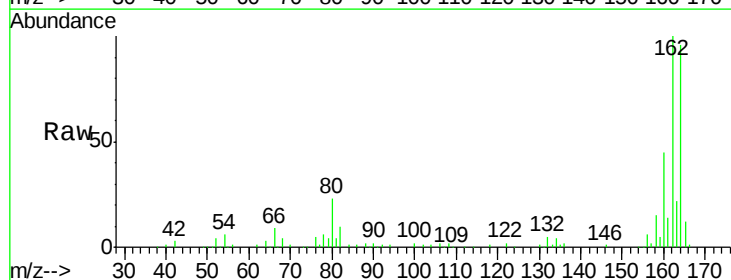


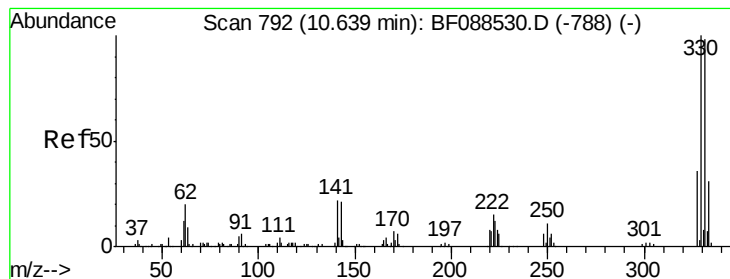

#41
 2,4,6-Tribromophenol
 Concen: 134.61 ng
 RT: 10.55 min Scan# 784
 Delta R.T. -0.06 min
 Lab File: BF088821.D
 Acq: 8 Jul 2016 13:04




Instrument :
 BNA_F
 ClientSampleId :
 PB91866BL


Tgt Ion:330 Resp: 173008
 Ion Ratio Lower Upper
 330 100
 332 96.1 0.0 0.0#
 141 43.1 0.0 0.0#

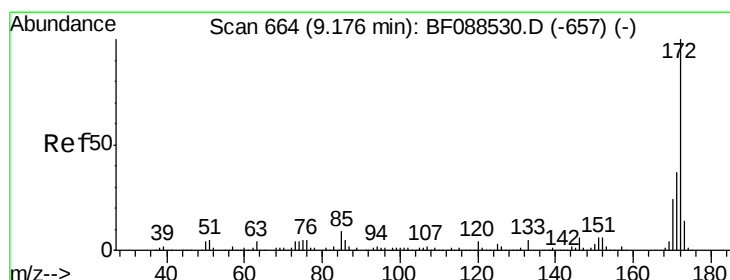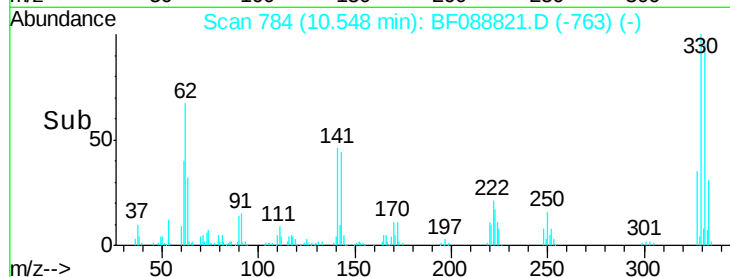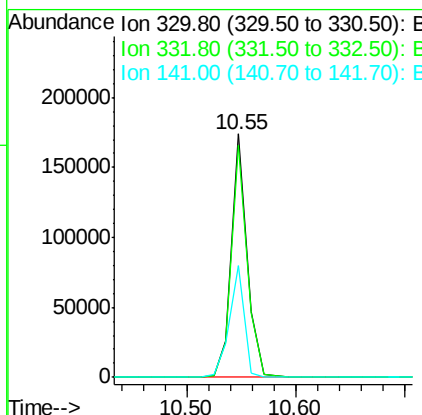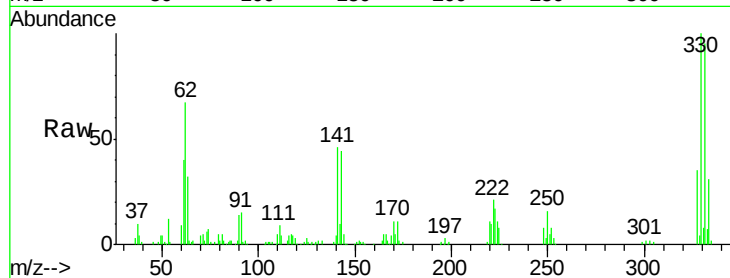

#44
 2-Fluorobiphenyl
 Concen: 100.72 ng
 RT: 9.10 min Scan# 657
 Delta R.T. -0.05 min
 Lab File: BF088821.D
 Acq: 8 Jul 2016 13:04

Tgt Ion:172 Resp: 882510
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.6 43.0
 170 23.6 19.2 28.8

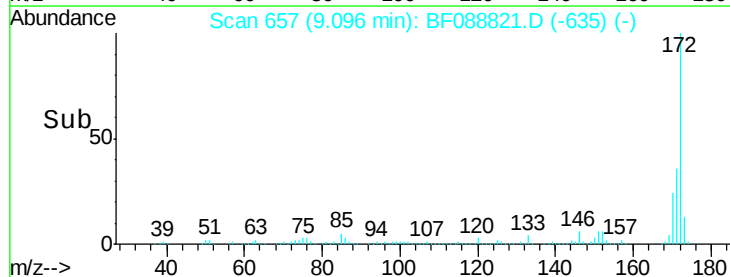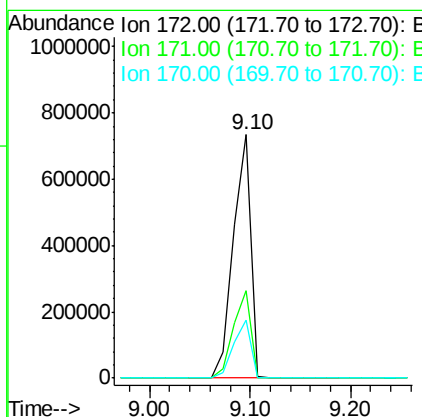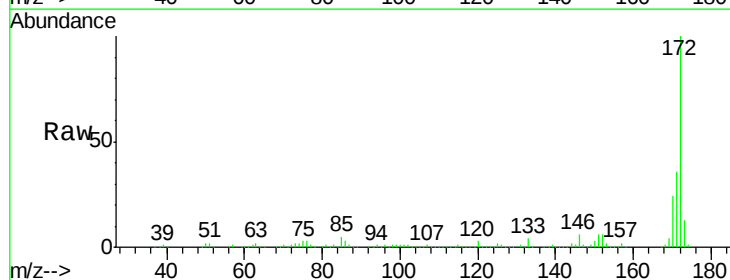

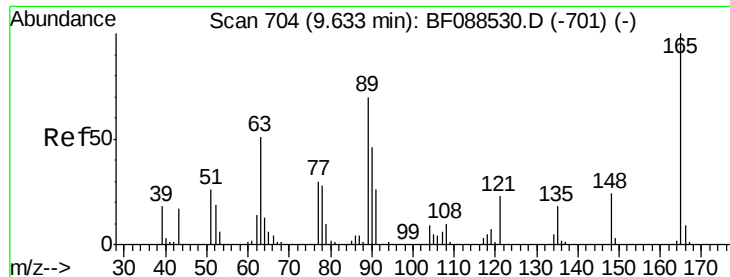

#50

2,6-Dinitrotoluene

Concen: 8.21 ng

RT: 9.76 min Scan# 715

Delta R.T. 0.16 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Instrument :

BNA_F

ClientSampleId :

PB91866BL


Tgt Ion:165 Resp: 17932

Ion Ratio Lower Upper

165 100

63 0.0 28.1 42.1#




89 1.8 32.2 48.2#

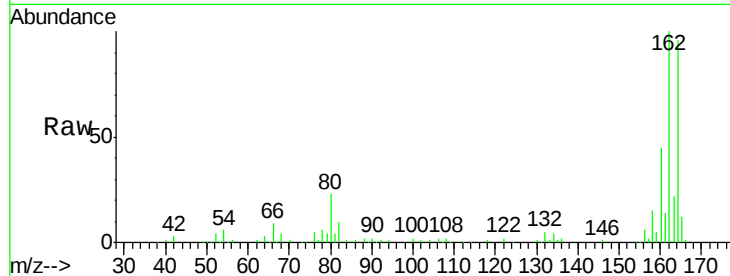

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

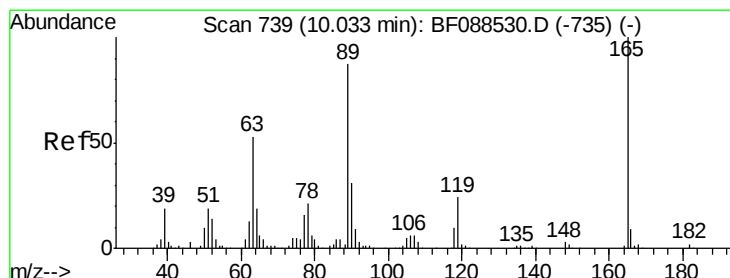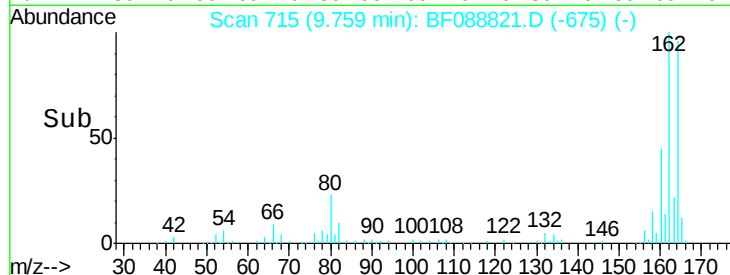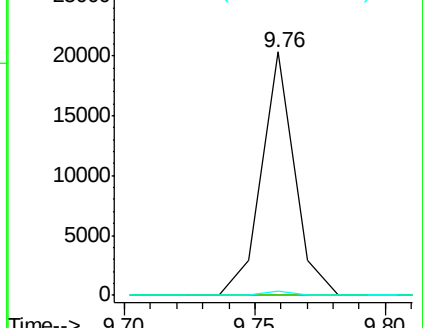

#56

2,4-Dinitrotoluene

Concen: 6.27 ng

RT: 9.76 min Scan# 715

Delta R.T. -0.24 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Tgt Ion:165 Resp: 17929


Ion Ratio Lower Upper

165 100

63 0.0 22.0 33.0#

89 1.8 41.1 61.7#

182 0.0 2.0 3.0#


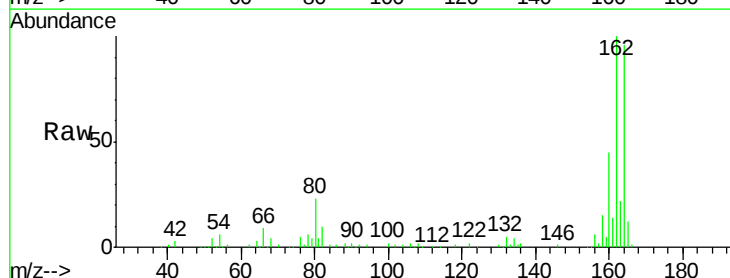


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E



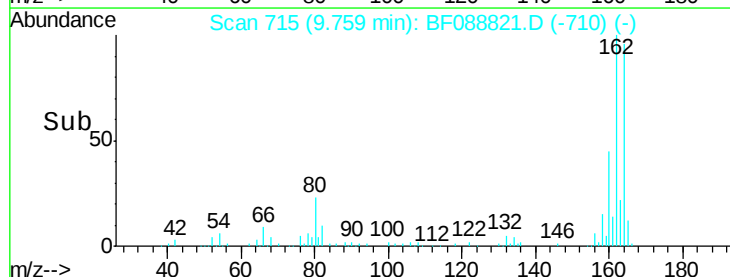
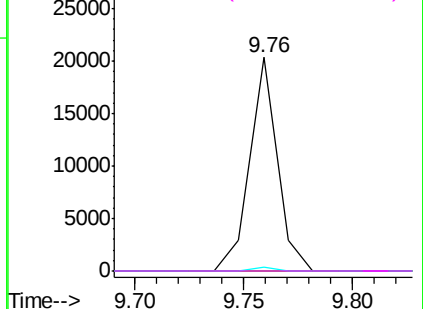




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.23 min Scan# 844
 Delta R.T. -0.06 min
 Lab File: BF088821.D
 Acq: 8 Jul 2016 13:04




Instrument :
 BNA_F
 ClientSampleId :
 PB91866BL


Tgt Ion:188 Resp: 266012
 Ion Ratio Lower Upper
 188 100
 94 12.9 9.0 13.6
 80 15.0 10.0 15.0#

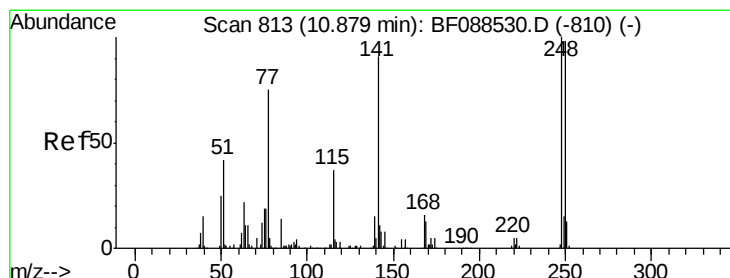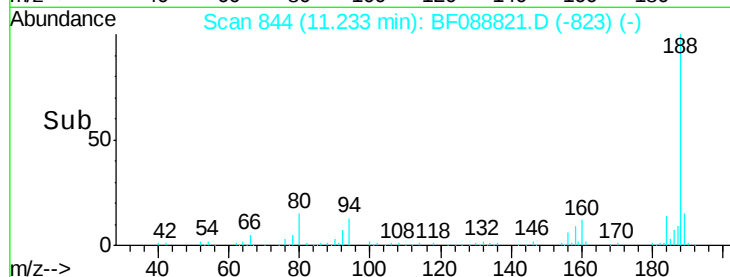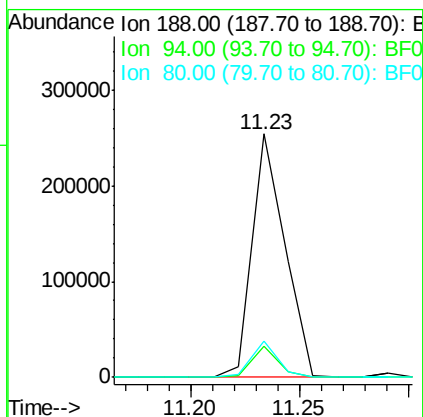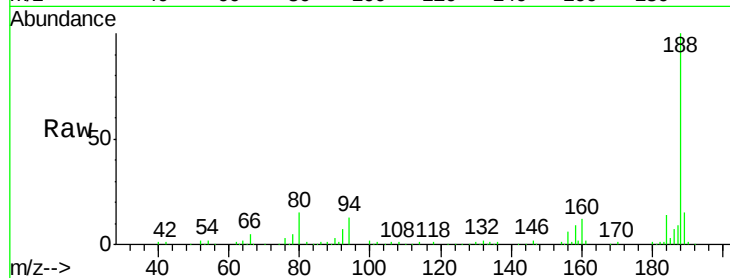

#66
 4-Bromophenyl-phenylether
 Concen: 4.40 ng
 RT: 10.55 min Scan# 784
 Delta R.T. -0.30 min
 Lab File: BF088821.D
 Acq: 8 Jul 2016 13:04

Tgt Ion:248 Resp: 11798
 Ion Ratio Lower Upper
 248 100
 250 205.7 77.1 115.7#
 141 602.2 50.6 76.0#

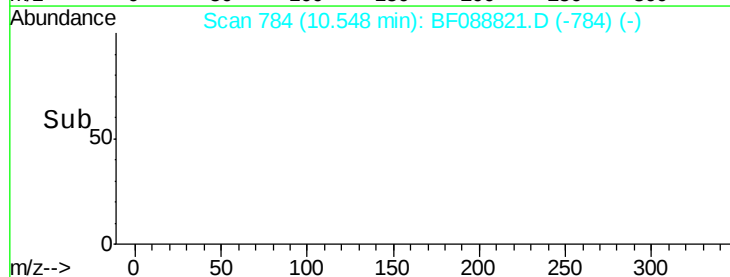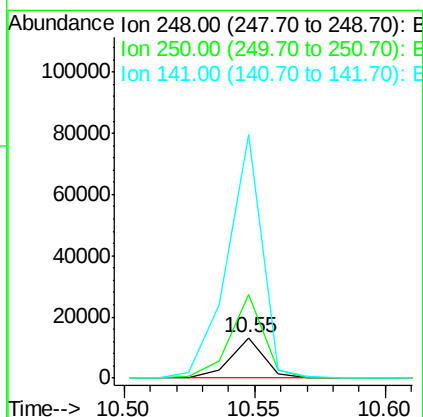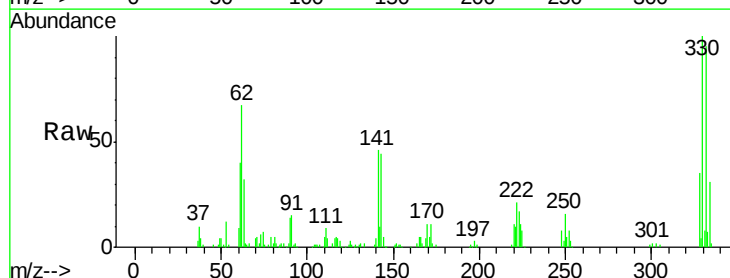

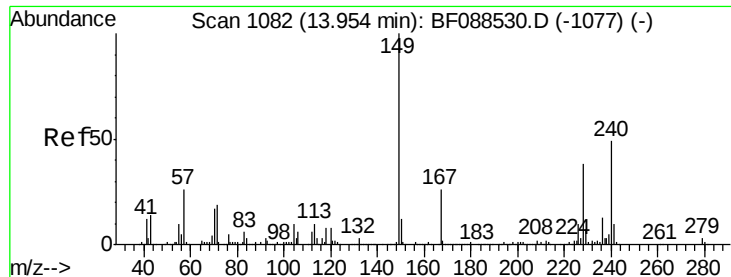

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.86 min Scan# 1074

Delta R.T. -0.06 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04

Instrument :

BNA_F

ClientSampleId :

PB91866BL


Tgt Ion:240 Resp: 241968

Ion Ratio Lower Upper

240 100

120 10.7 6.8 10.2#




236 25.7 20.2 30.2

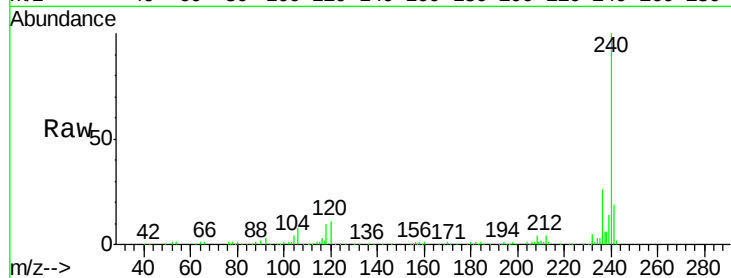

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

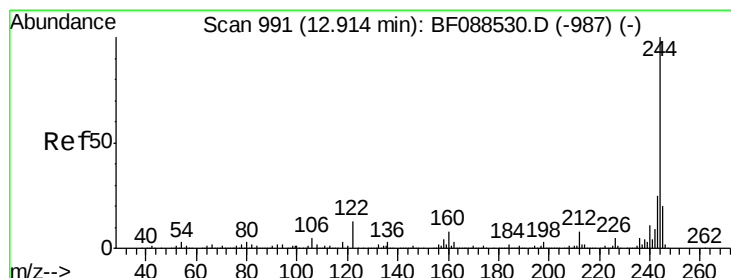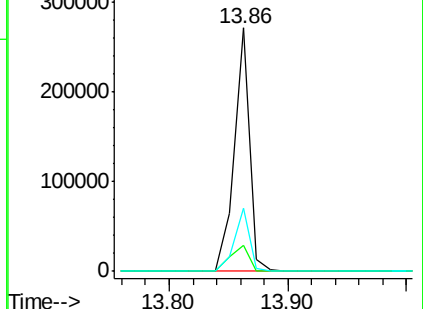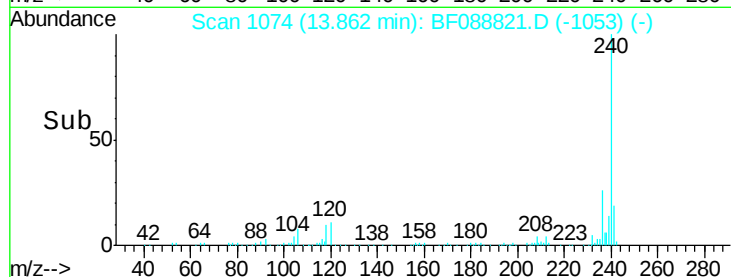

#78

Terphenyl-d14

Concen: 74.64 ng

RT: 12.82 min Scan# 983

Delta R.T. -0.05 min

Lab File: BF088821.D

Acq: 8 Jul 2016 13:04


Tgt Ion:244 Resp: 810841

Ion Ratio Lower Upper

244 100

212 8.1 6.0 9.0



122 15.3 11.2 16.8

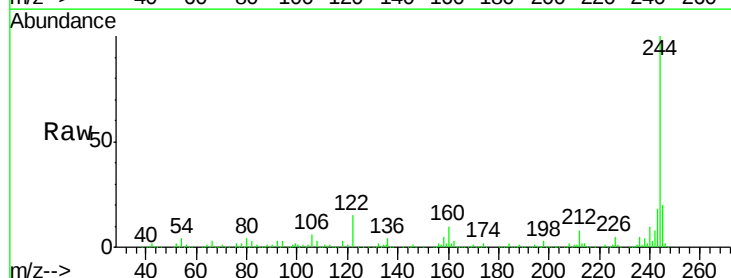


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

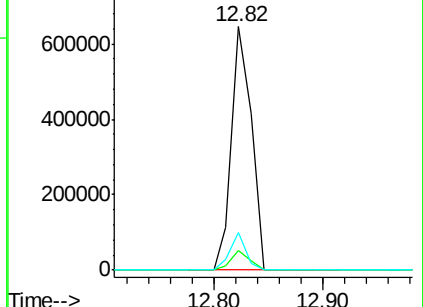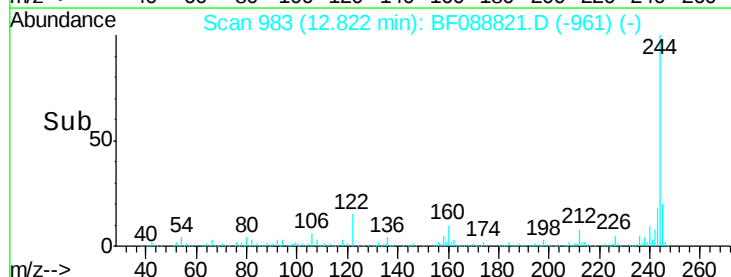


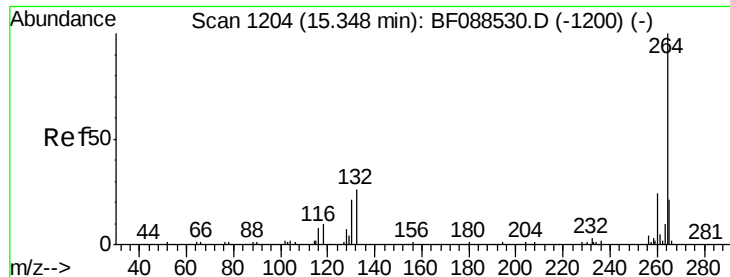

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.23 min Scan# 1194
Delta R.T. -0.07 min
Lab File: BF088821.D
Acq: 8 Jul 2016 13:04

Instrument :
BNA_F
ClientSampleId :
PB91866BL

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.2	28.8
265	21.0	16.9	25.3

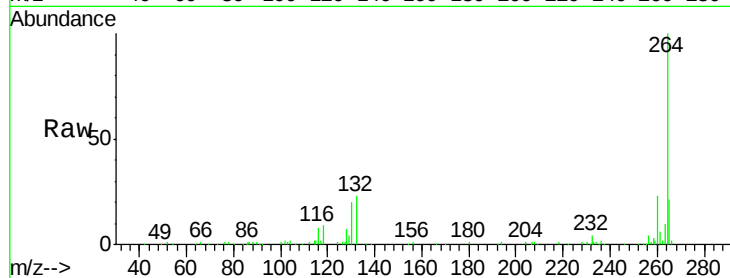

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

