

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070816\
 Data File : BF088832.D
 Acq On : 8 Jul 2016 18:57
 Operator : UM/SJ
 Sample : H3813-02 50X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 08 23:22:35 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 18:51:20 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	77984	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	300942	20.00	ng	-0.01
38) Acenaphthene-d10	9.76	164	145482	20.00	ng	-0.01
63) Phenanthrene-d10	11.23	188	273540	20.00	ng	-0.01
75) Chrysene-d12	13.86	240	186791	20.00	ng	-0.01
86) Perylene-d12	15.23	264	159767	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	703	0.14	ng	-0.01
7) Phenol-d6	6.35	99	951	0.14	ng	-0.02
23) Nitrobenzene-d5	7.29	82	678	0.12	ng	-0.01
41) 2,4,6-Tribromophenol	10.55	330	211	0.16	ng	-0.01
44) 2-Fluorobiphenyl	9.08	172	1421	0.15	ng	-0.01
78) Terphenyl-d14	12.81	244	1393	0.17	ng	-0.01
Target Compounds						
50) 2,6-Dinitrotoluene	9.76	165	18762	8.17	ng	# 40
56) 2,4-Dinitrotoluene	9.76	165	18762	6.25	ng	# 38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF070816\
Data File : BF088832.D
Acq On : 8 Jul 2016 18:57
Operator : UM/SJ
Sample : H3813-02 50X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 08 23:22:35 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 18:51:20 2016
Response via : Initial Calibration

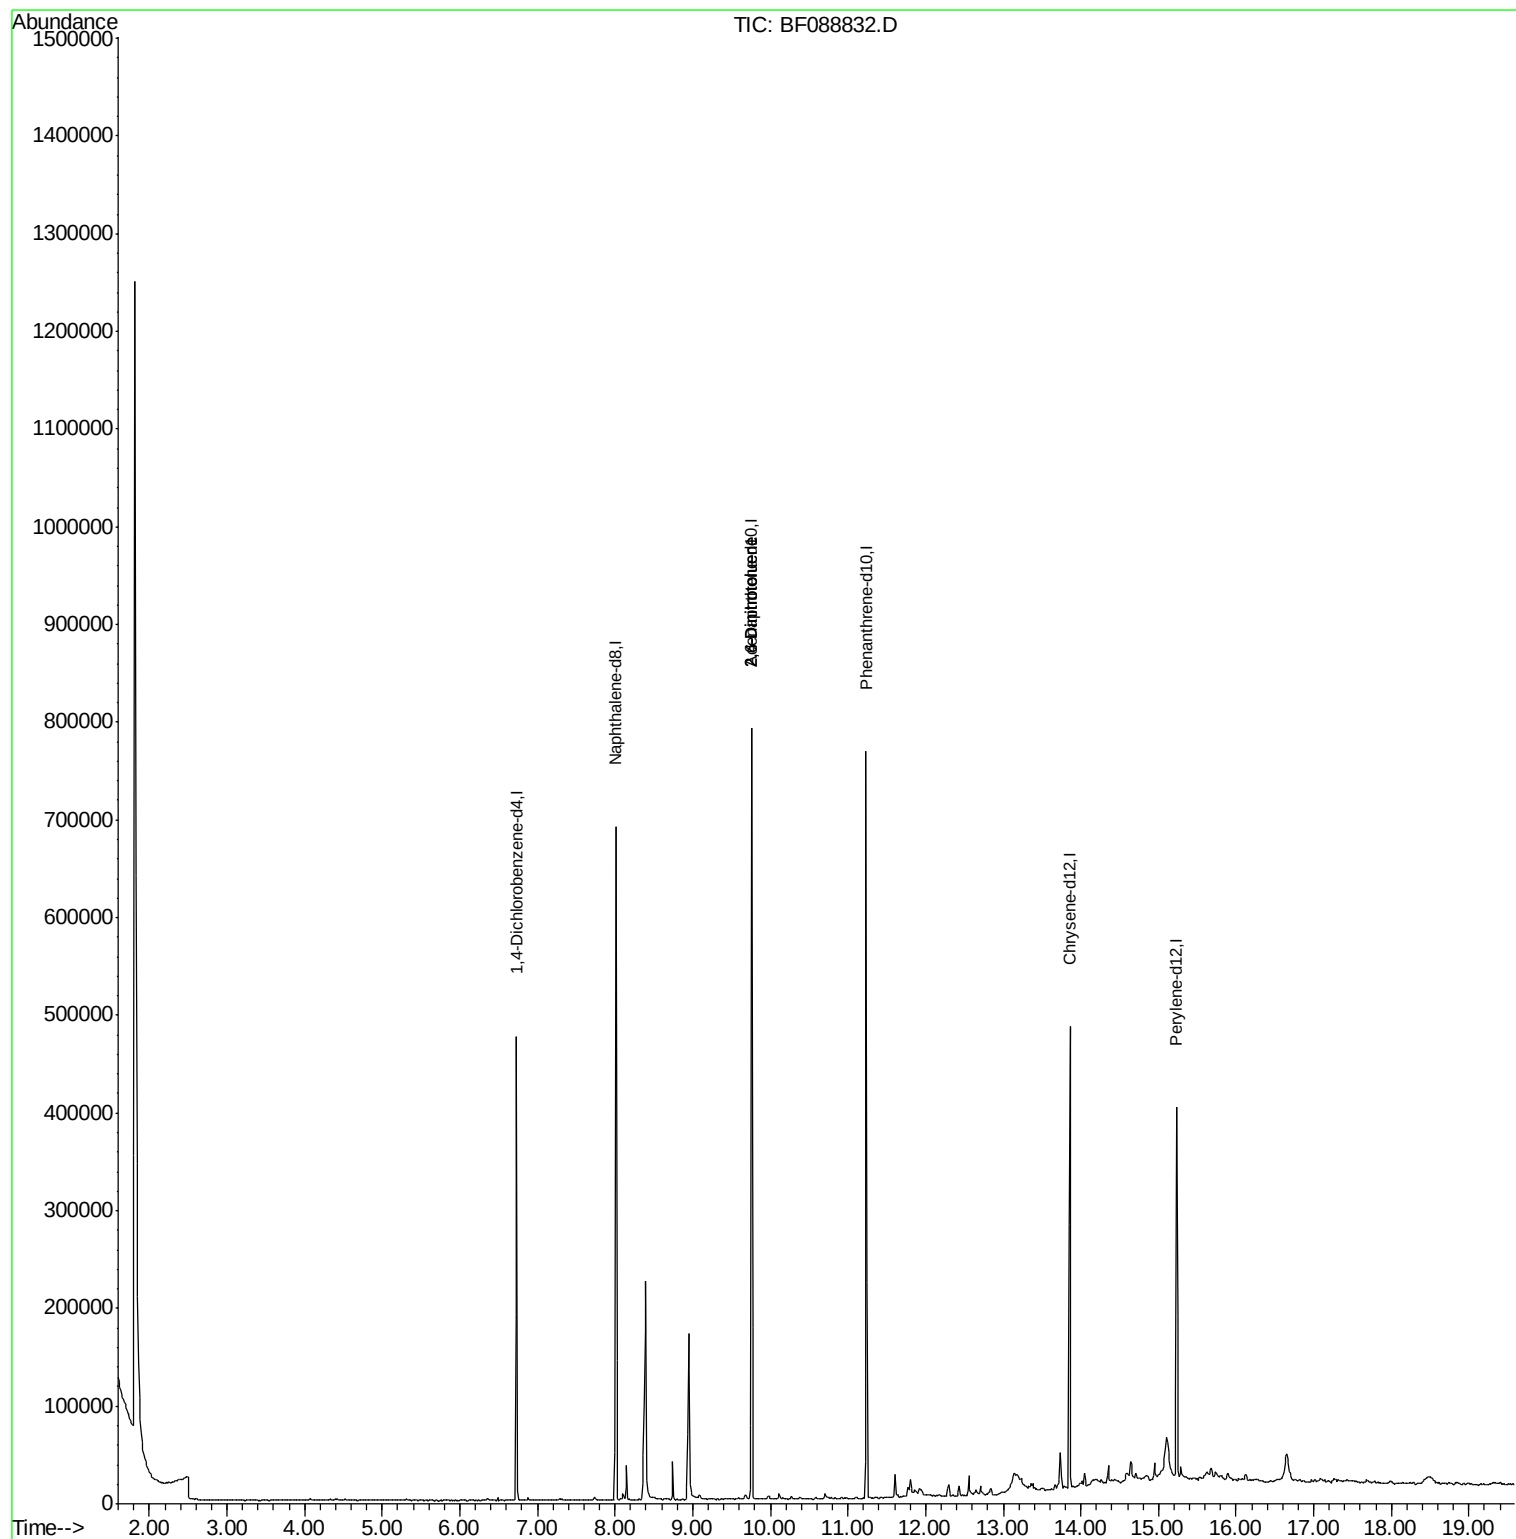

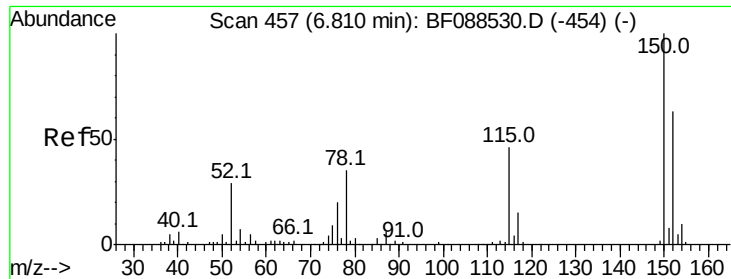


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.73 min Scan# 450
 Delta R.T. 0.00 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 77984
 Ion Ratio Lower Upper
 152 100
 150 152.5 123.8 185.6
 115 59.4 39.6 59.4#

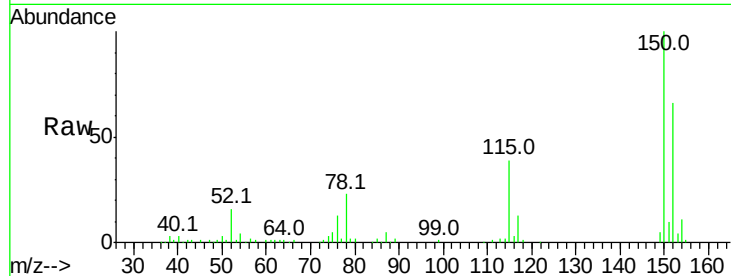


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

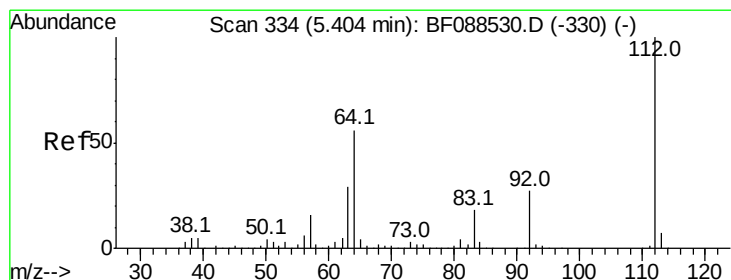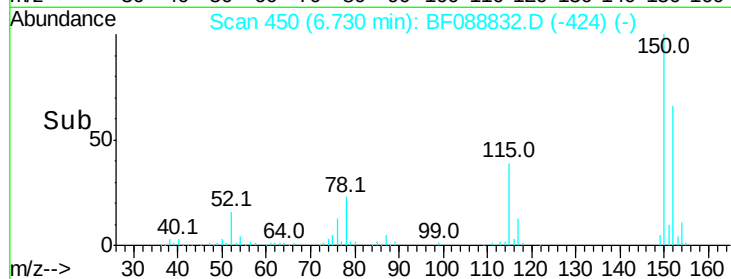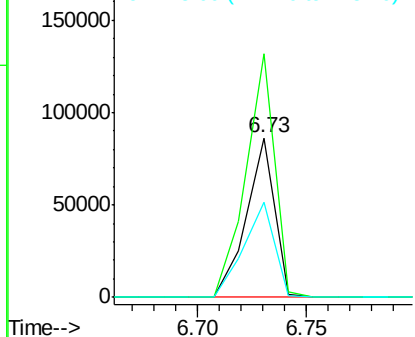



#5


2-Fluorophenol
 Concen: 0.14 ng
 RT: 5.31 min Scan# 326
 Delta R.T. -0.01 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57

Tgt Ion:112 Resp: 703
 Ion Ratio Lower Upper
 112 100
 64 59.3 42.2 63.2
 63 0.0 21.8 32.8#

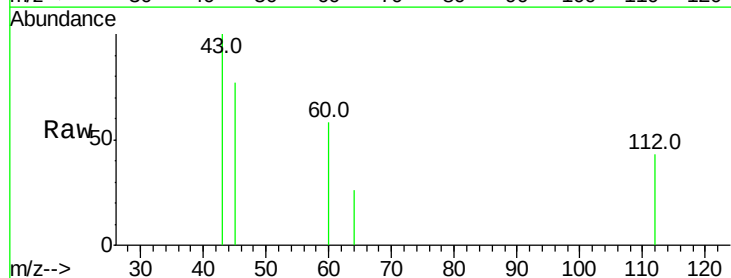

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

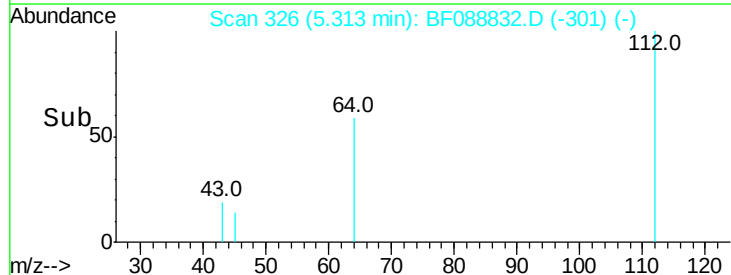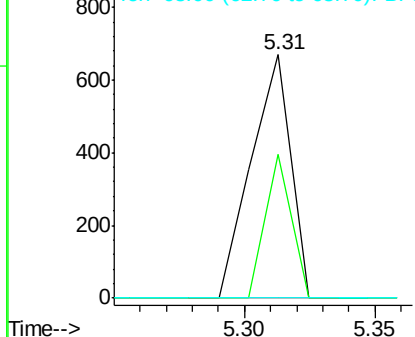

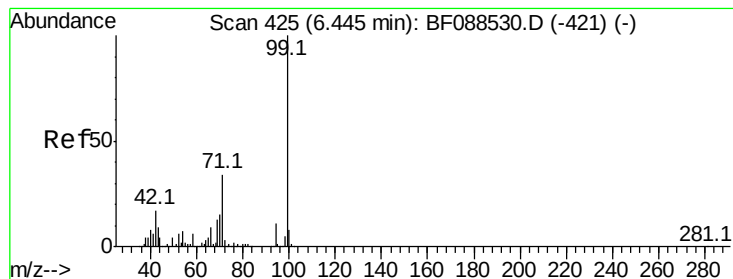

#7

Phenol-d6

Concen: 0.14 ng

RT: 6.35 min Scan# 417

Delta R.T. -0.02 min

Lab File: BF088832.D

Acq: 8 Jul 2016 18:57

Instrument :

BNA_F

ClientSampled :





Tot Ion: 99 Resp: 951

Ion Ratio Lower Upper

99 100

42 56.4 12.2 18.2#

71 41.9 23.4 35.0#

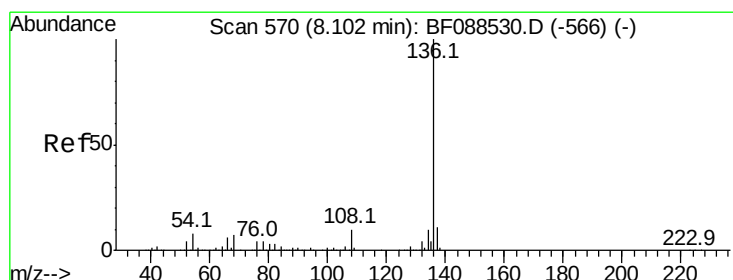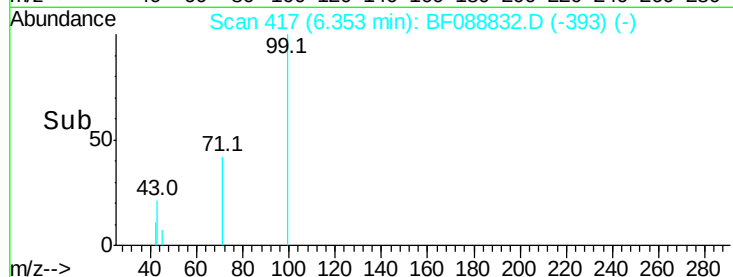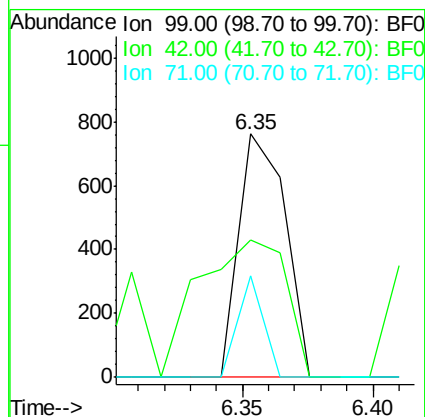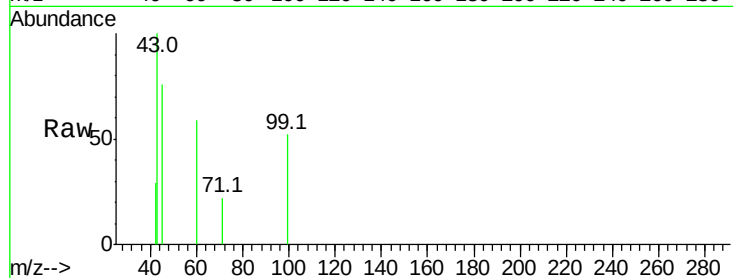

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.01 min Scan# 562

Delta R.T. -0.01 min

Lab File: BF088832.D

Acq: 8 Jul 2016 18:57

Tgt Ion: 136 Resp: 300942




Ion Ratio Lower Upper


136 100

137 11.2 9.1 13.7

54 8.3 6.6 10.0

68 6.6 5.1 7.7


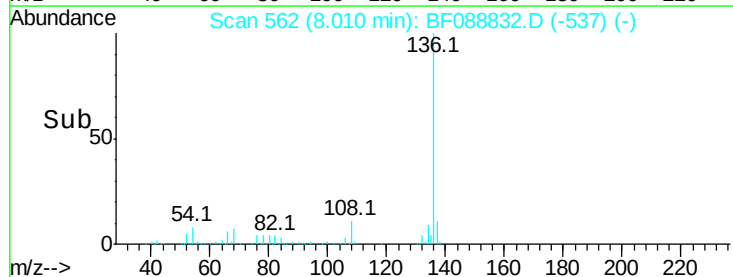
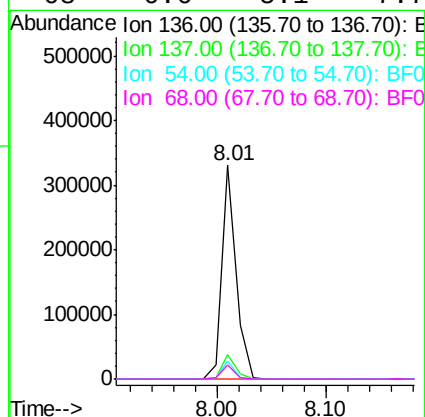
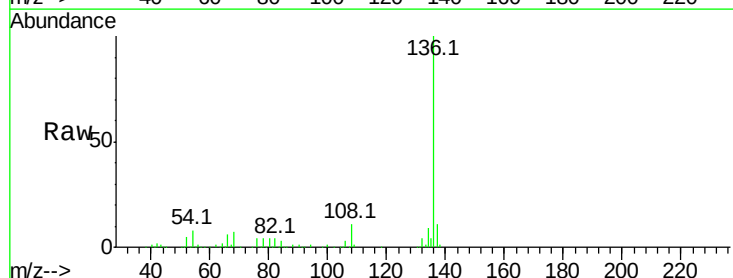


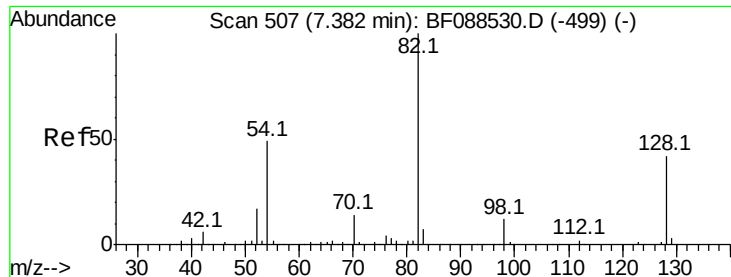

#23
 Nitrobenzene-d5
 Concen: 0.12 ng
 RT: 7.29 min Scan# 499
 Delta R.T. -0.01 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57




Instrument :
 BNA_F
 ClientSampled :


Tot Ion: 82 Resp: 678
 Ion Ratio Lower Upper
 82 100
 128 53.3 35.9 53.9
 54 50.2 40.9 61.3

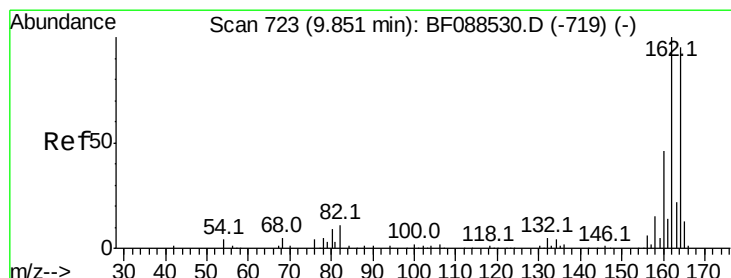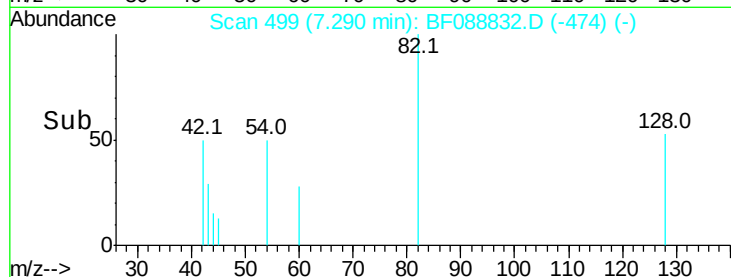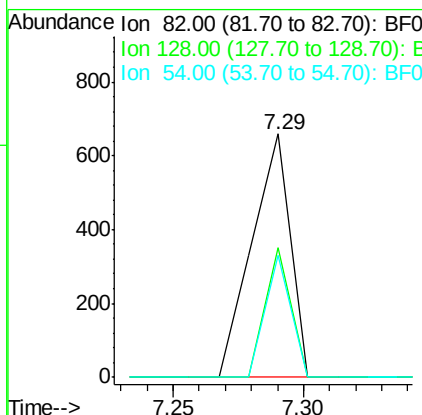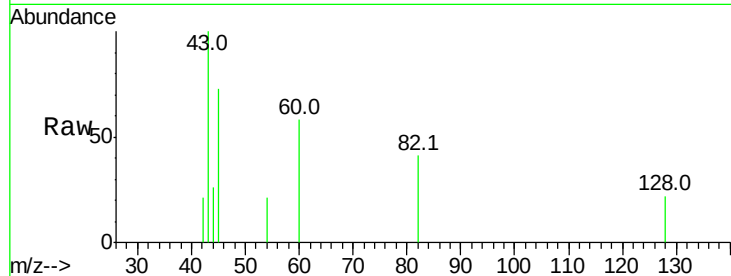

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.76 min Scan# 715
 Delta R.T. -0.01 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57

Tgt Ion:164 Resp: 145482
 Ion Ratio Lower Upper
 164 100
 162 105.6 85.4 128.2
 160 47.4 39.5 59.3

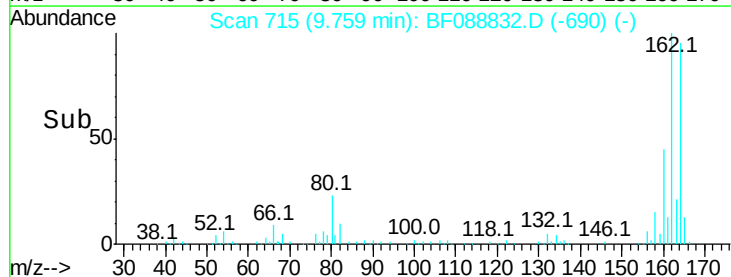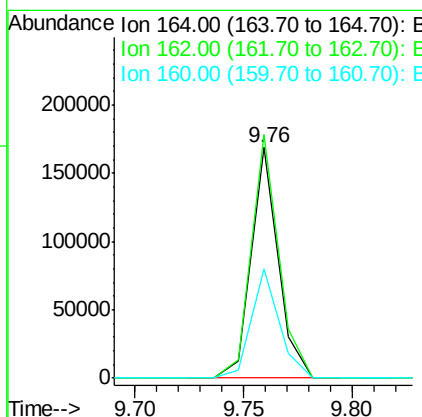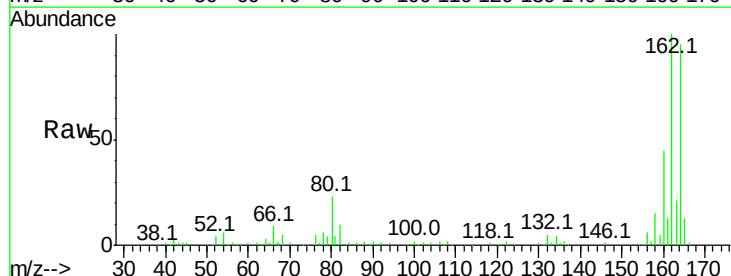


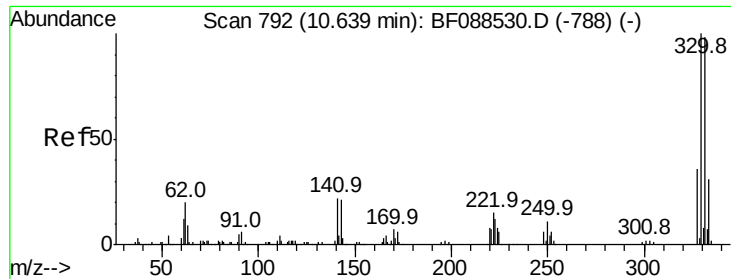




#41
 2,4,6-Tribromophenol
 Concen: 0.16 ng
 RT: 10.55 min Scan# 784
 Delta R.T. -0.01 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 211
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 0.0 0.0 0.0

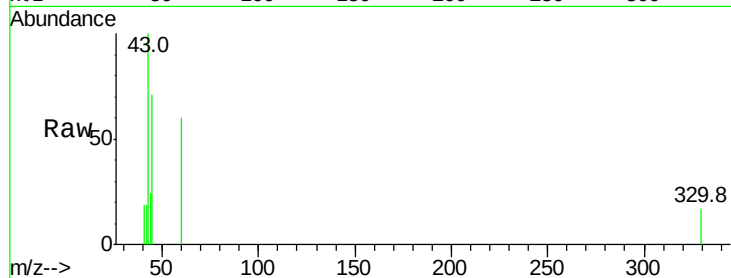


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

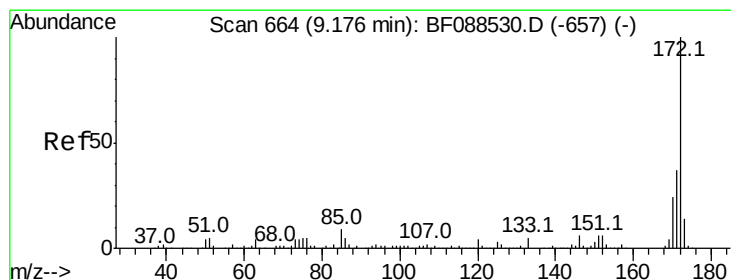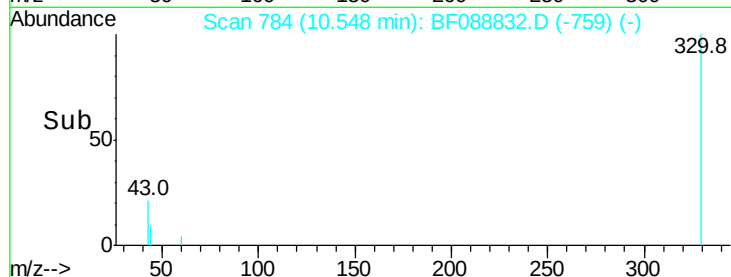
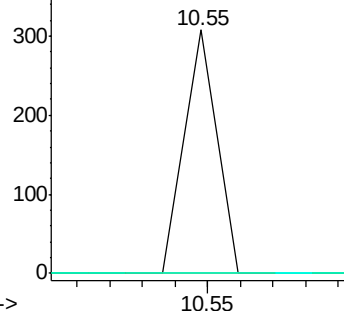



#44
 2-Fluorobiphenyl
 Concen: 0.15 ng
 RT: 9.08 min Scan# 656
 Delta R.T. -0.01 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57

Tgt Ion:172 Resp: 1421
 Ion Ratio Lower Upper
 172 100
 171 31.1 28.6 43.0
 170 20.8 19.2 28.8

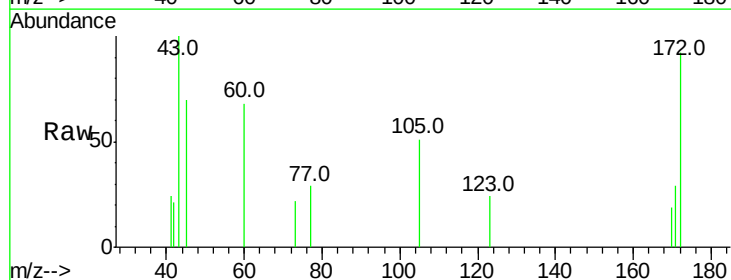

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

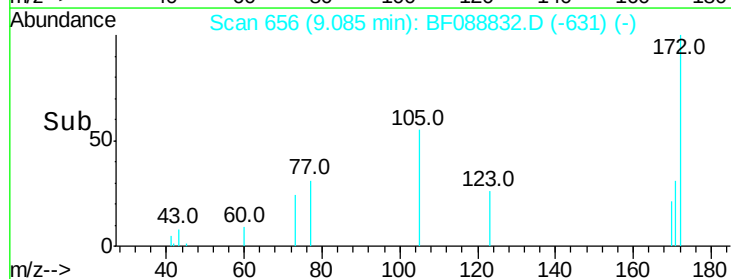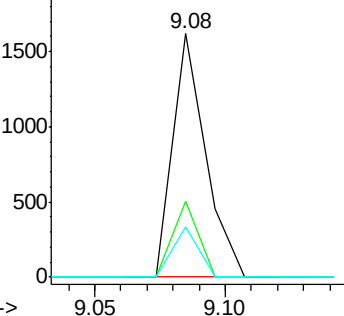


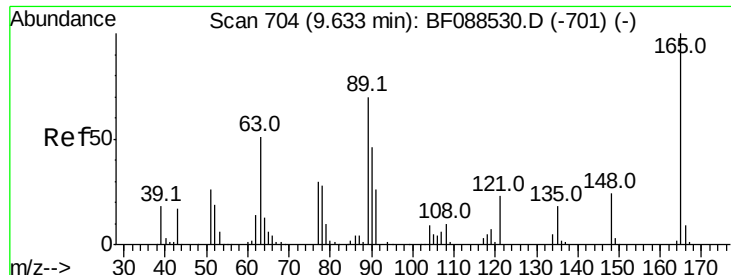

#50
 2,6-Dinitrotoluene
 Concen: 8.17 ng
 RT: 9.76 min Scan# 715
 Delta R.T. 0.19 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57

Instrument :
 BNA_F
 ClientSampleId :




Tot Ion	Ratio	Lower	Upper
165	100		
63	1.4	28.1	42.1#
89	1.4	32.2	48.2#

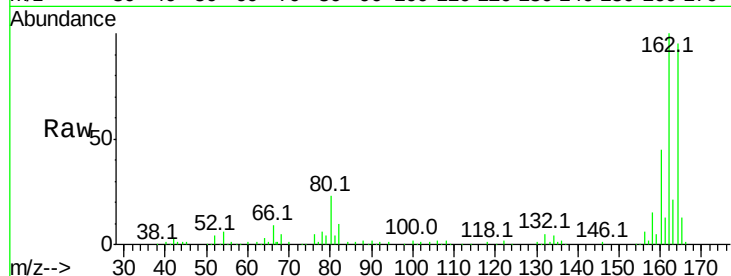

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

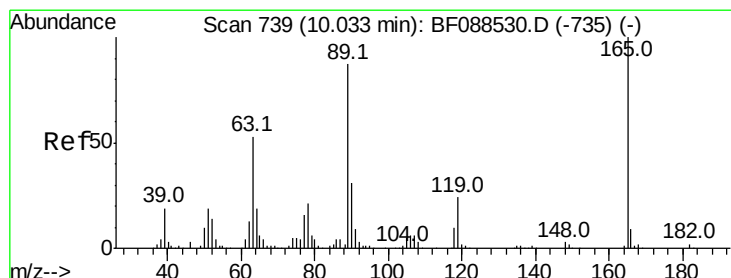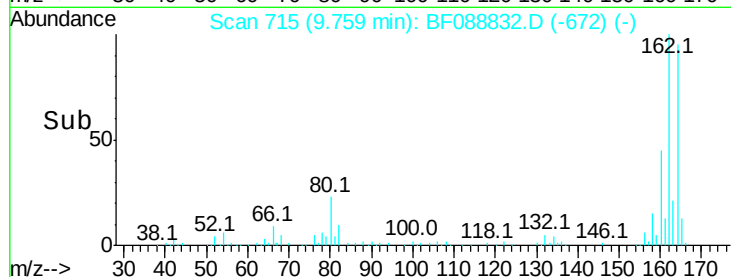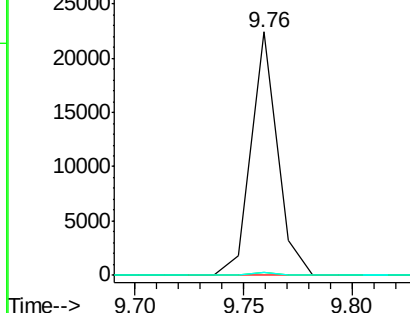

#56
 2,4-Dinitrotoluene
 Concen: 6.25 ng
 RT: 9.76 min Scan# 715
 Delta R.T. -0.19 min
 Lab File: BF088832.D
 Acq: 8 Jul 2016 18:57




Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.4	22.0	33.0#
89	1.4	41.1	61.7#
182	0.0	2.0	3.0#


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

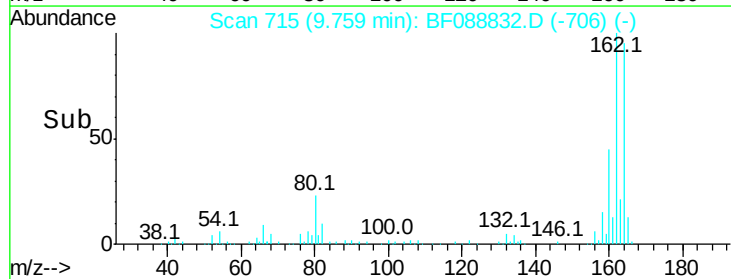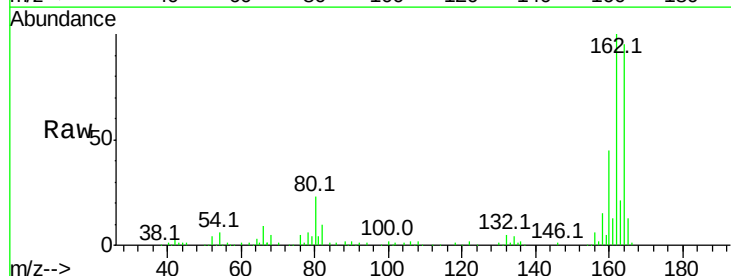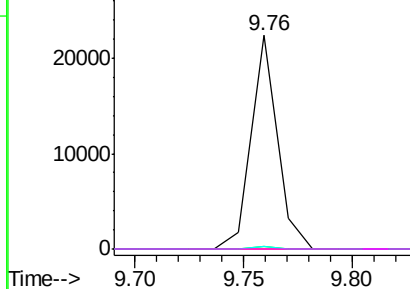


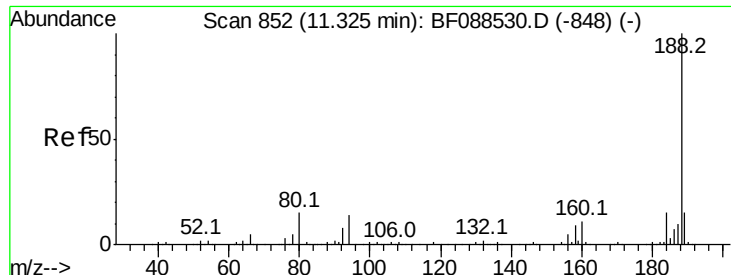




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.23 min Scan# 844
Delta R.T. -0.01 min
Lab File: BF088832.D
Acq: 8 Jul 2016 18:57

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 273540
Ion Ratio Lower Upper
188 100
94 12.1 9.0 13.6
80 14.2 10.0 15.0

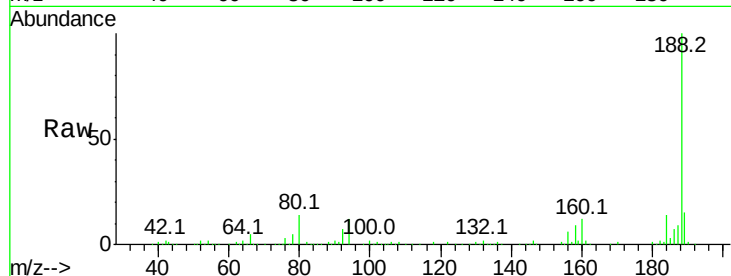


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

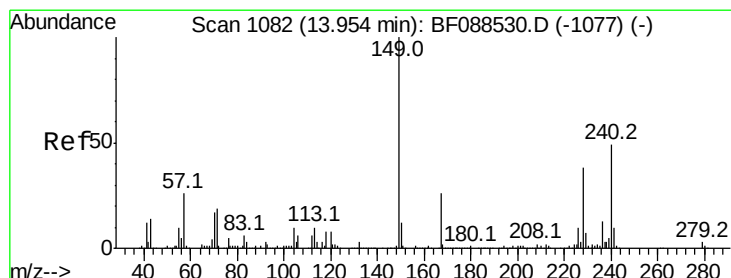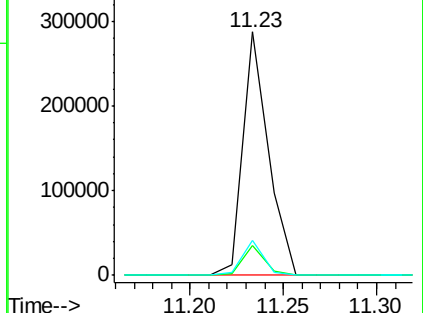
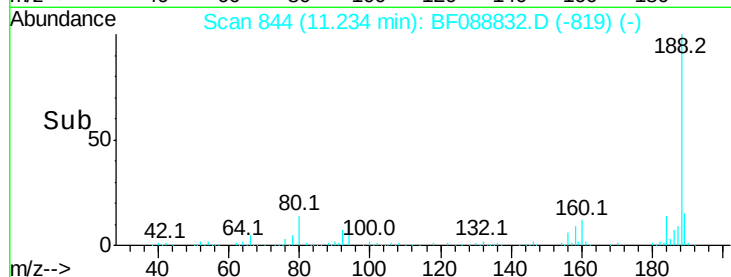



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.86 min Scan# 1074
Delta R.T. -0.01 min
Lab File: BF088832.D
Acq: 8 Jul 2016 18:57

Tgt Ion:240 Resp: 186791
Ion Ratio Lower Upper
240 100
120 8.2 6.8 10.2
236 26.0 20.2 30.2

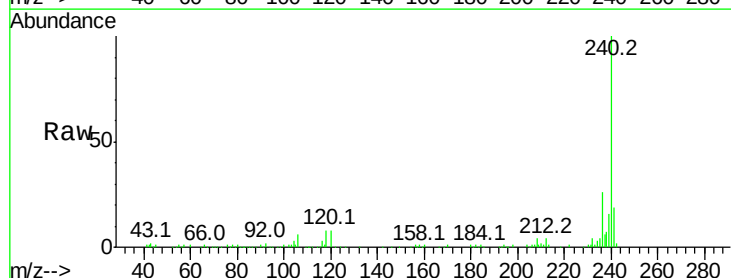

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

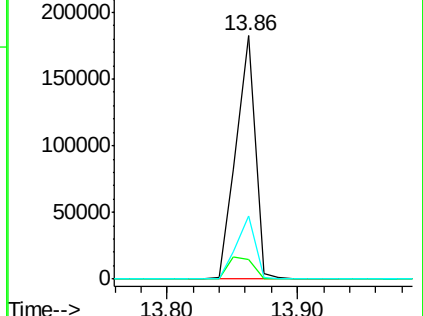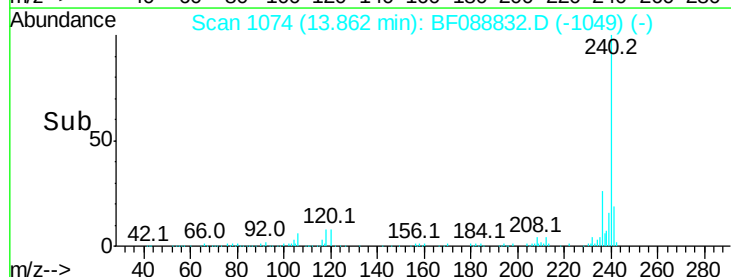

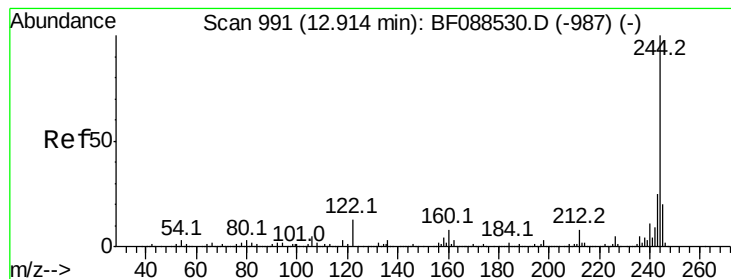

#78

Terphenyl-d14

Concen: 0.17 ng

RT: 12.81 min Scan# 982

Delta R.T. -0.01 min

Lab File: BF088832.D

Acq: 8 Jul 2016 18:57

Instrument :

BNA_F

ClientSampled :


Tot Ion:244 Resp: 1393

Ion Ratio Lower Upper




244 100

212 0.0 6.0 9.0#

122 28.4 11.2 16.8#

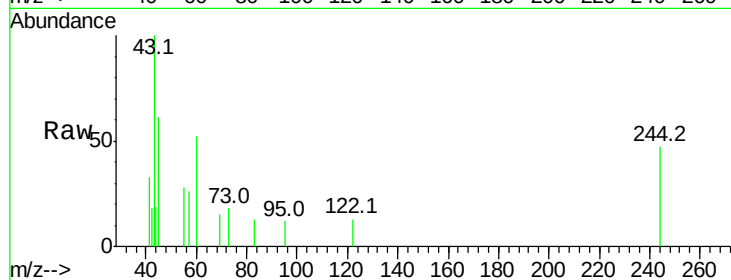

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

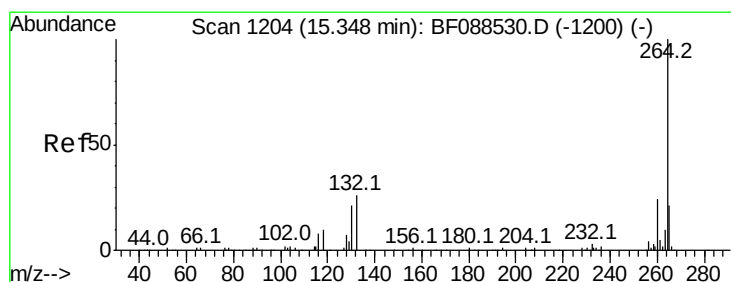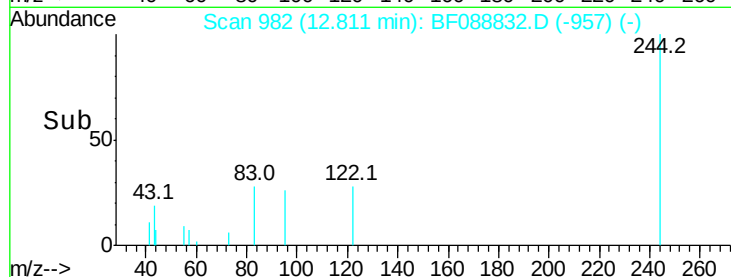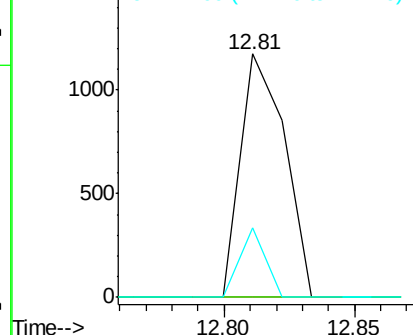

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.23 min Scan# 1194

Delta R.T. -0.01 min

Lab File: BF088832.D

Acq: 8 Jul 2016 18:57


Tgt Ion:264 Resp: 159767

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 21.2 16.9 25.3

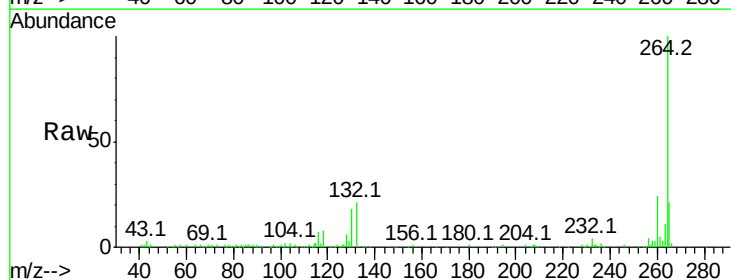

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

