
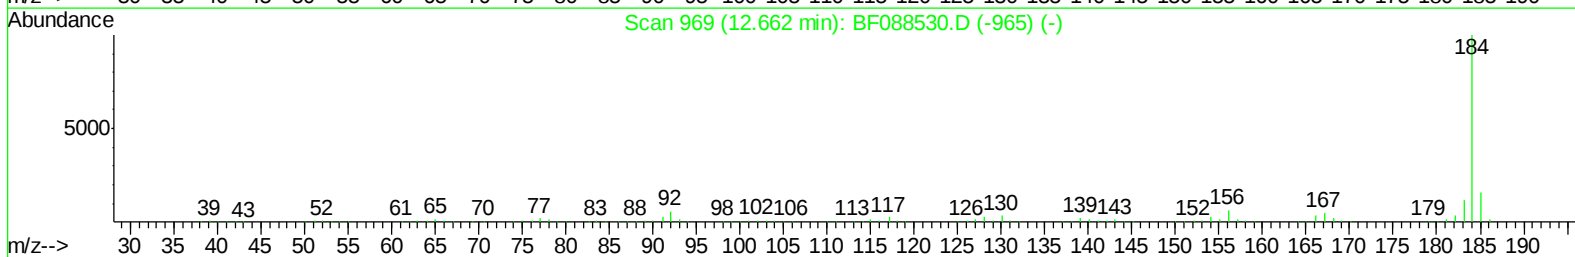
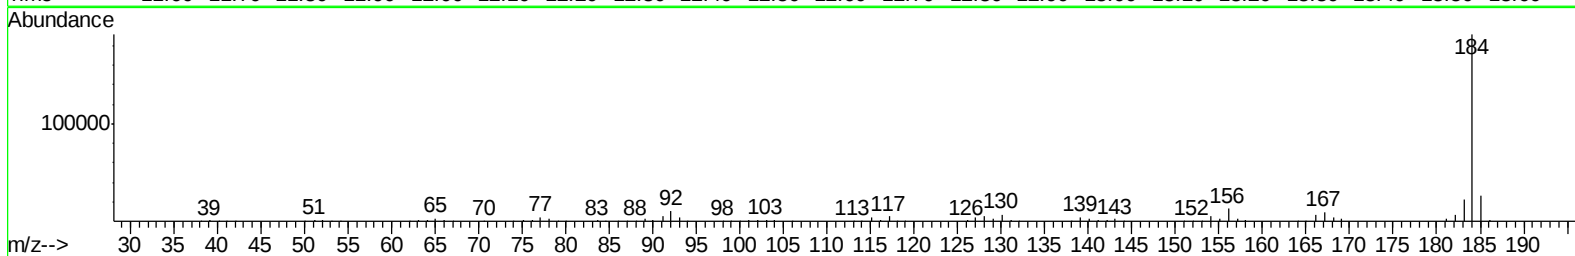


Data Path : Z:\HPCHEM1\BNA_F\Data\BF070816\
Data File : BF088855.D
Acq On : 9 Jul 2016 6:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 07:43:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 18:51:20 2016
Response via : Initial Calibration

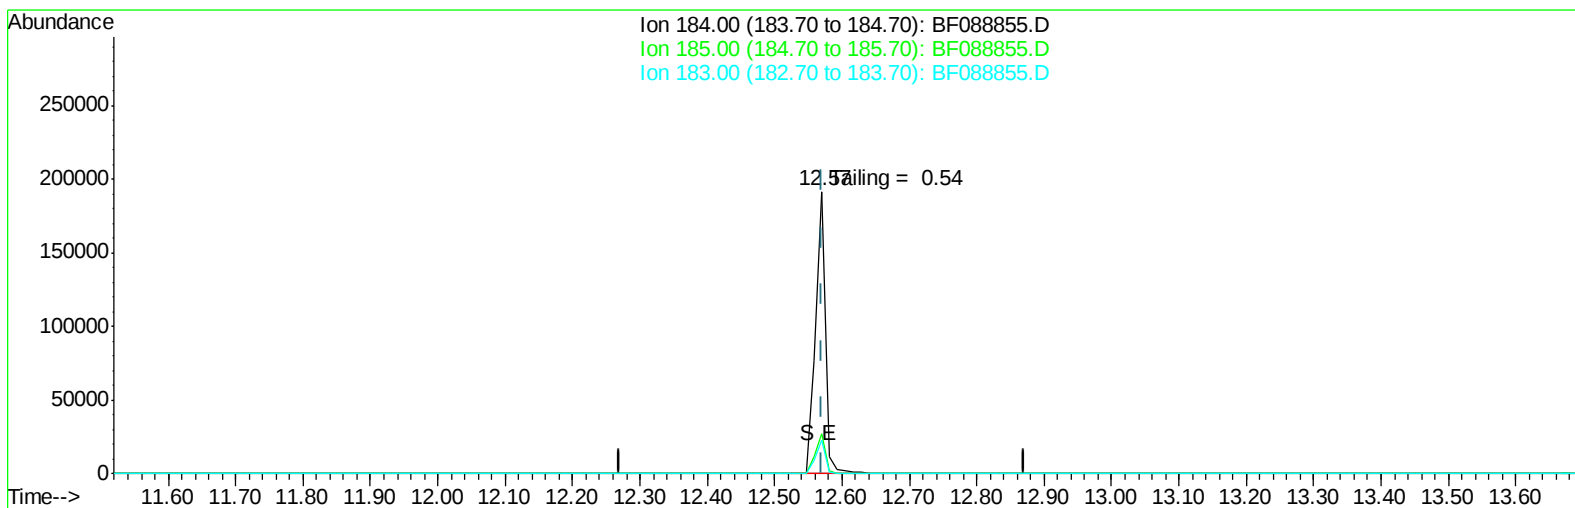

TIC: BF088855.D

(76) Benzidine




12.571min (-0.000) 0.00ng

response 196929

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.93
183.00	11.60	11.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF070816\
Data File : BF088855.D
Acq On : 9 Jul 2016 6:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 07:43:19 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 18:51:20 2016
Response via : Initial Calibration

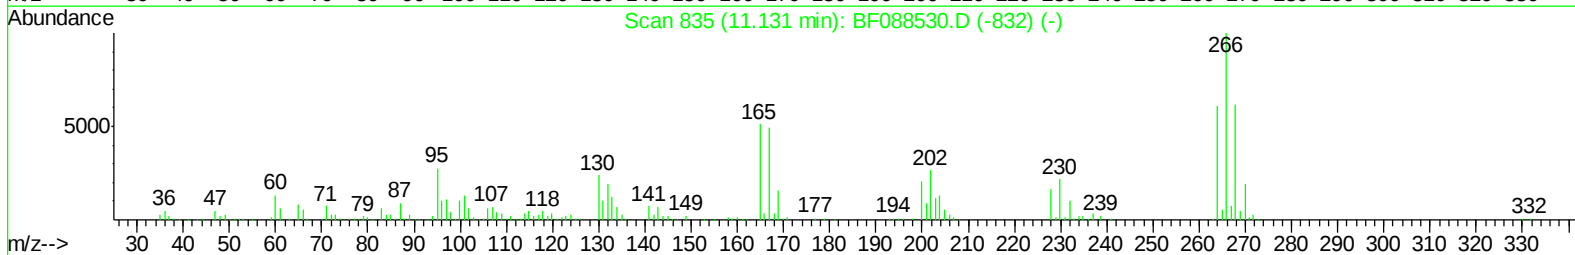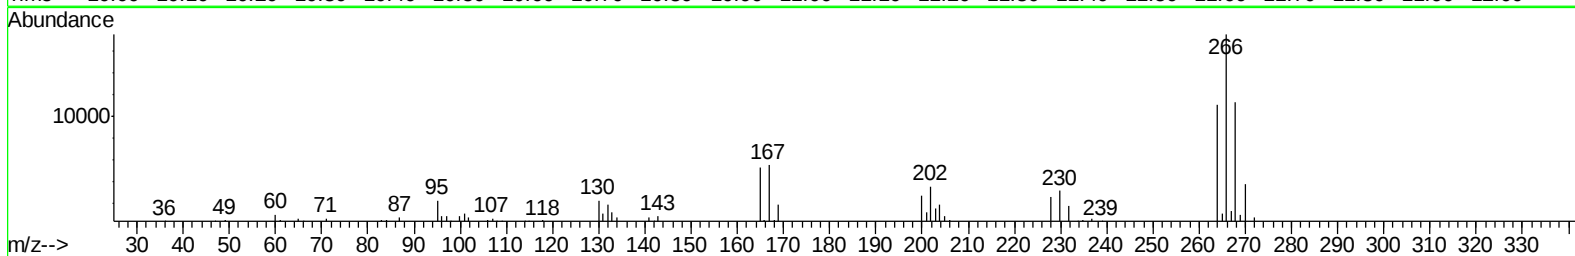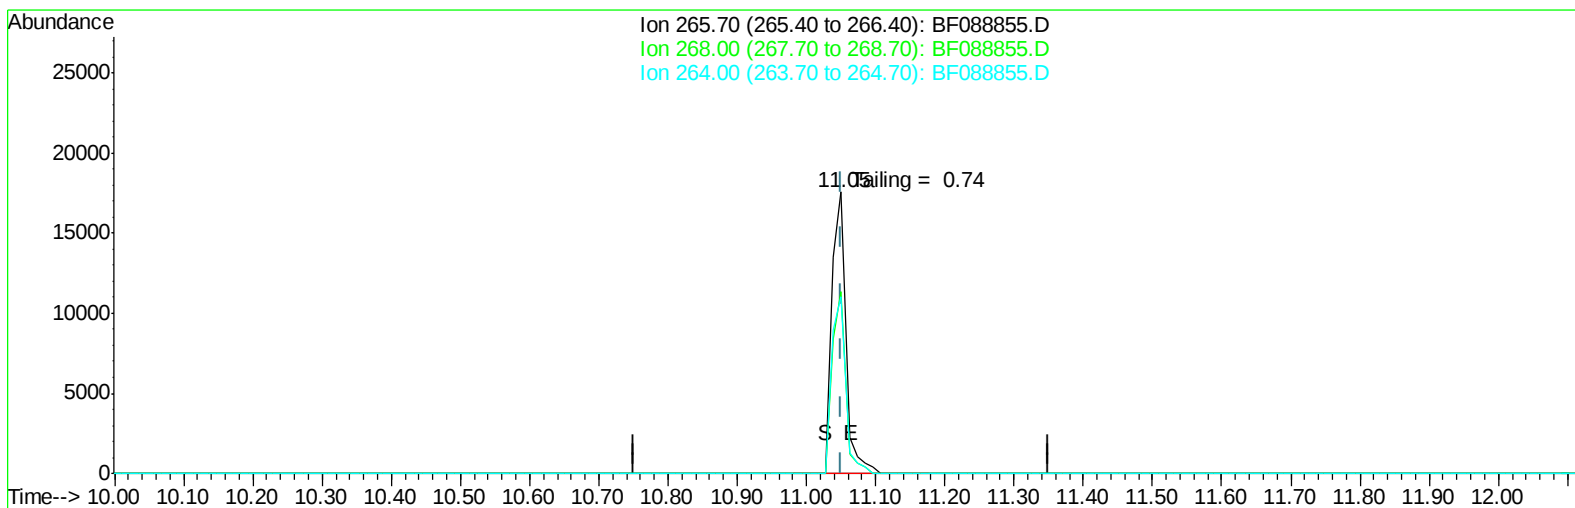

TIC: BF088855.D

(69) Pentachlorophenol (C)

11.051min (-0.000) 0.00ng

response 24248

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.42
264.00	62.00	62.80
0.00	0.00	0.00