

Data Path : V:\HPCHEM1\BNA F\DATA\BF070816\
 Data File : BF088851.D
 Acq On : 9 Jul 2016 4:10
 Operator : UM/SJ
 Sample : H3813-25 50X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-WW001-02

Quant Time: Jul 09 04:55:14 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 18:51:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	72905	20.00	ng	0.00
21) Naphthalene-d8	8.01	136	275644	20.00	ng	-0.01
38) Acenaphthene-d10	9.76	164	133723	20.00	ng	-0.01
63) Phenanthrene-d10	11.23	188	241961	20.00	ng	-0.01
75) Chrysene-d12	13.86	240	162420	20.00	ng	-0.01
86) Perylene-d12	15.23	264	148185	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	3480	0.72	ng	-0.01
7) Phenol-d6	6.35	99	3385	0.54	ng	-0.02
23) Nitrobenzene-d5	7.29	82	7548	1.44	ng	-0.01
41) 2,4,6-Tribromophenol	10.55	330	2568	2.07	ng	-0.01
44) 2-Fluorobiphenyl	9.08	172	17352	2.05	ng	-0.01
78) Terphenyl-d14	12.82	244	12327	1.69	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : V:\HPCHEM1\BNA F\DATA\BF070816\
Data File : BF088851.D
Acq On : 9 Jul 2016 4:10
Operator : UM/SJ
Sample : H3813-25 50X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-WW001-02

Quant Time: Jul 09 04:55:14 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 18:51:20 2016
Response via : Initial Calibration




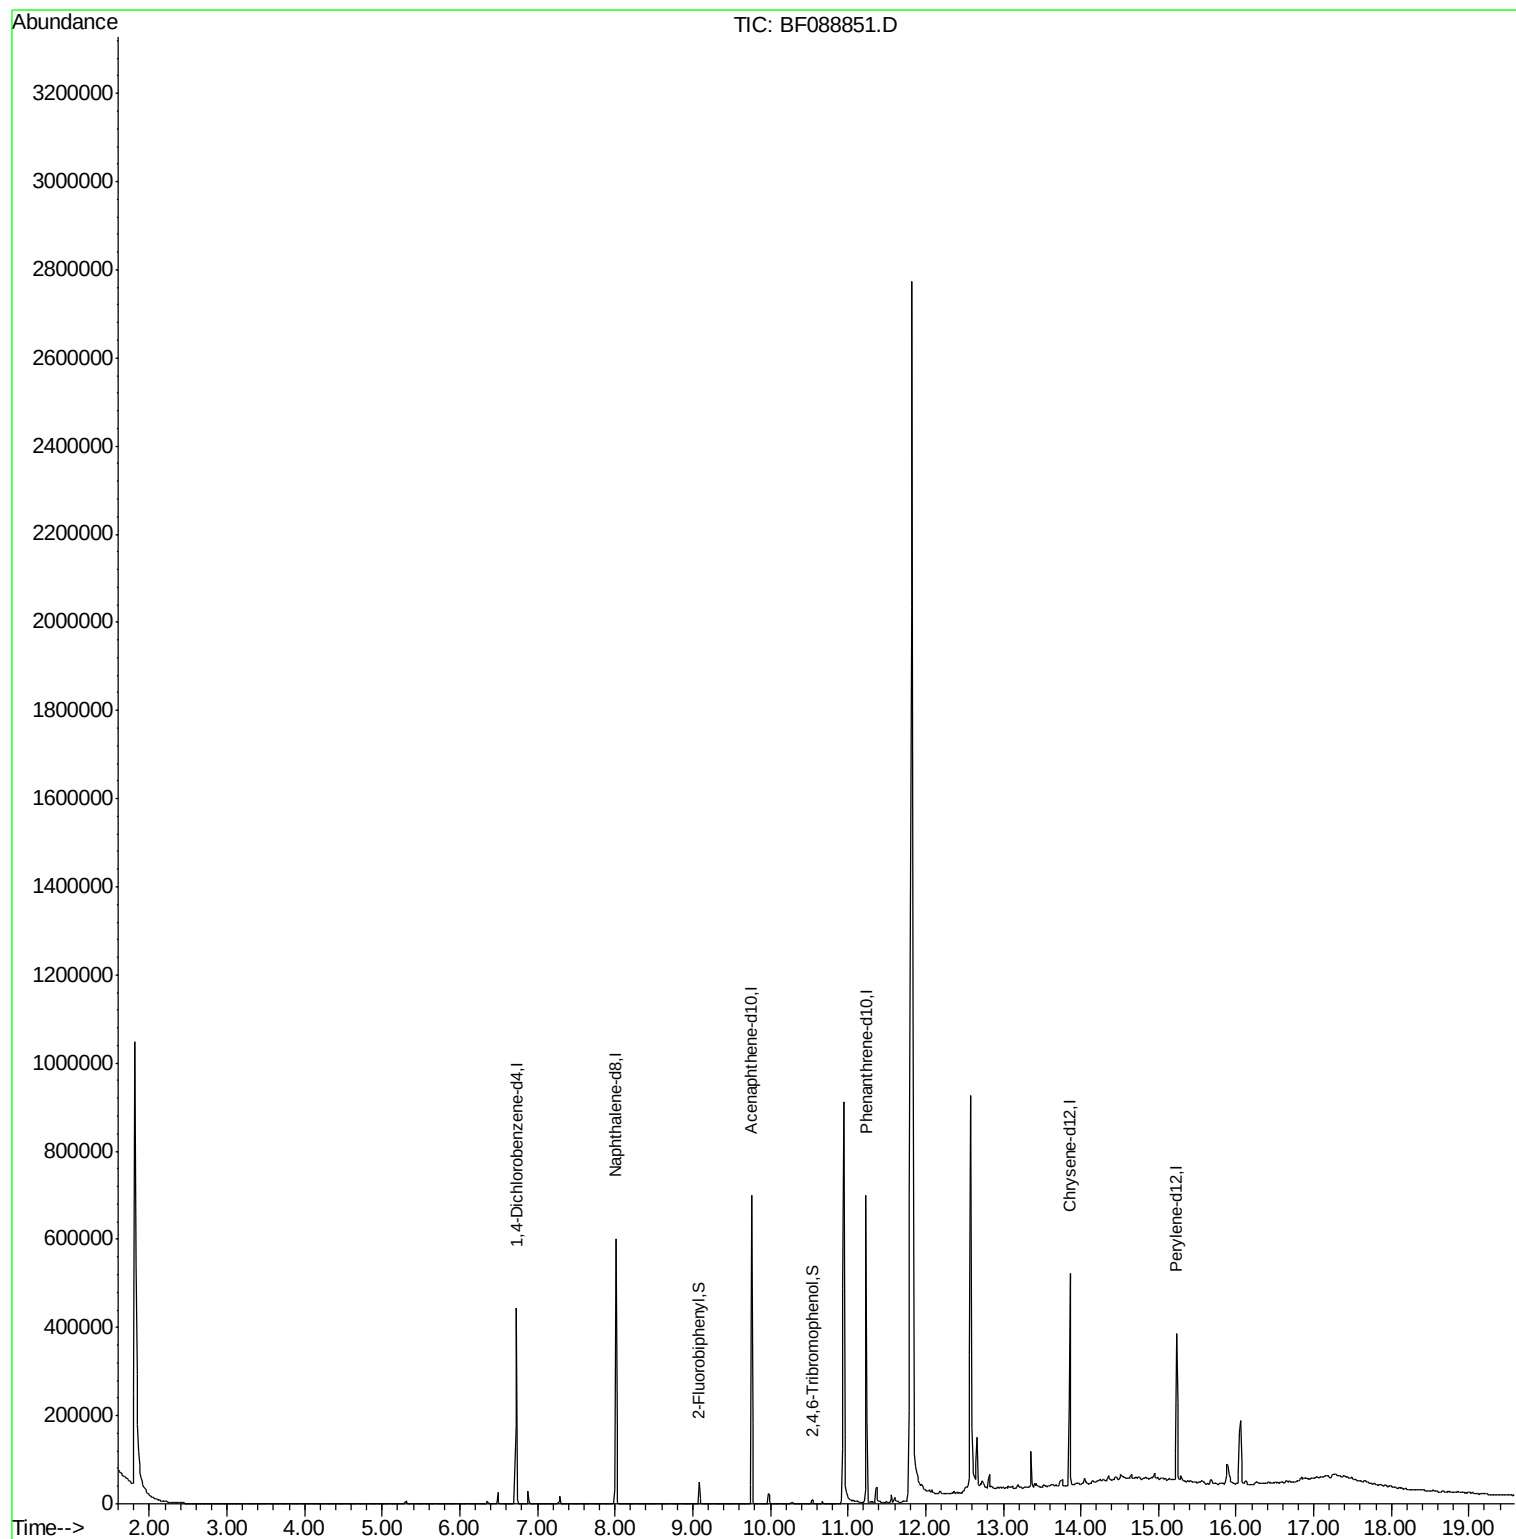


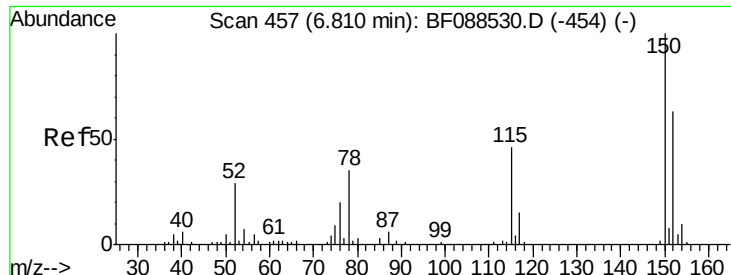

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.73 min Scan# 450
 Delta R.T. 0.00 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10




Instrument :
 BNA_F
 ClientSampleId :
 P001-WW001-02


Tot Ion:152 Resp: 72905
 Ion Ratio Lower Upper
 152 100
 150 156.1 123.8 185.6
 115 60.6 39.6 59.4#

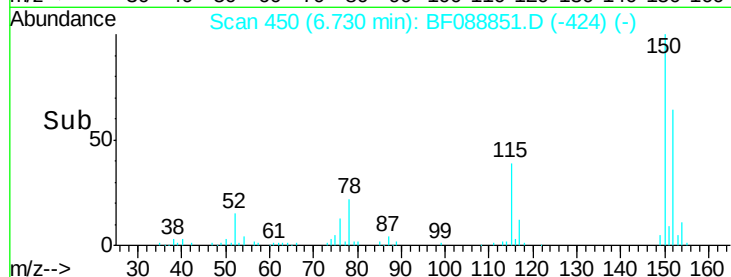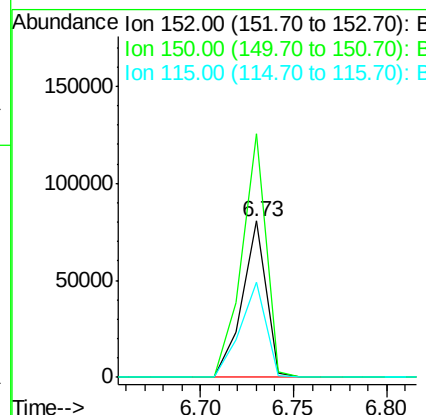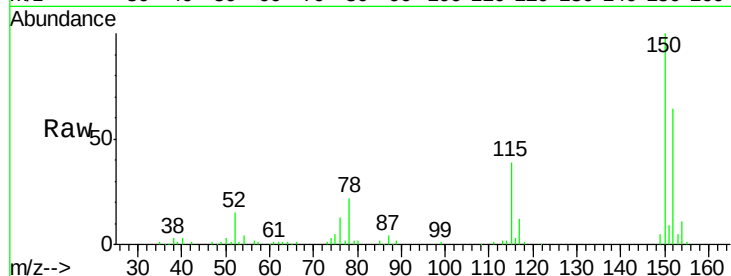

#5
 2-Fluorophenol
 Concen: 0.72 ng
 RT: 5.31 min Scan# 326
 Delta R.T. -0.01 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Tgt Ion:112 Resp: 3480
 Ion Ratio Lower Upper
 112 100
 64 47.7 42.2 63.2
 63 24.2 21.8 32.8

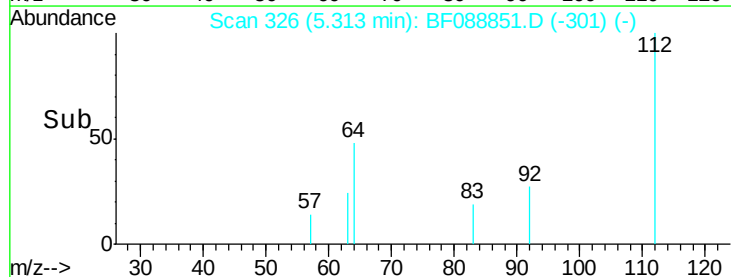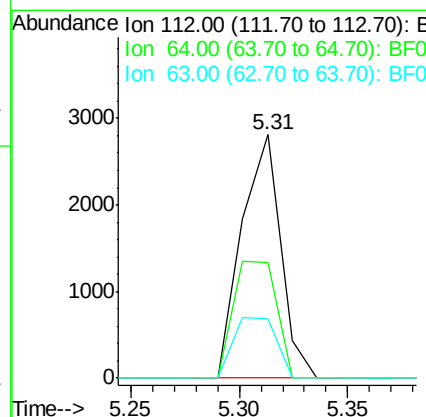

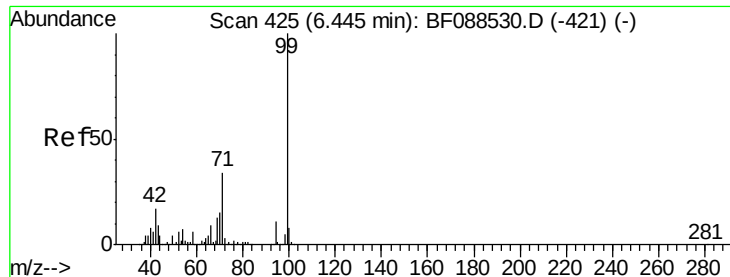

#7

Phenol-d6

Concen: 0.54 ng

RT: 6.35 min Scan# 417

Delta R.T. -0.02 min

Lab File: BF088851.D

Acq: 9 Jul 2016 4:10

Instrument :


BNA_F

ClientSampleId :

P001-WW001-02

Tot Ion: 99 Resp: 3385




Ion	Ratio	Lower	Upper
99	100		
42	20.2	12.2	18.2#
71	34.4	23.4	35.0

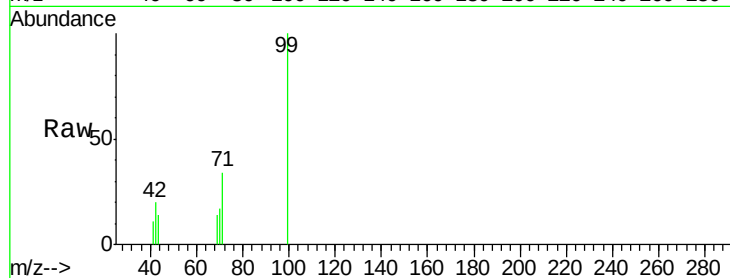

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

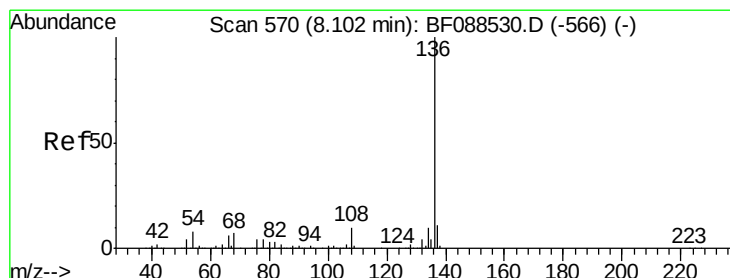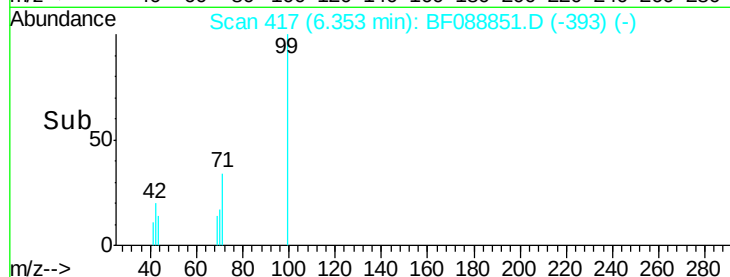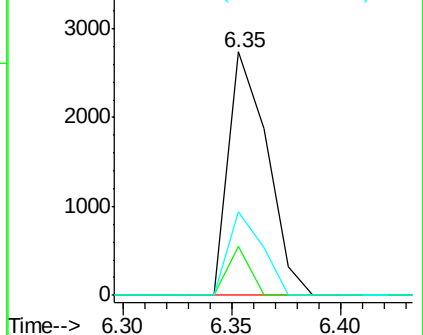

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.01 min Scan# 562

Delta R.T. -0.01 min

Lab File: BF088851.D

Acq: 9 Jul 2016 4:10

Tgt Ion: 136 Resp: 275644




Ion	Ratio	Lower	Upper
136	100		
137	11.4	9.1	13.7
54	9.0	6.6	10.0
68	6.9	5.1	7.7


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

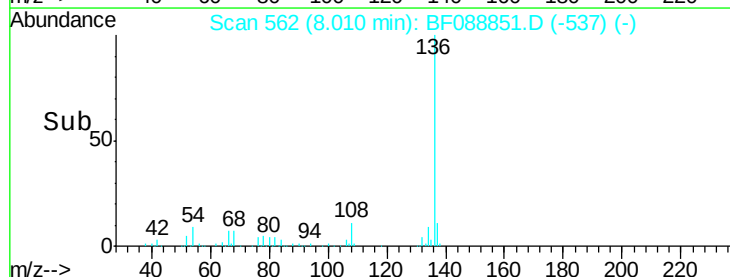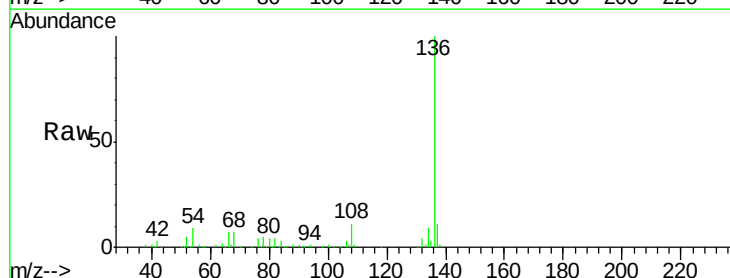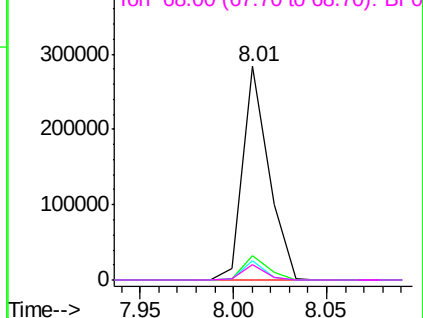


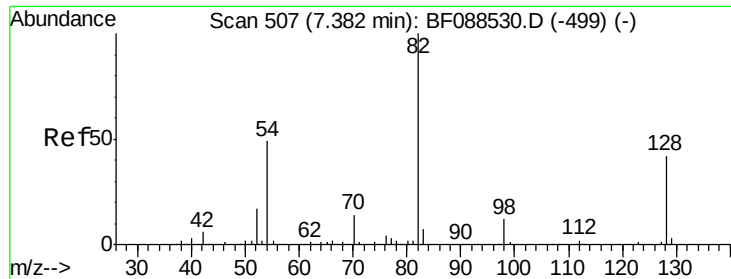




#23
 Nitrobenzene-d5
 Concen: 1.44 ng
 RT: 7.29 min Scan# 499
 Delta R.T. -0.01 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Instrument :
 BNA_F
 ClientSampleId :
 P001-WW001-02

Tot Ion	82	Resp	7548
Ion Ratio	Lower	Upper	
82	100		
128	46.6	35.9	53.9
54	42.0	40.9	61.3

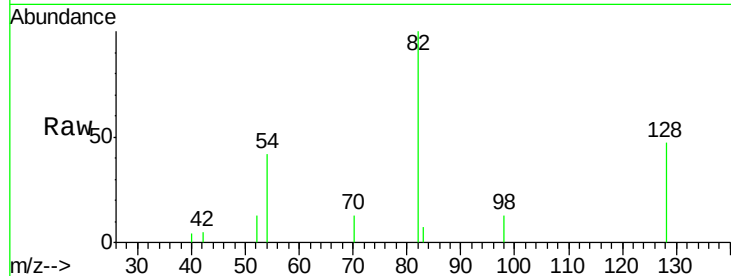


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

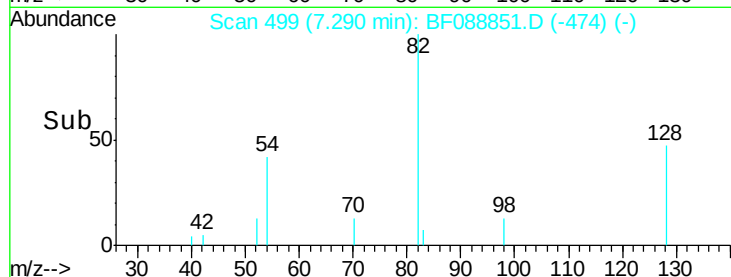
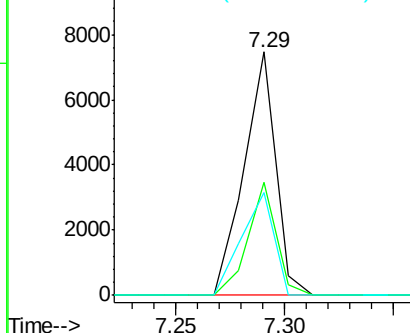



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.76 min Scan# 715
 Delta R.T. -0.01 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Tgt Ion	164	Resp	133723
Ion Ratio	Lower	Upper	
164	100		
162	102.5	85.4	128.2
160	46.2	39.5	59.3



Abundance Ion 164.00 (163.70 to 164.70): B
 Ion 162.00 (161.70 to 162.70): B
 Ion 160.00 (159.70 to 160.70): B

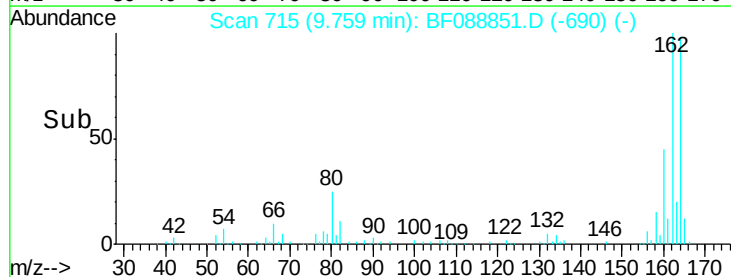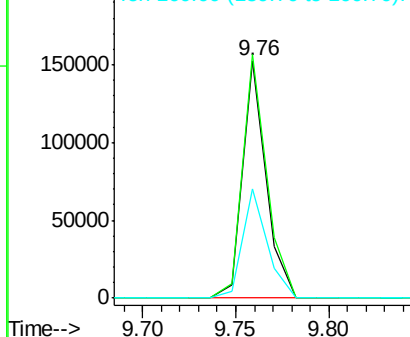


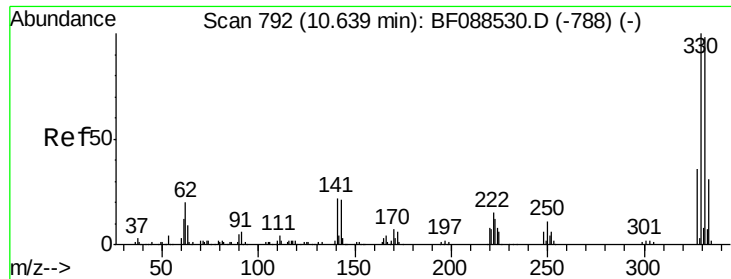




#41
 2,4,6-Tribromophenol
 Concen: 2.07 ng
 RT: 10.55 min Scan# 784
 Delta R.T. -0.01 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Instrument :
 BNA_F
 ClientSampleId :
 P001-WW001-02

Tot Ion:330 Resp: 2568
 Ion Ratio Lower Upper
 330 100
 332 87.3 0.0 0.0#
 141 43.4 0.0 0.0#

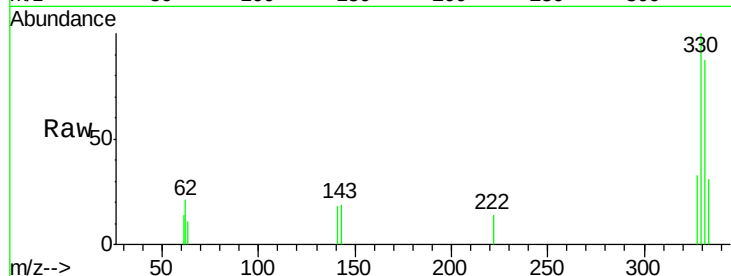


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

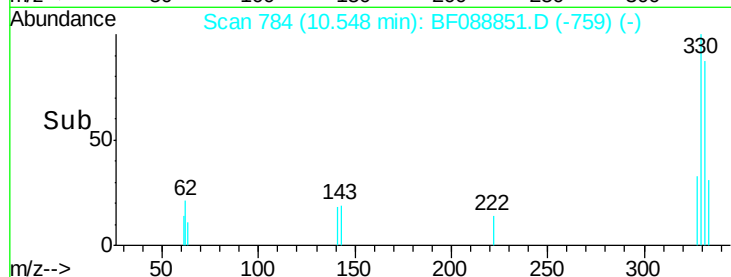
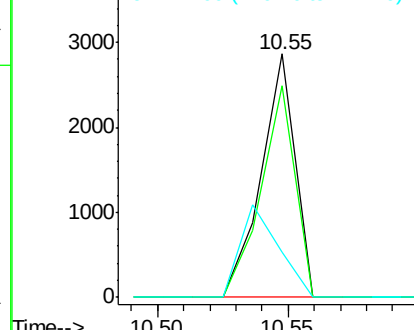



#44
 2-Fluorobiphenyl
 Concen: 2.05 ng
 RT: 9.08 min Scan# 656
 Delta R.T. -0.01 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Tgt Ion:172 Resp: 17352
 Ion Ratio Lower Upper
 172 100
 171 35.0 28.6 43.0
 170 23.5 19.2 28.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



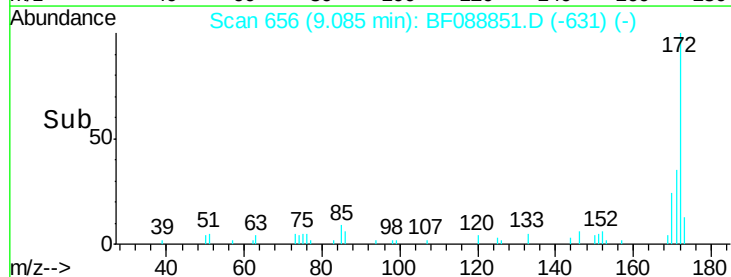
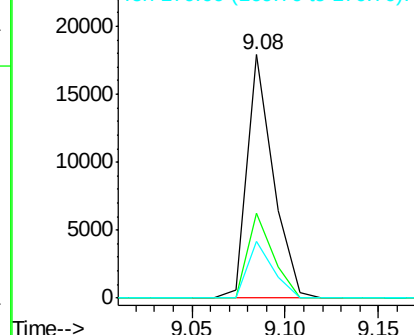


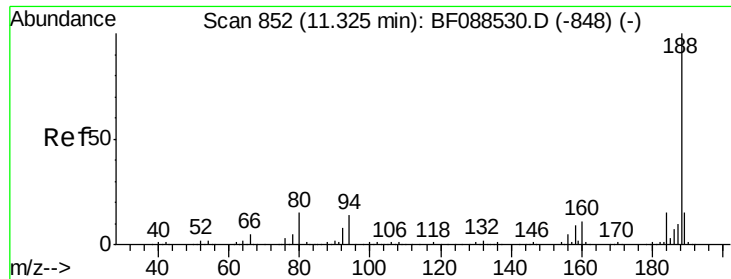

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.23 min Scan# 844
Delta R.T. -0.01 min
Lab File: BF088851.D
Acq: 9 Jul 2016 4:10




Instrument :
BNA_F
ClientSampleId :
P001-WW001-02


Tot Ion:188 Resp: 241961
Ion Ratio Lower Upper
188 100
94 12.3 9.0 13.6
80 14.1 10.0 15.0

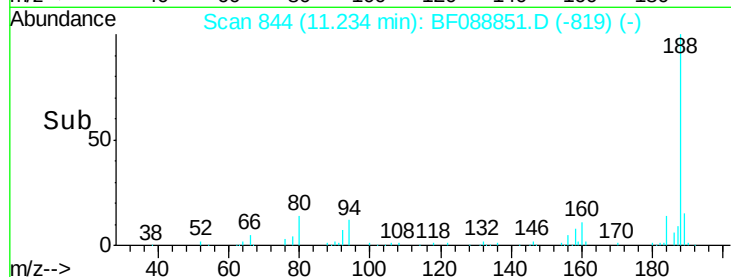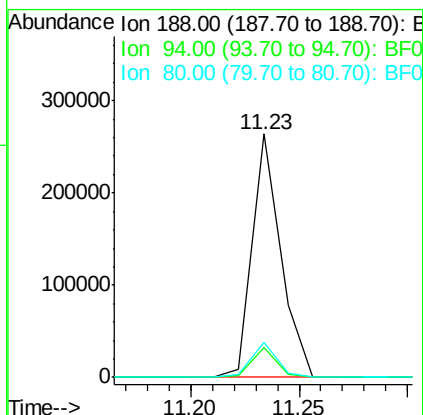

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.86 min Scan# 1074
Delta R.T. -0.01 min
Lab File: BF088851.D
Acq: 9 Jul 2016 4:10

Tgt Ion:240 Resp: 162420
Ion Ratio Lower Upper
240 100
120 9.8 6.8 10.2
236 25.6 20.2 30.2


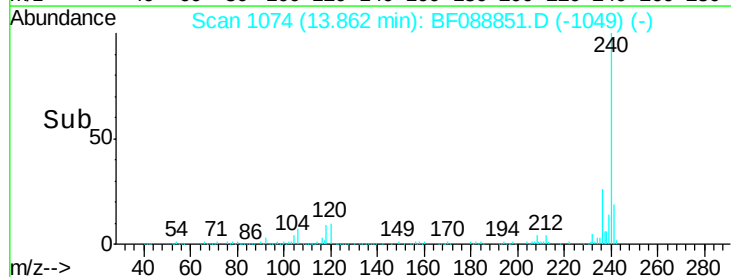
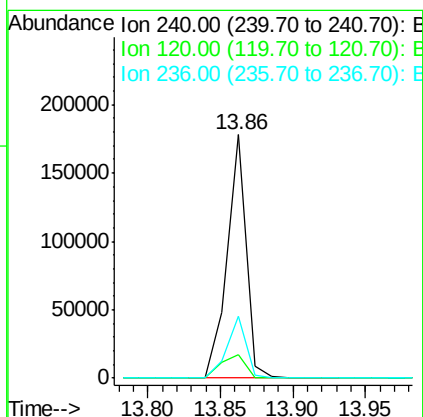



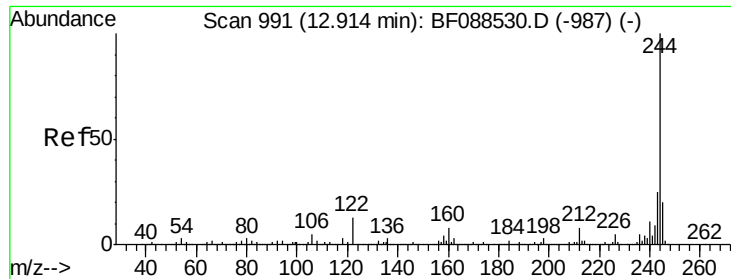

#78
 Terphenyl-d14
 Concen: 1.69 ng
 RT: 12.82 min Scan# 983
 Delta R.T. 0.00 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Instrument :
 BNA_F
 ClientSampleId :
 P001-WW001-02

Tot Ion:244 Resp: 12327
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.0 9.0
 122 9.0 11.2 16.8#

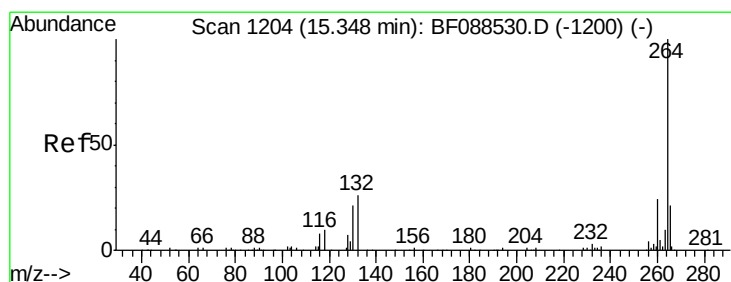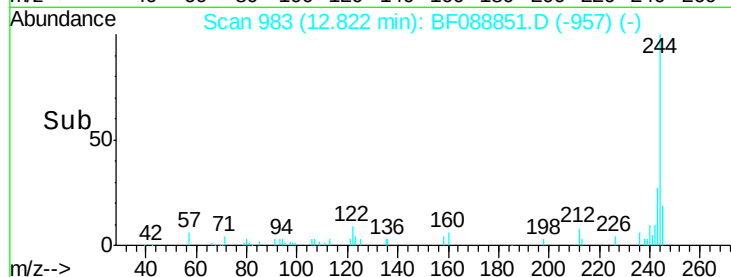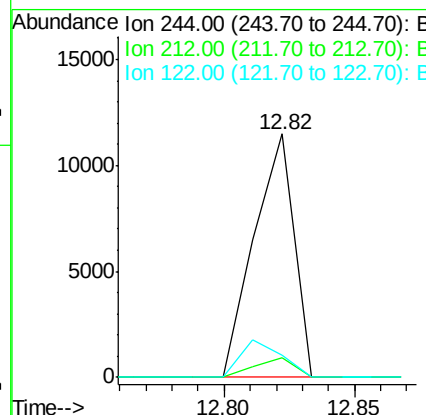

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.23 min Scan# 1194
 Delta R.T. -0.01 min
 Lab File: BF088851.D
 Acq: 9 Jul 2016 4:10

Tgt Ion:264 Resp: 148185
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 20.8 16.9 25.3

