

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
 Data File : BF088822.D
 Acq On : 8 Jul 2016 13:33
 Operator : UM/SJ
 Sample : PB91874BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB91874BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.690	7	9	18	rVV	254229	535136	19.86%	2.377%
2	1.804	18	19	61	rVB	798821	1923508	71.40%	8.545%
3	4.901	288	290	295	rVB	69084	111629	4.14%	0.496%
4	5.324	324	327	330	rBV	1409206	2083827	77.35%	9.257%
5	6.376	415	419	421	rBV	1793373	2276464	84.50%	10.113%
6	6.502	427	430	432	rBV	2035732	2260400	83.90%	10.042%
7	6.730	447	450	452	rBV	532358	454399	16.87%	2.019%
8	6.890	461	464	466	rBV	1612831	1776129	65.93%	7.890%
9	7.290	496	499	502	rBV	1058069	1252535	46.49%	5.564%
10	8.010	560	562	565	rBV	598542	581867	21.60%	2.585%
11	9.096	653	657	659	rBV	2112034	2694054	100.00%	11.968%
12	9.759	712	715	718	rVB	696857	668082	24.80%	2.968%
13	10.548	781	784	787	rBV	1569905	1544762	57.34%	6.863%
14	11.233	842	844	847	rBV	647923	682027	25.32%	3.030%
15	12.822	980	983	986	rBV	2194554	2442039	90.65%	10.849%
16	13.862	1071	1074	1076	rBV	715494	691243	25.66%	3.071%
17	15.234	1192	1194	1197	rBV	403962	531702	19.74%	2.362%




Sum of corrected areas: 22509803

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088822.D
Acq On : 8 Jul 2016 13:33
Operator : UM/SJ
Sample : PB91874BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91874BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

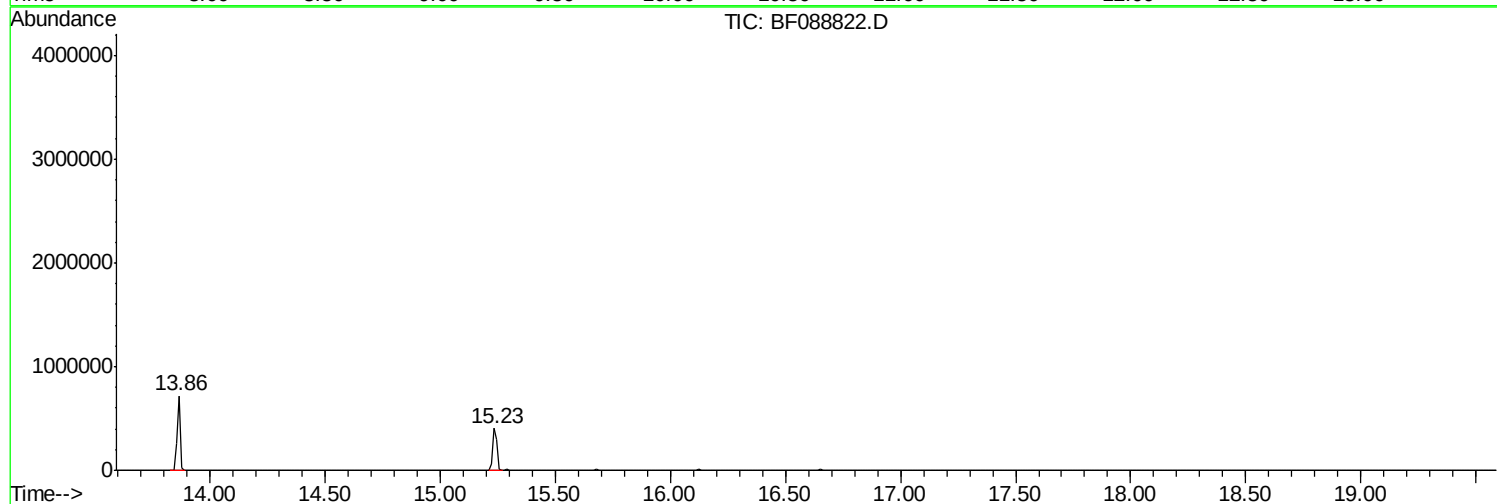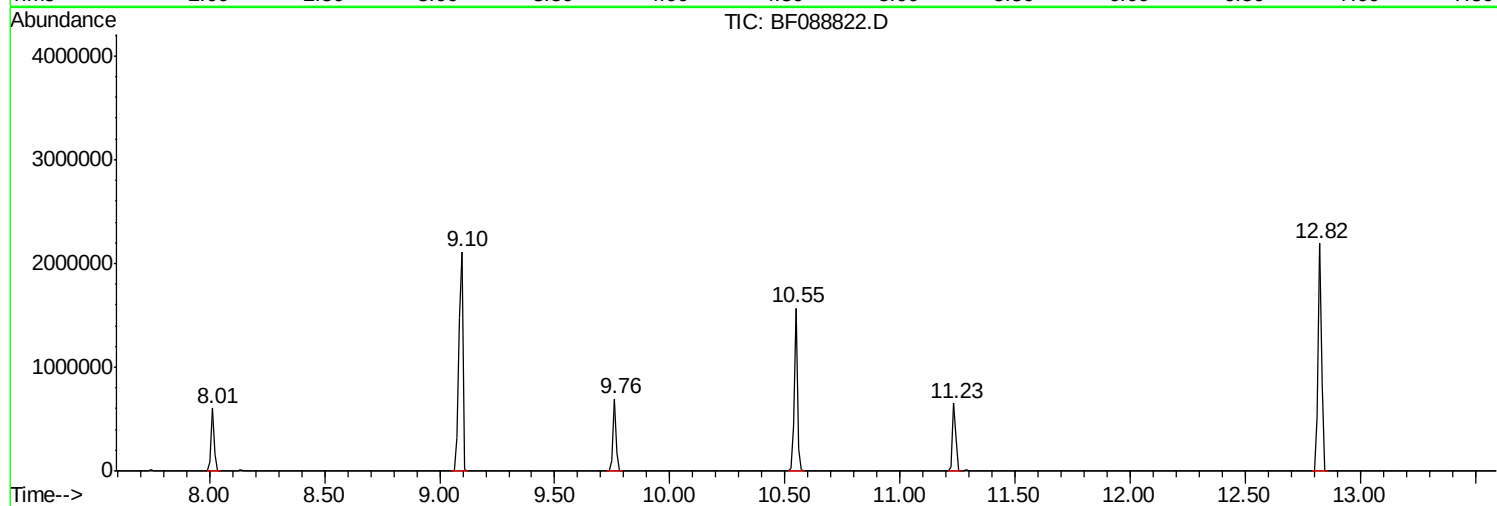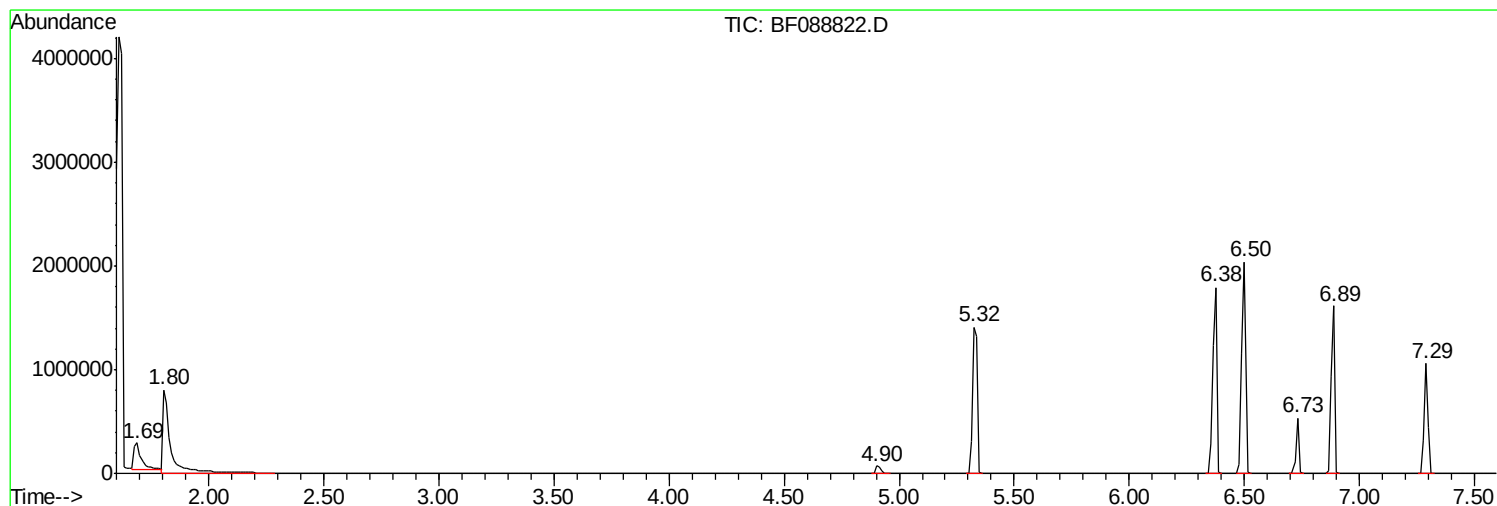

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088822.D
Acq On : 8 Jul 2016 13:33
Operator : UM/SJ
Sample : PB91874BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91874BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.90	4.91 ng	111629	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28
3		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4		Acetone	58	C3H6O	000067-64-1	10
5		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9

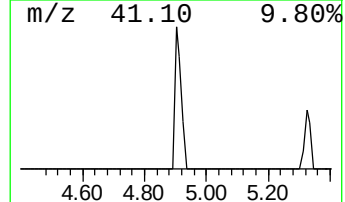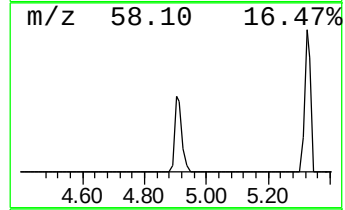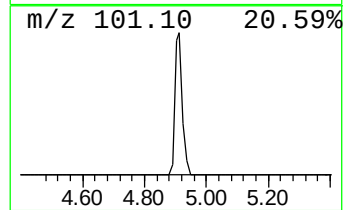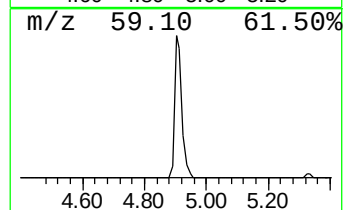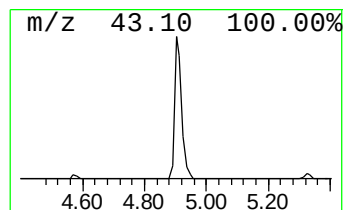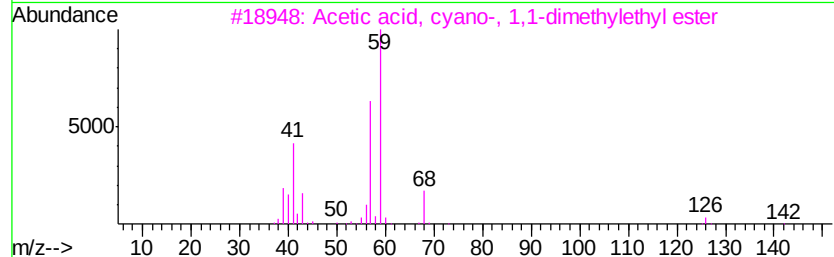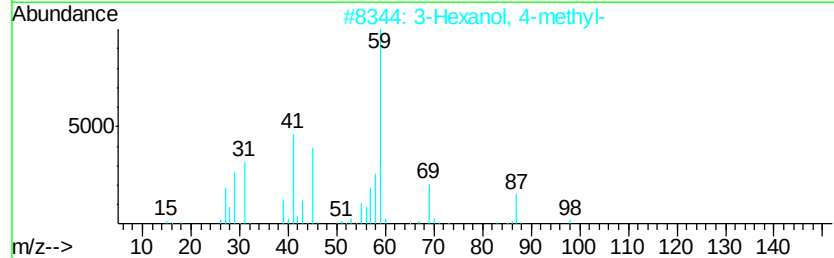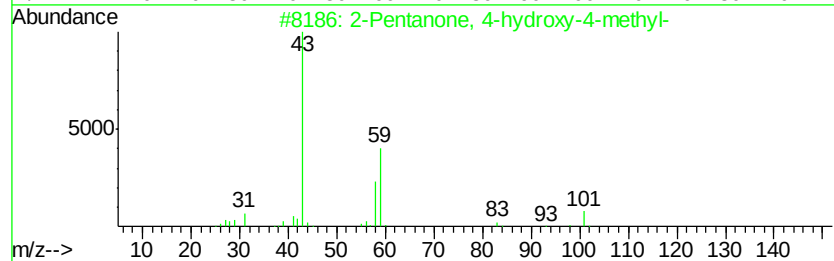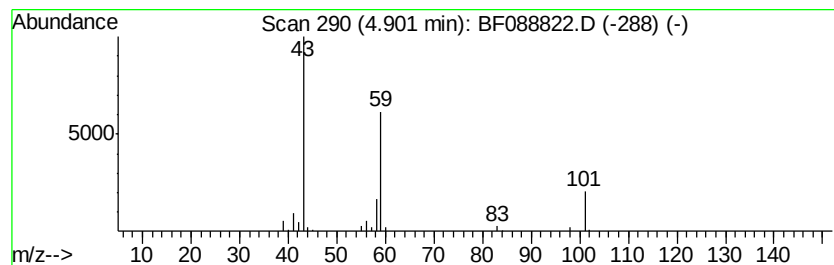

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088822.D
Acq On : 8 Jul 2016 13:33
Operator : UM/SJ
Sample : PB91874BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91874BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	99.49 ng	2260400	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		1,2,4-Trifluorobenzene	132	C6H3F3	000367-23-7	9
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

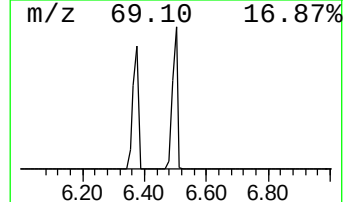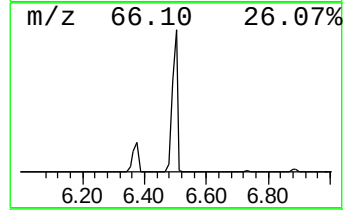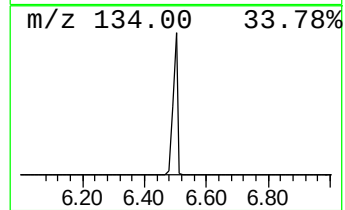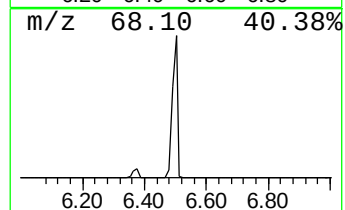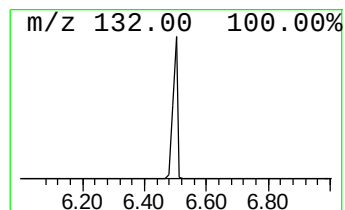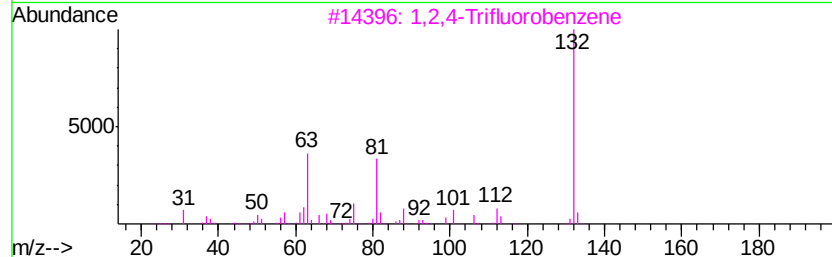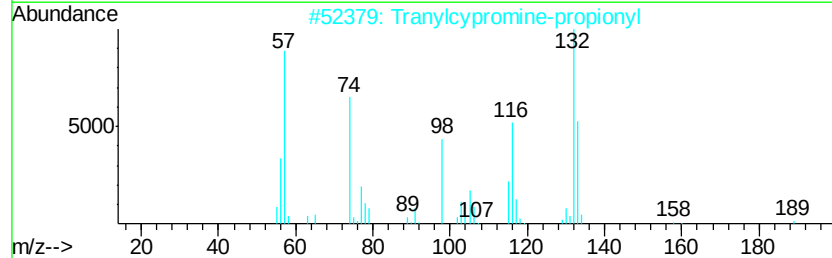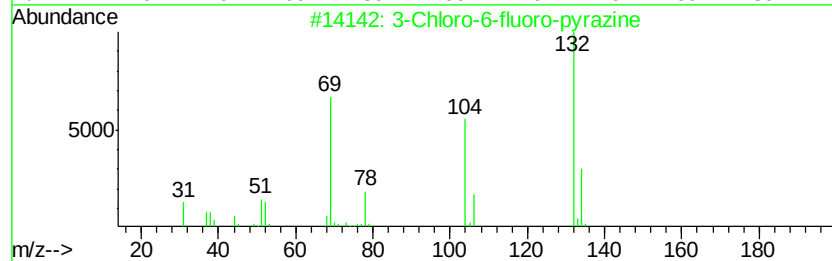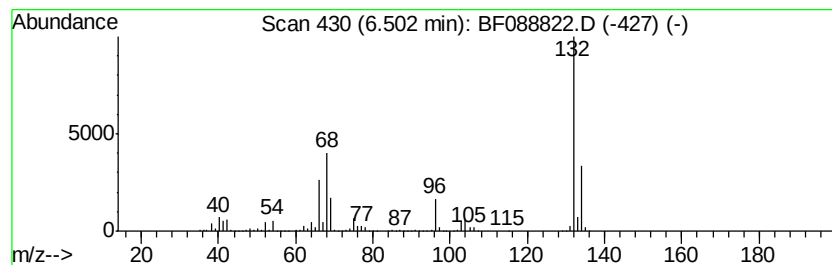

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088822.D
Acq On : 8 Jul 2016 13:33
Operator : UM/SJ
Sample : PB91874BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91874BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.90	4.9	ng	111629	1	6.73	454399	20.0
unknown6.50	6.50	99.5	ng	2260400	1	6.73	454399	20.0