

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
 Data File : BF088839.D
 Acq On : 8 Jul 2016 22:21
 Operator : UM/SJ
 Sample : H3813-09 50X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-DS001-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.815	18	20	52	rVB	1255864	2445898	100.00%	38.534%
2	5.313	323	326	328	rBV	22241	30069	1.23%	0.474%
3	6.353	415	417	423	rBV	37223	38677	1.58%	0.609%
4	6.490	427	429	431	rVB	47599	39450	1.61%	0.622%
5	6.730	447	450	452	rBV	492033	492667	20.14%	7.762%
6	6.879	461	463	466	rVB	37583	32001	1.31%	0.504%
7	8.010	560	562	565	rBV	731226	663579	27.13%	10.454%
8	9.085	654	656	659	rBV	62379	53200	2.18%	0.838%
9	9.759	713	715	718	rBV	876738	759794	31.06%	11.970%
10	11.234	842	844	847	rBV	834522	746646	30.53%	11.763%
11	12.811	981	982	985	rBV	40488	46343	1.89%	0.730%
12	13.862	1071	1074	1076	rBV	497527	539318	22.05%	8.497%
13	15.234	1191	1194	1197	rBV	420930	459680	18.79%	7.242%




Sum of corrected areas: 6347322

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088839.D
Acq On : 8 Jul 2016 22:21
Operator : UM/SJ
Sample : H3813-09 50X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

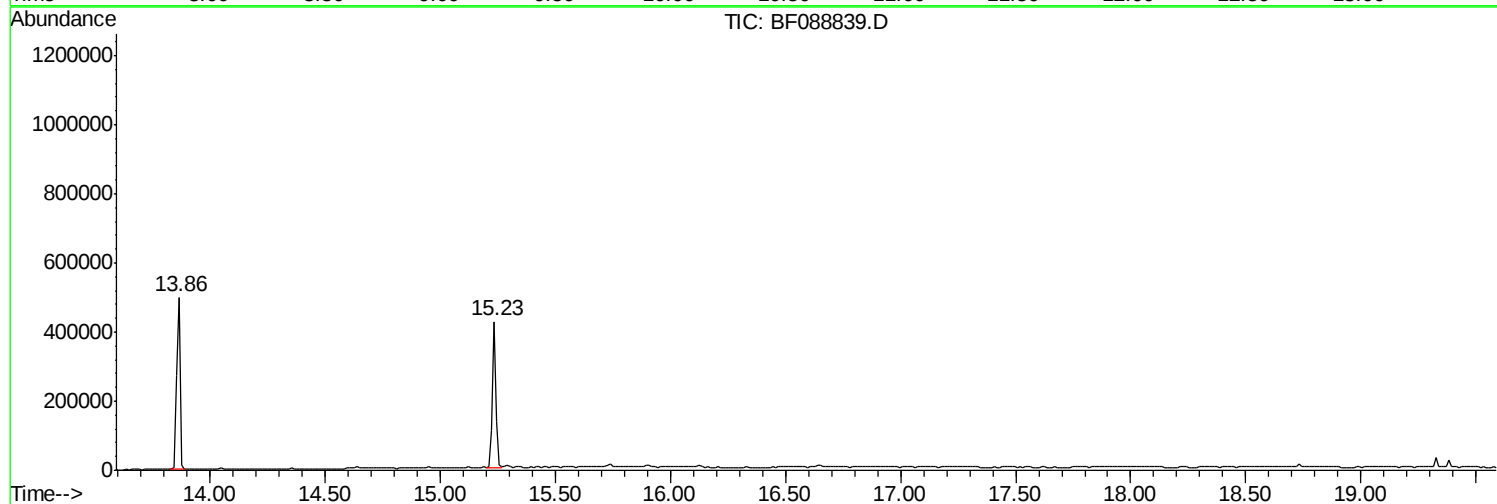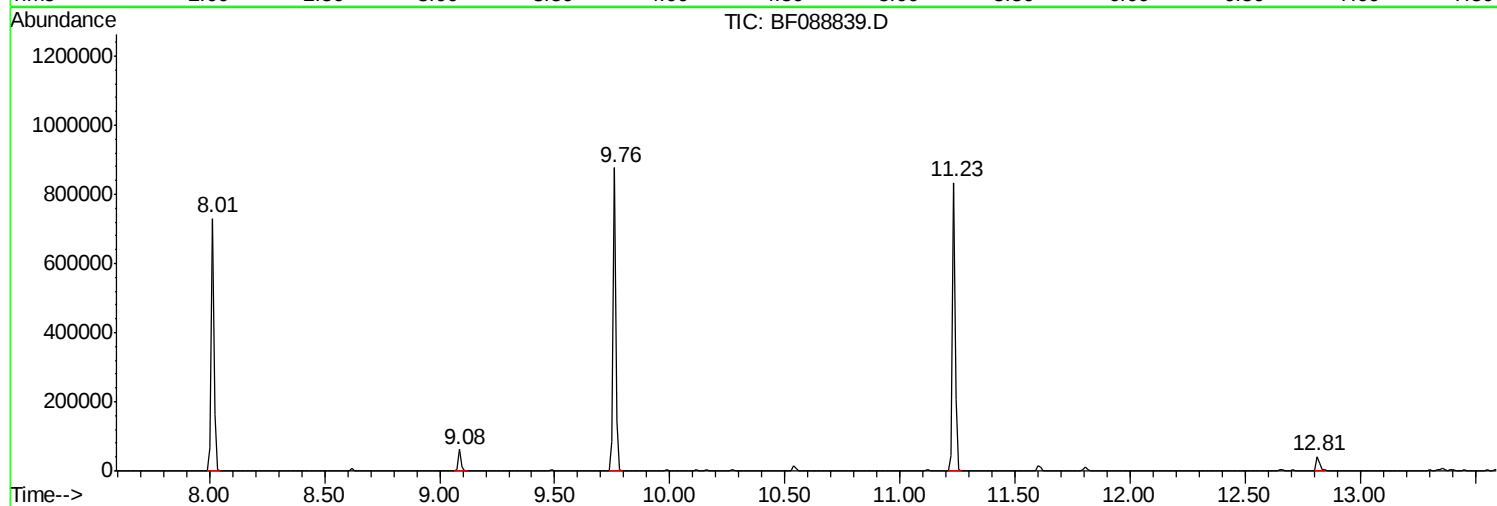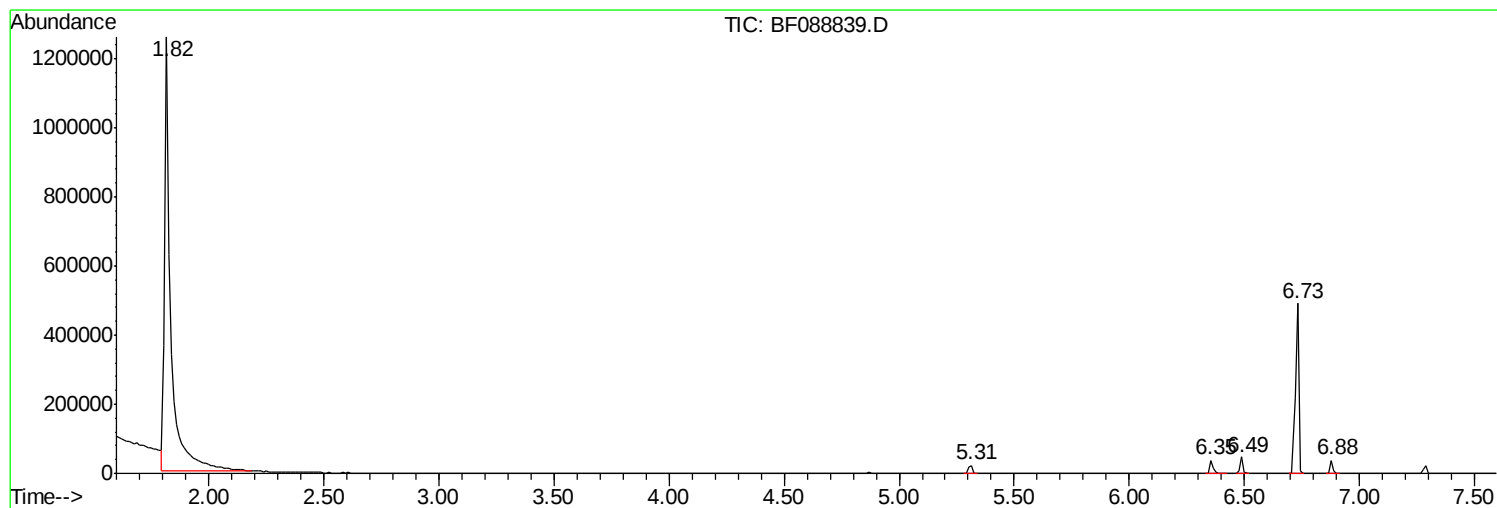

Data_Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data_File : BF088839.D
Acq_On : 8_Jul_2016 22:211
Operator : UM/SJJ
Sample : H3813-09_50XX
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
