

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
 Data File : BF088846.D
 Acq On : 9 Jul 2016 1:45
 Operator : UM/SJ
 Sample : H3813-16 50X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS004-0006-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.815	18	20	64	rVB	1449903	2975570	100.00%	42.900%
2	5.313	323	326	328	rBV	21513	30152	1.01%	0.435%
3	6.353	416	417	419	rBV	35118	34924	1.17%	0.504%
4	6.490	427	429	431	rBV	46691	36533	1.23%	0.527%
5	6.730	448	450	452	rBV	586977	531286	17.85%	7.660%
6	8.010	560	562	565	rBV	696975	669657	22.51%	9.655%
7	8.719	621	624	625	rBB	31085	33212	1.12%	0.479%
8	9.085	654	656	659	rBV	50627	46761	1.57%	0.674%
9	9.759	713	715	718	rBV	804382	746527	25.09%	10.763%
10	11.234	842	844	847	rBV2	669419	708711	23.82%	10.218%
11	12.822	981	983	985	rBV3	30623	41893	1.41%	0.604%
12	13.862	1071	1074	1076	rBV	540214	549067	18.45%	7.916%
13	14.514	1129	1131	1133	rBV2	56819	123159	4.14%	1.776%
14	15.245	1192	1195	1197	rBV	307948	408612	13.73%	5.891%


Sum of corrected areas: 6936064

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088846.D
Acq On : 9 Jul 2016 1:45
Operator : UM/SJ
Sample : H3813-16 50X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS004-0006-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

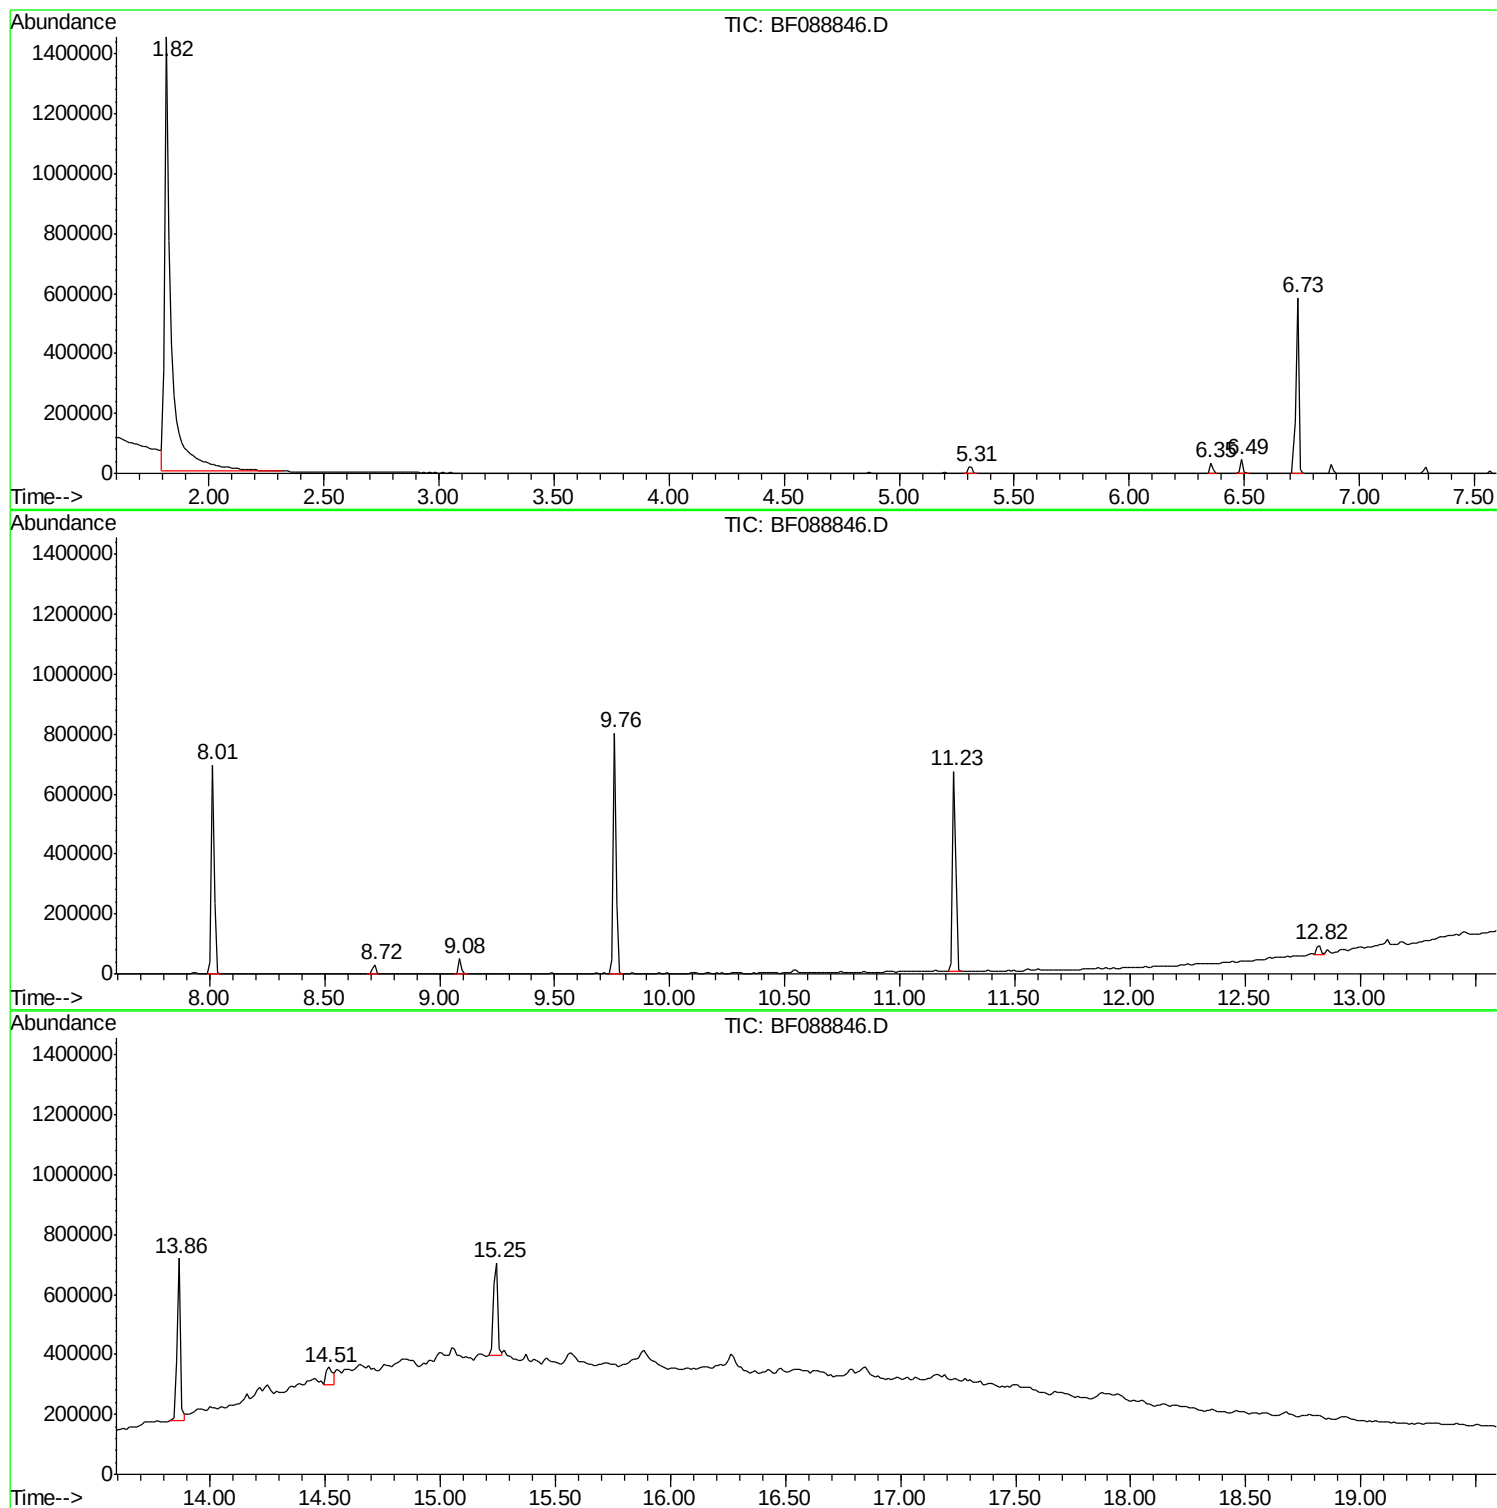

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088846.D
Acq On : 9 Jul 2016 1:45
Operator : UM/SJ
Sample : H3813-16 50X
Misc :
ALS Vial : 26 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
P001-SS004-0006-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Dodecane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.	
14.51	4.49 ng	123159	Chrysene-d12	13.86	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Dodecane	170	C12H26	000112-40-3	62
2	Tetratetracontane	619	C44H90	007098-22-8	58
3	Nonadecane, 1-bromo-	346	C19H39Br	004434-66-6	58
4	Hexadecane	226	C16H34	000544-76-3	52
5	Eicosane, 7-hexyl-	366	C26H54	055333-99-8	52

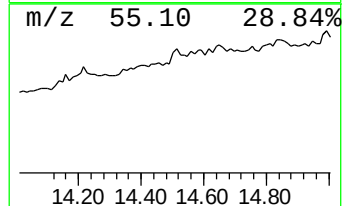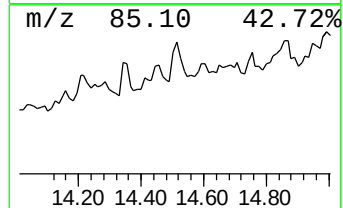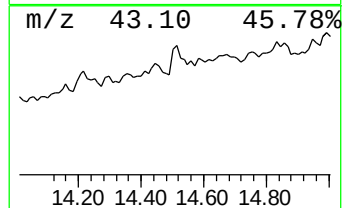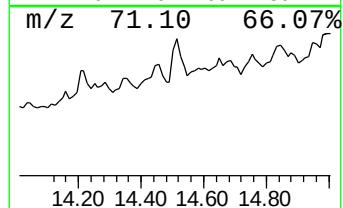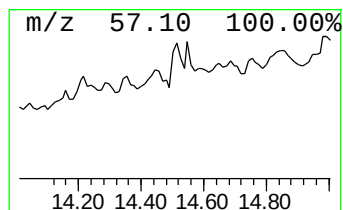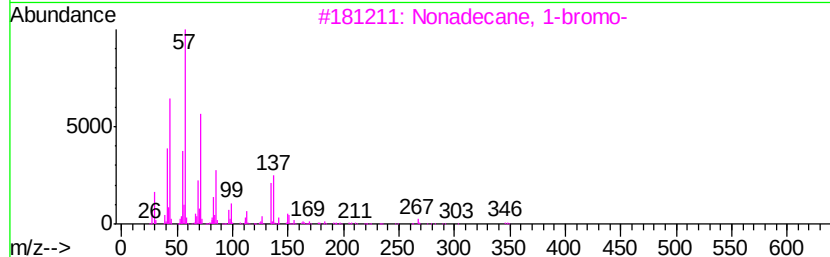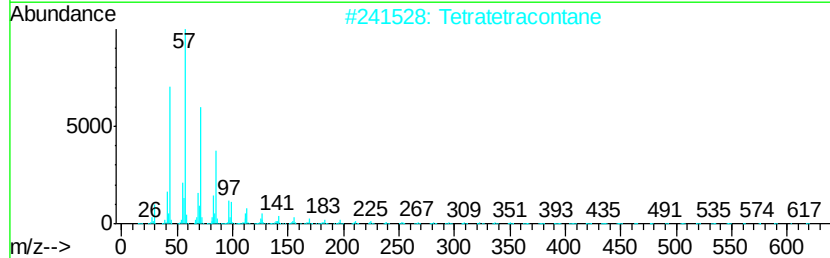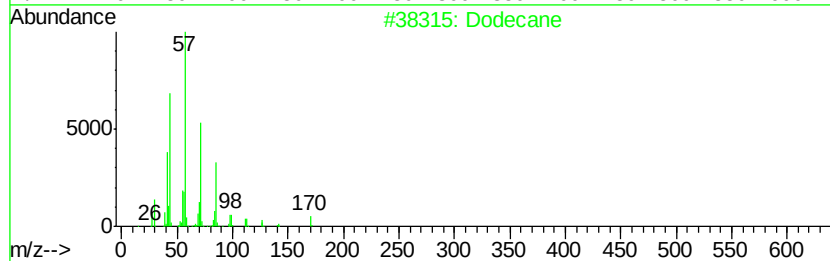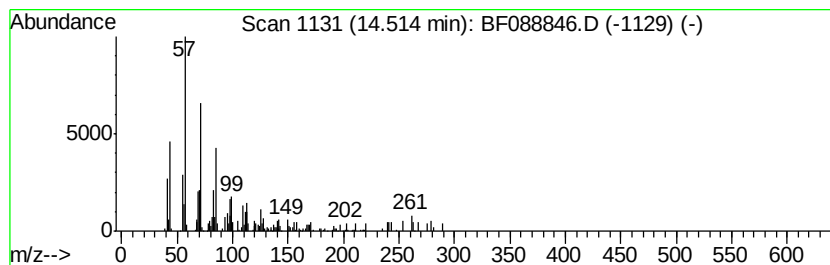

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088846.D
Acq On : 9 Jul 2016 1:45
Operator : UM/SJ
Sample : H3813-16 50X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS004-0006-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dodecane	14.51	4.5	ng	123159	5	13.86	549067	20.0