

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
 Data File : BF088847.D
 Acq On : 9 Jul 2016 2:14
 Operator : UM/SJ
 Sample : H3813-17 50X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS005-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.815	18	20	60	rVB	1242471	2448122	100.00%	40.434%
2	5.313	324	326	328	rBV	19792	25638	1.05%	0.423%
3	6.353	416	417	421	rBB	31820	35893	1.47%	0.593%
4	6.490	427	429	431	rBB	43910	34997	1.43%	0.578%
5	6.730	448	450	452	rBV	517069	472209	19.29%	7.799%
6	6.879	462	463	465	rBB	29589	26644	1.09%	0.440%
7	8.010	560	562	565	rBV	641627	606671	24.78%	10.020%
8	9.085	654	656	659	rBB	40450	36166	1.48%	0.597%
9	9.759	713	715	718	rBV	766657	701882	28.67%	11.593%
10	11.234	842	844	847	rVB	686217	668458	27.30%	11.041%
11	12.811	981	982	985	rBV3	21346	27121	1.11%	0.448%
12	13.862	1071	1074	1076	rBV	484012	488215	19.94%	8.064%
13	15.234	1192	1194	1197	rBV	340179	447455	18.28%	7.390%
14	15.291	1197	1199	1204	rVB4	19102	35081	1.43%	0.579%


Sum of corrected areas: 6054552

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088847.D
Acq On : 9 Jul 2016 2:14
Operator : UM/SJ
Sample : H3813-17 50X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS005-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

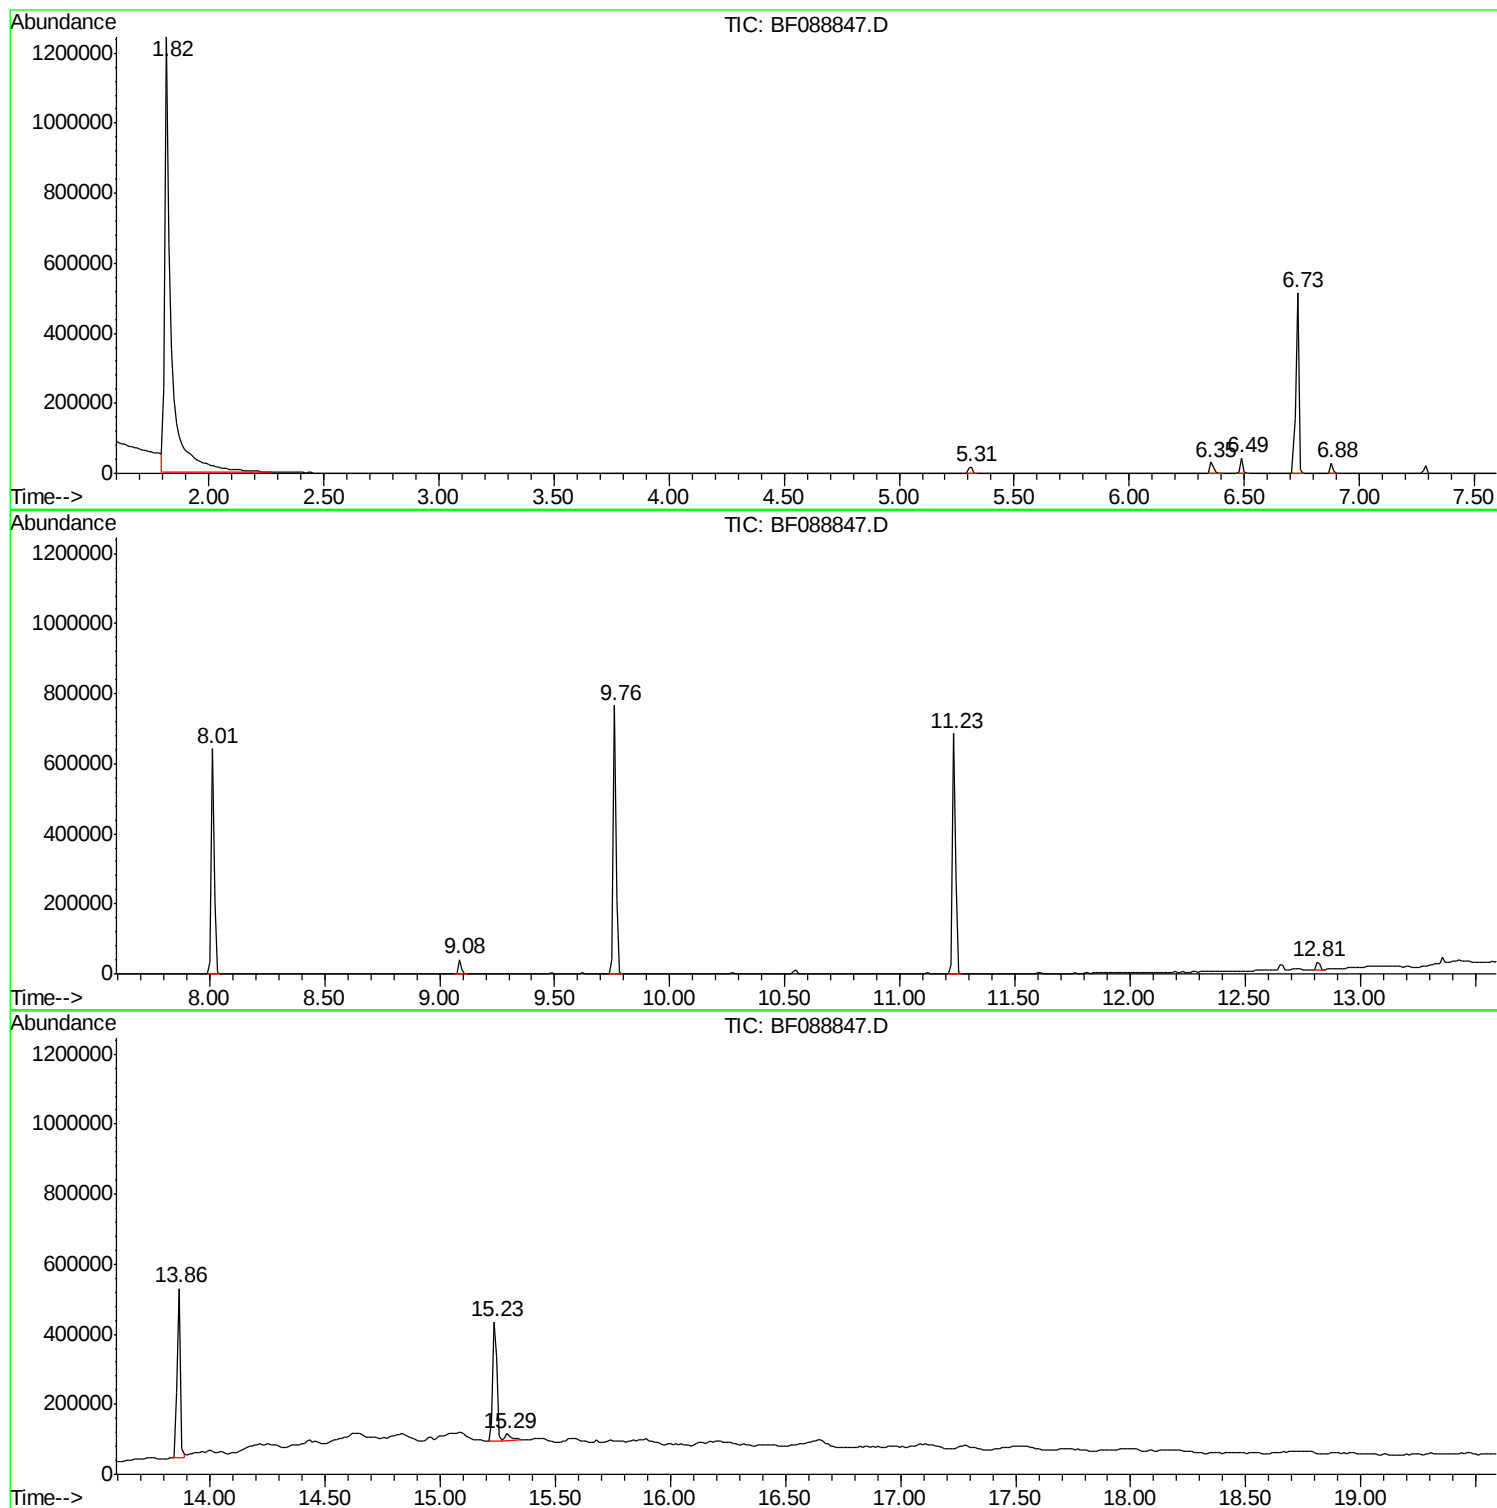

Data_Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data_File : BF088847.D
Acq_On : 9 Jul 2016 2:144
Operator : UM/SJJ
Sample : H3813-17.50XX
Misc :
ALS_Vial : 27 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
P001-SS005-0006-01

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
