

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088852.D
Acq On : 9 Jul 2016 4:39
Operator : UM/SJ
Sample : H3813-26 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-WW002-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.815	18	20	61	rVB	1125578	2317088	100.00%	41.263%
2	6.490	427	429	431	rBV	29996	24876	1.07%	0.443%
3	6.730	448	450	452	rBV	465325	457214	19.73%	8.142%
4	6.879	461	463	465	rBB	33046	28797	1.24%	0.513%
5	8.010	560	562	565	rBV	663583	595755	25.71%	10.609%
6	9.085	654	656	659	rBV	54775	47803	2.06%	0.851%
7	9.759	713	715	718	rBV	758445	664740	28.69%	11.838%
8	11.234	842	844	847	rBV	705825	632571	27.30%	11.265%
9	12.811	981	982	984	rBB	27002	32294	1.39%	0.575%
10	13.862	1071	1074	1076	rBV	364399	417813	18.03%	7.440%
11	15.234	1191	1194	1197	rBV	350950	396473	17.11%	7.060%


Sum of corrected areas: 5615424

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data File : BF088852.D
Acq On : 9 Jul 2016 4:39
Operator : UM/SJ
Sample : H3813-26 50X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-WW002-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

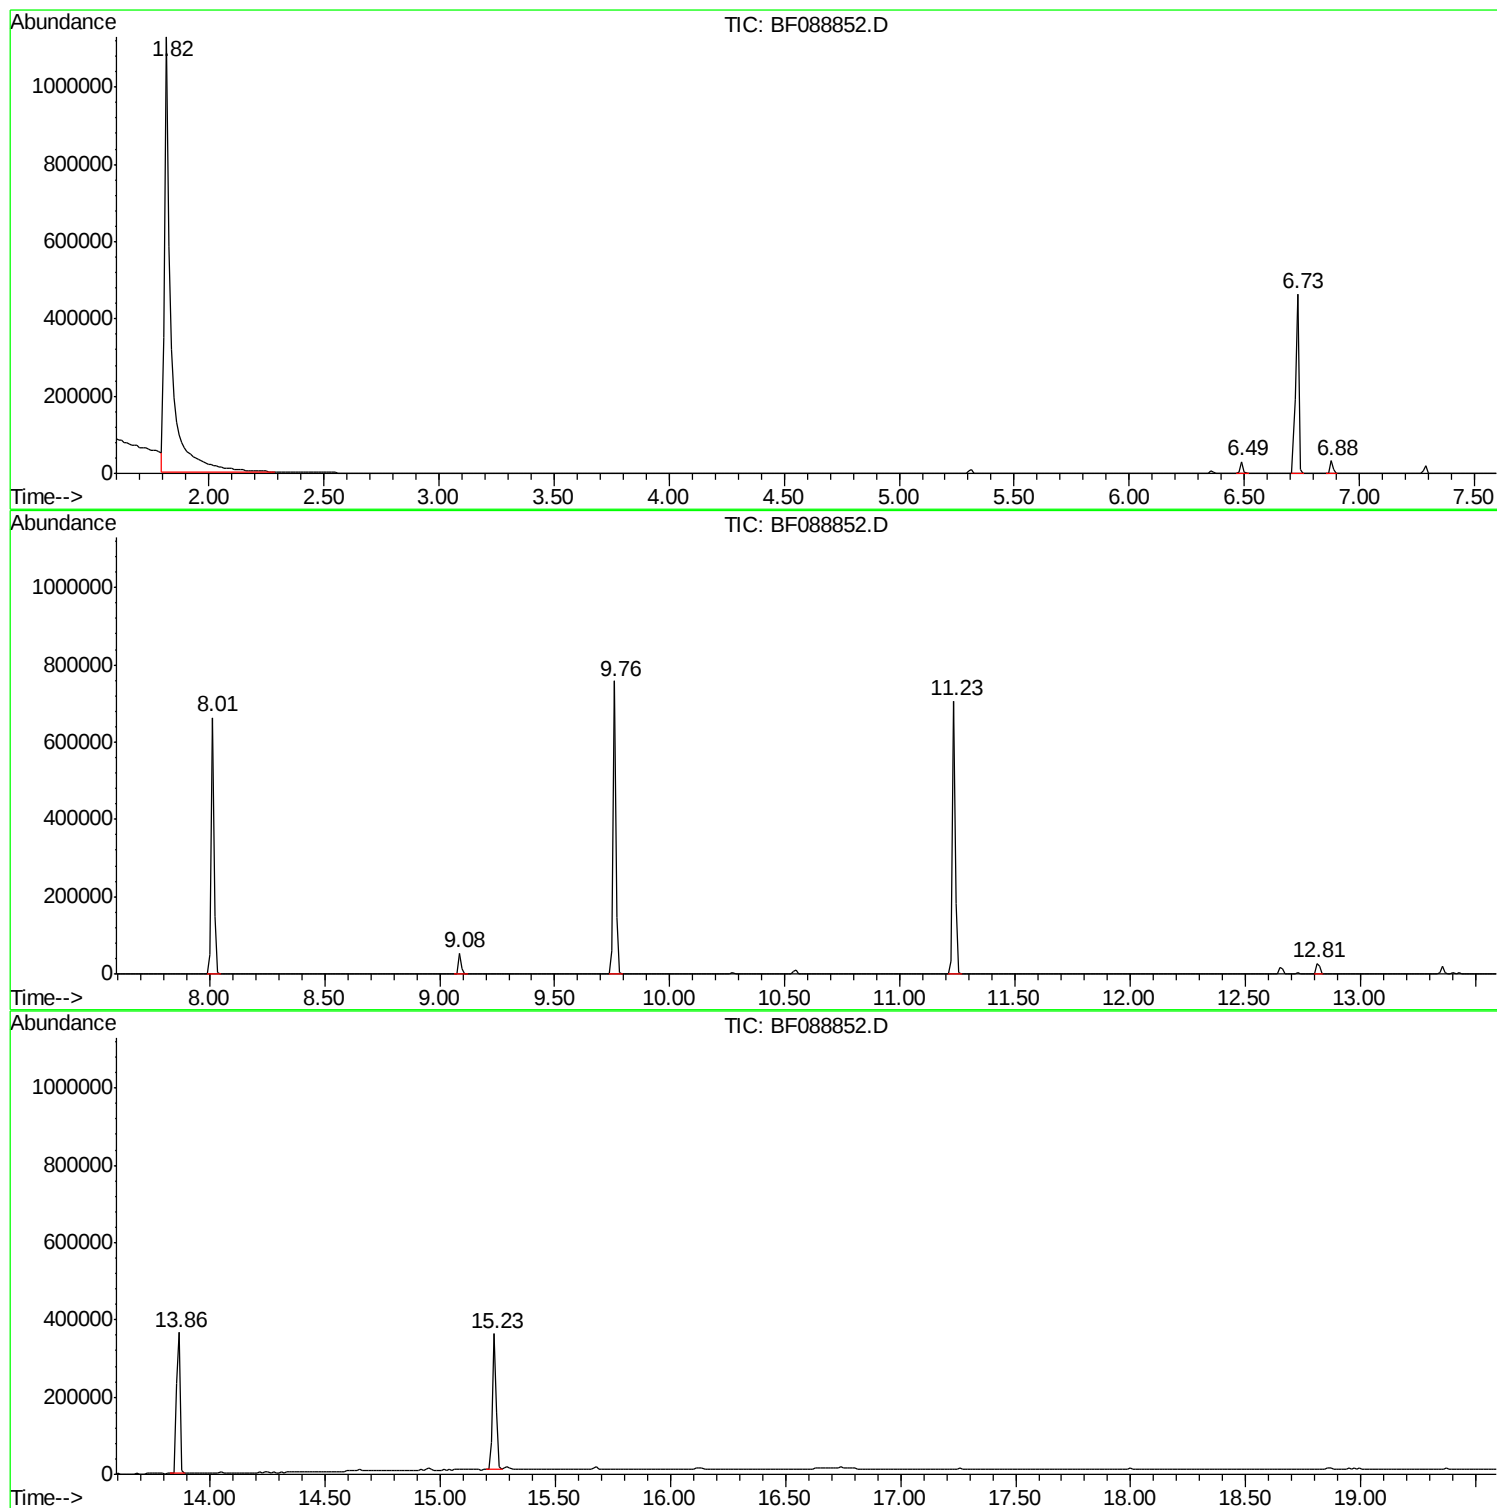

Data_Path : V:\HPCHEM1\BNA_F\DATA\BF070816\
Data_File : BF088852.D
Acq_On : 9_Jul_2016 4:399
Operator : UM/SJJ
Sample : H3813-26_50XX
Misc :
ALS_Vial : 32 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
P001-WW002-01

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
