
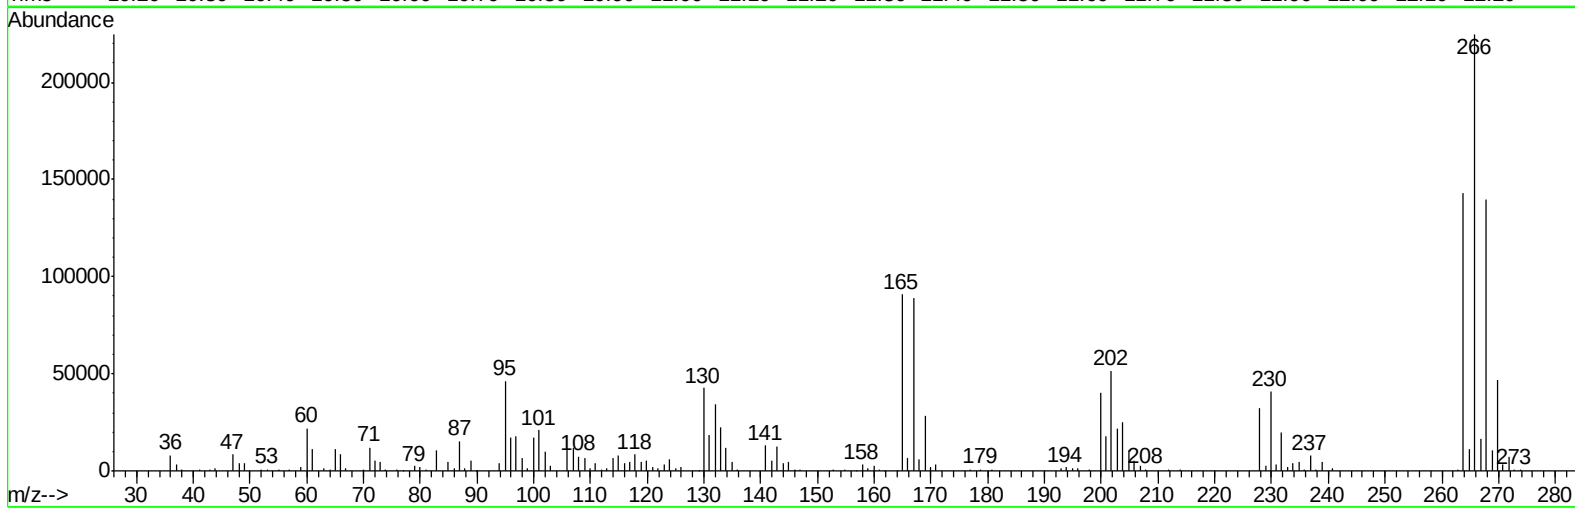


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070819\
Data File : BF115410.D
Acq On : 8 Jul 2019 17:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 01:26:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 14:57:35 2019
Response via : Initial Calibration

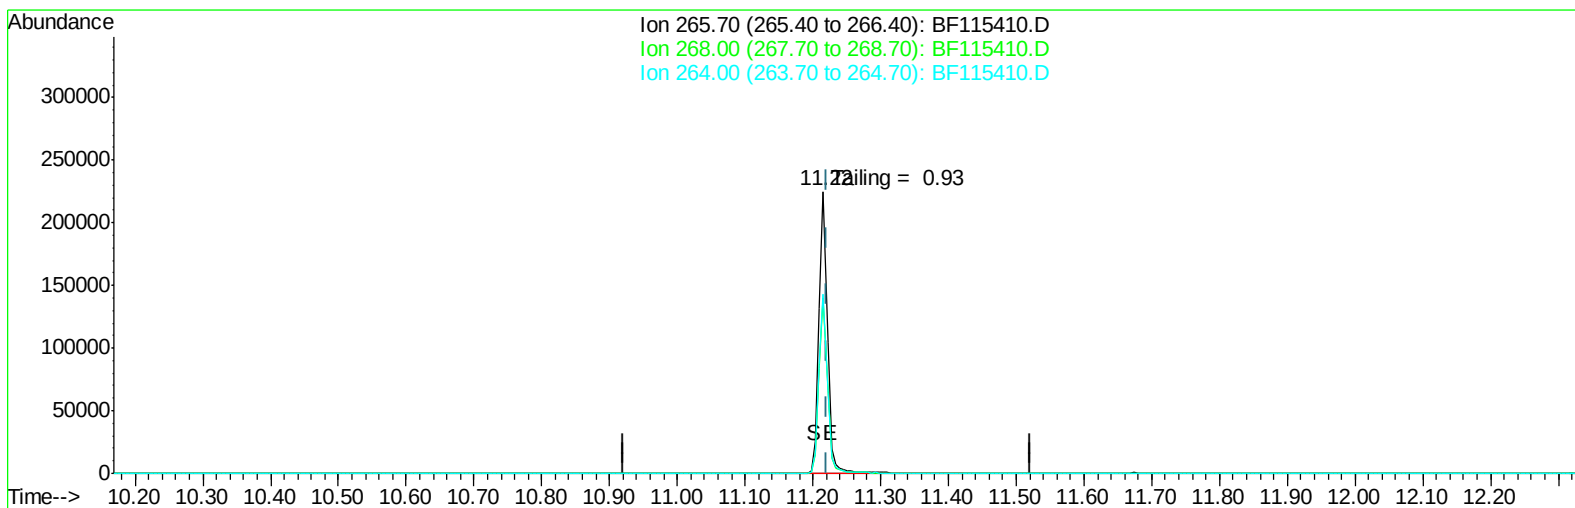

TIC: BF115410.D

(70) Pentachlorophenol (C)



11.216min (-0.006) 43130.43ng

response 189969

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	62.15
264.00	64.50	63.74
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070819\
Data File : BF115410.D
Acq On : 8 Jul 2019 17:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 01:26:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 14:57:35 2019
Response via : Initial Calibration

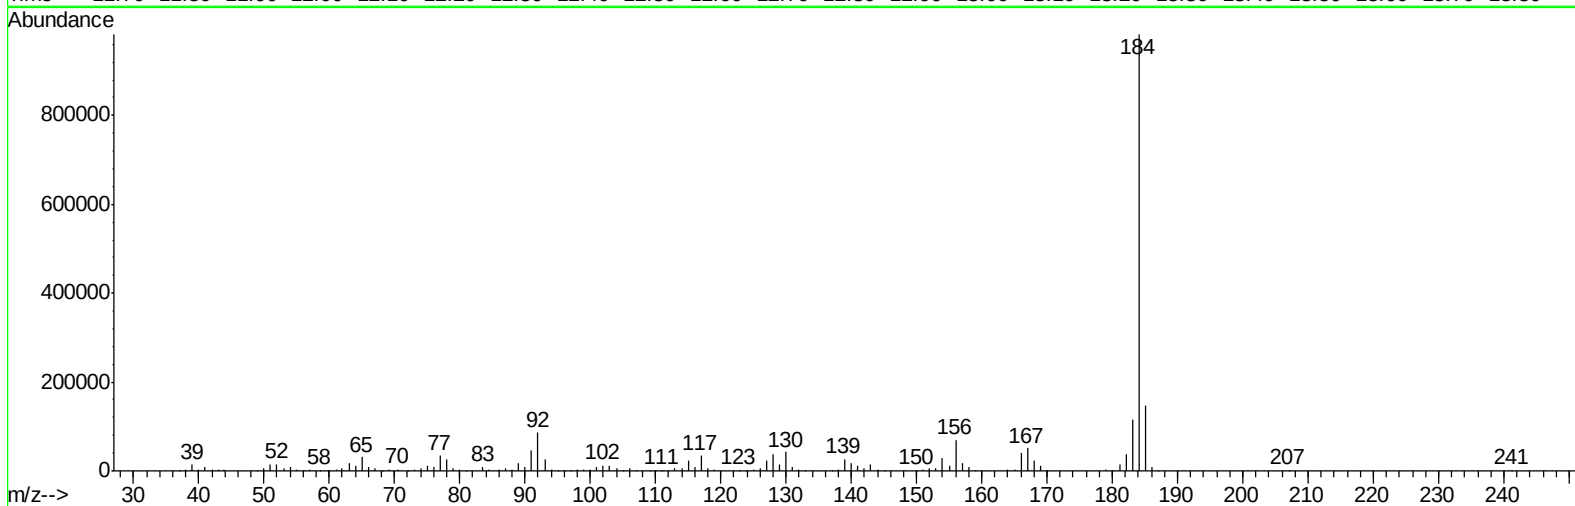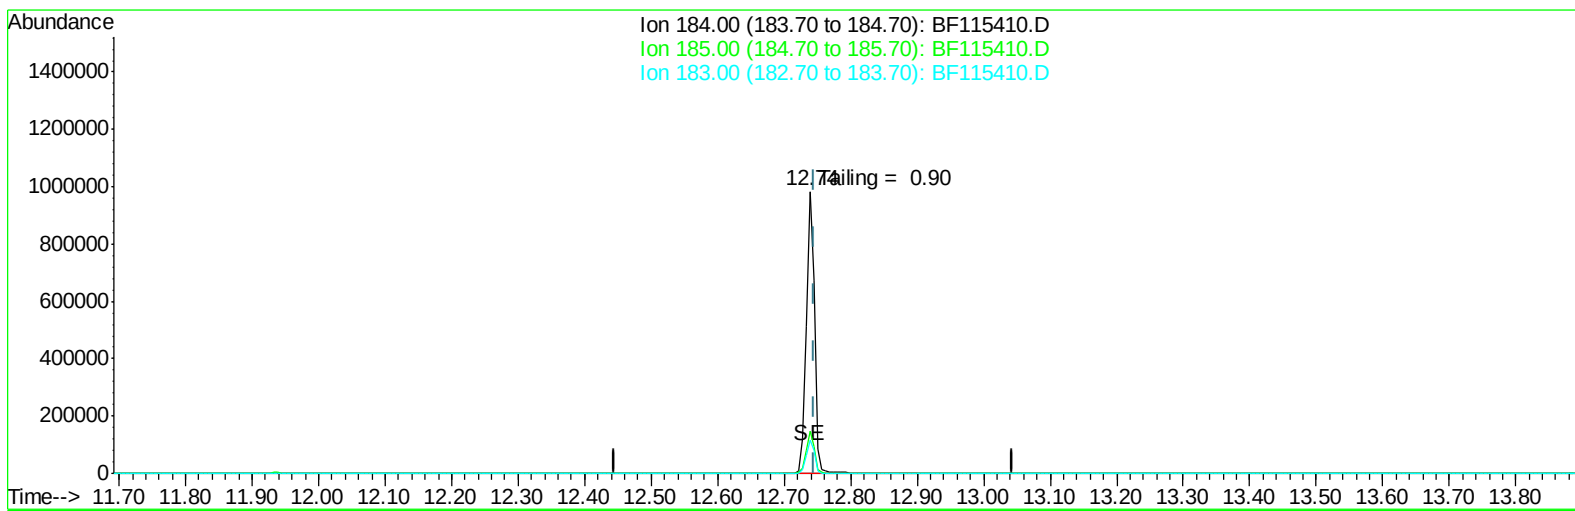

TIC: BF115410.D

(77) Benzidine

12.739min (-0.006) 0.00ng

response 864718

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.08
183.00	11.70	11.80
0.00	0.00	0.00