


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070819\
Data File : BF115399.D
Acq On : 8 Jul 2019 11:17
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 05 14:57:35 2019

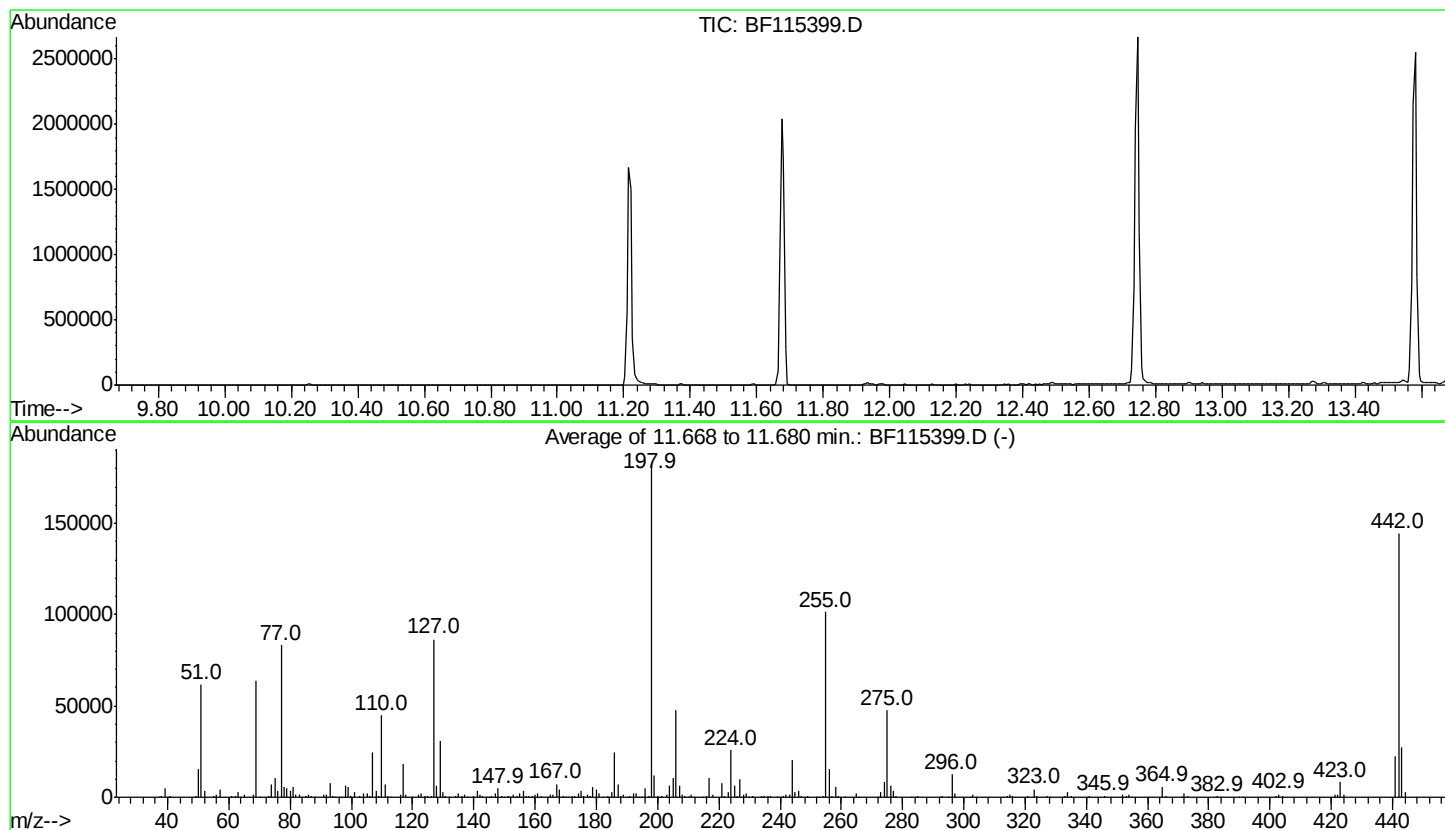

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	61578	PASS
68	69	0.00	2	1.8	1141	PASS
69	198	0.00	100	35.2	63992	PASS
70	69	0.00	2	0.5	291	PASS
127	198	10	80	47.5	86293	PASS
197	198	0.00	2	0.5	914	PASS
198	198	100	100	100.0	181653	PASS
199	198	5	9	6.6	11953	PASS
275	198	10	60	26.2	47656	PASS
365	198	1	100	3.2	5724	PASS
441	198	0.01	100	12.2	22200	PASS
442	198	50	100	79.5	144381	PASS
443	442	15	24	19.1	27557	PASS