
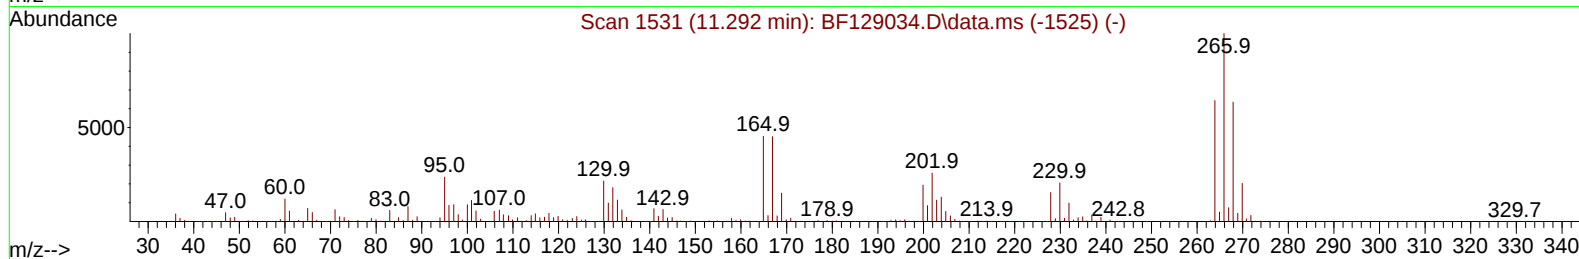
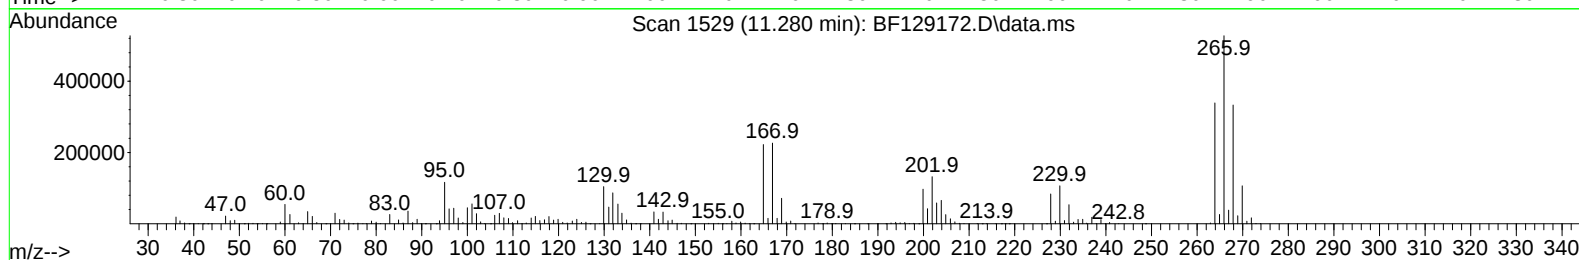


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070822\
 Data File : BF129172.D
 Acq On : 08 Jul 2022 11:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 23:22:06 2022
 Response via : Initial Calibration



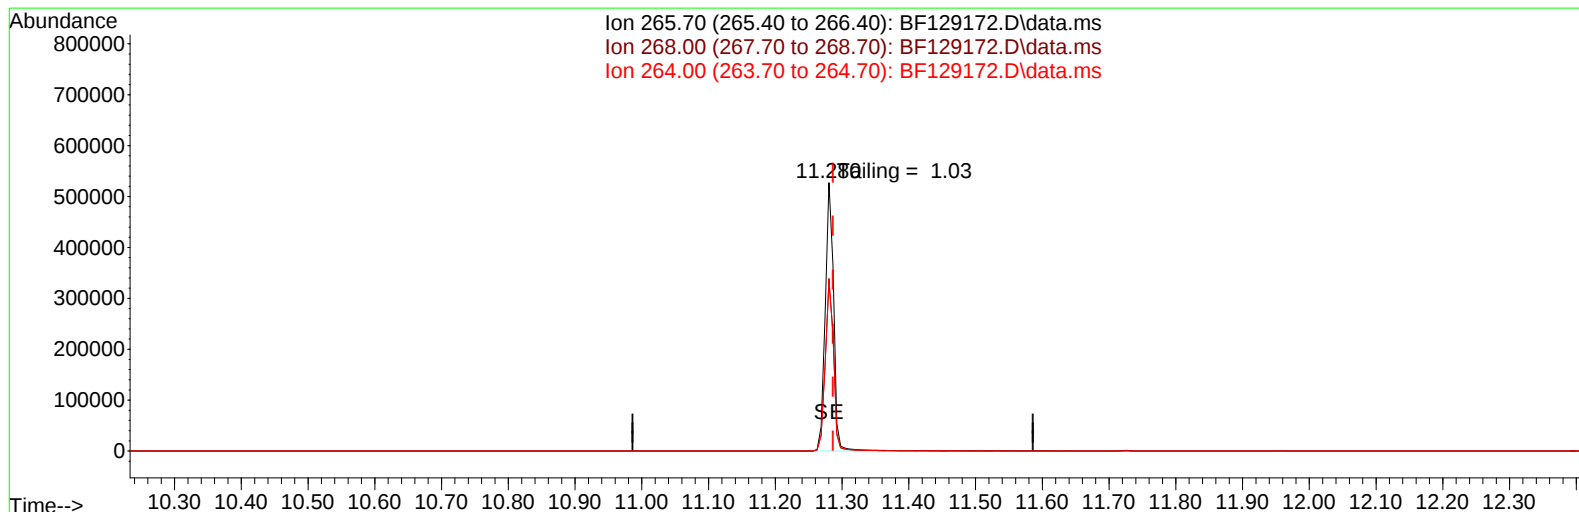


TIC: BF129172.D\data.ms

(70) Pentachlorophenol (C)**11.280min (-0.006) 433876.01 ng****response 459152**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.16
264.00	61.80	64.30
0.00	0.00	0.00

Quant Time: Jul 09 01:07:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 23:22:06 2022
Response via : Initial Calibration

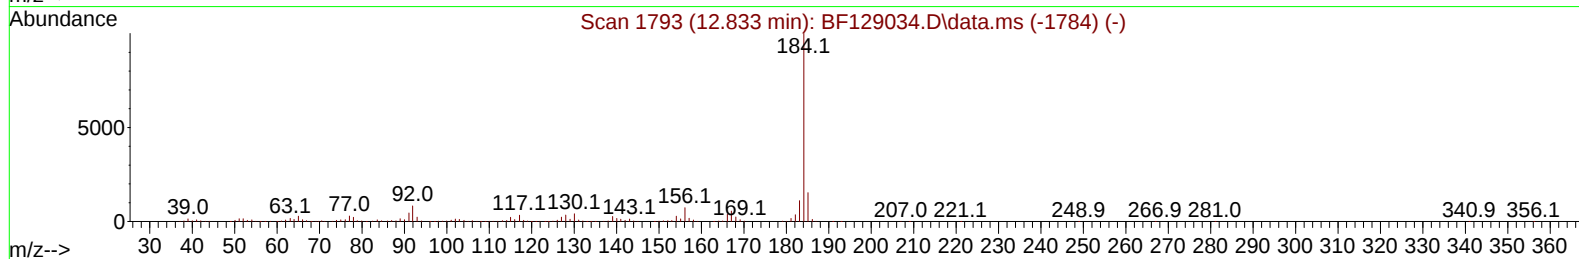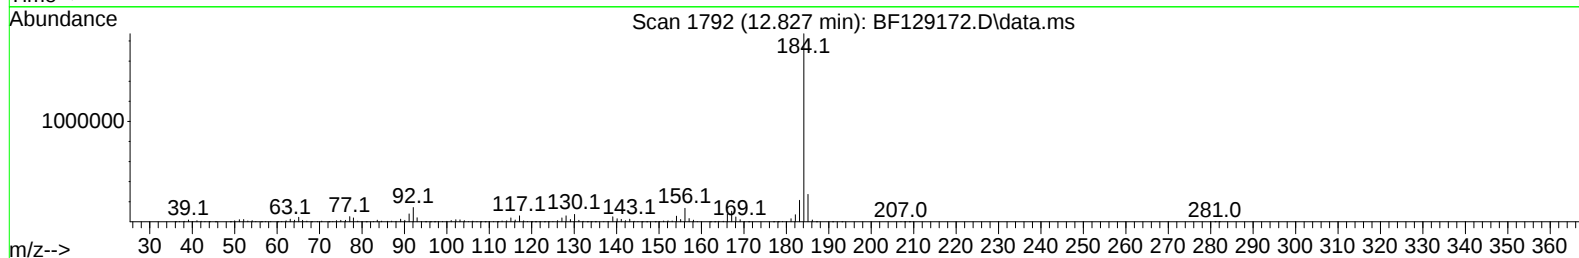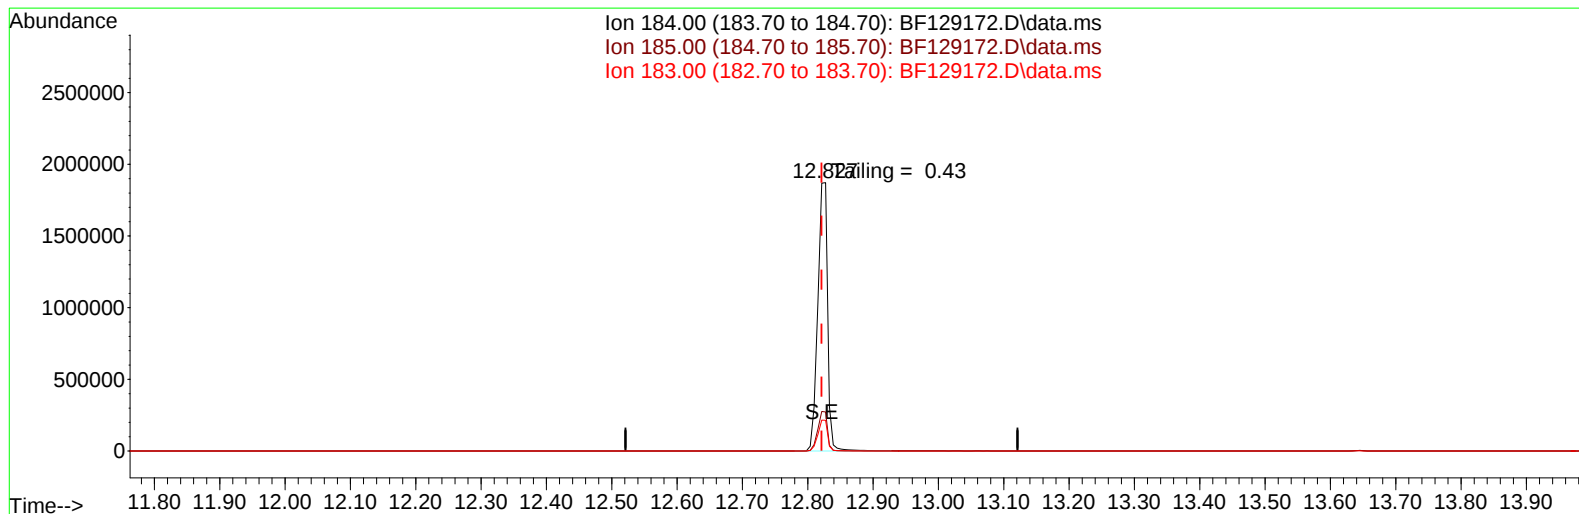

TIC: BF129172.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 45889.86 ng

response **1969284**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.57
--------	-------	-------

183.00	11.60	11.44
--------	-------	-------

0.00 0.00 0.00