
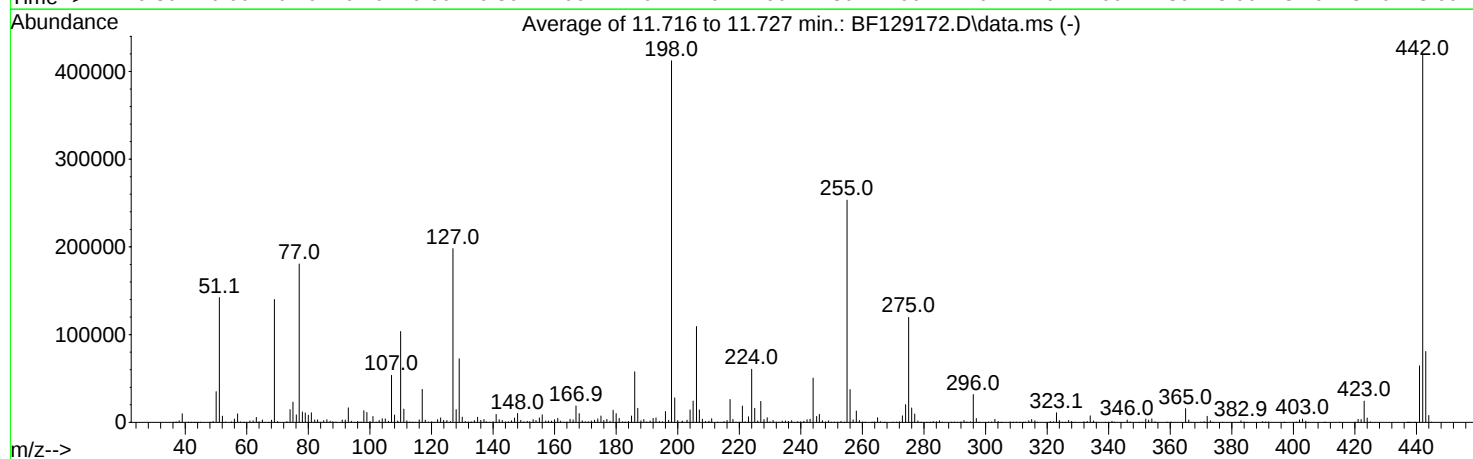


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070822\
 Data File : BF129172.D
 Acq On : 08 Jul 2022 11:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 08 23:22:06 2022

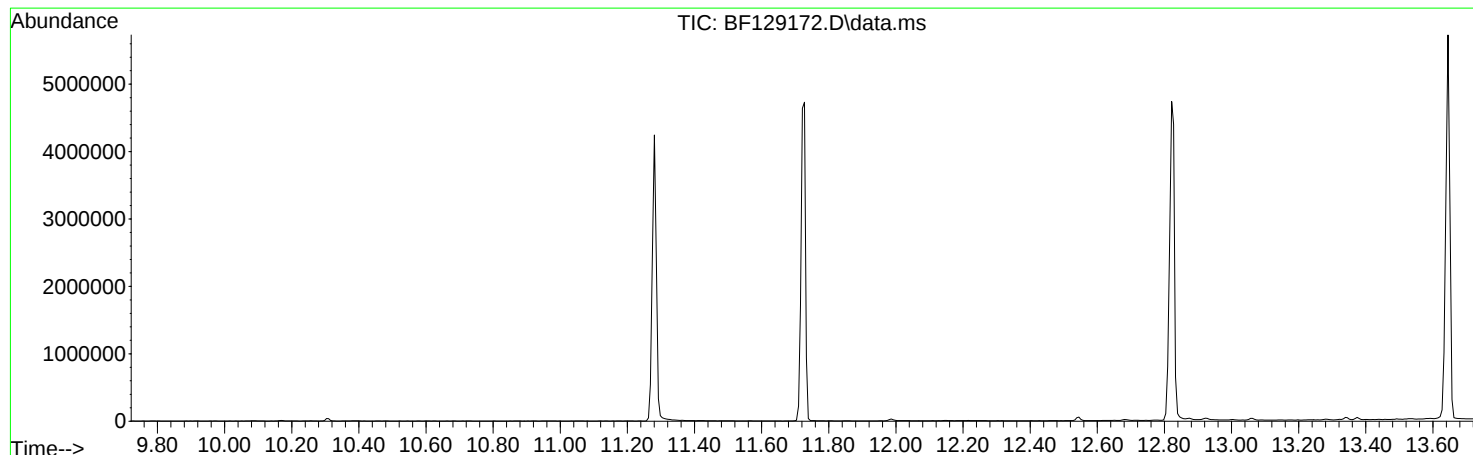




AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	142283	PASS
68	69	0.00	2	1.8	2575	PASS
69	198	0.00	100	34.0	140061	PASS
70	69	0.00	2	0.6	840	PASS
127	198	10	80	48.1	198088	PASS
197	198	0.00	2	0.6	2343	PASS
198	198	100	100	100.0	412245	PASS
199	198	5	9	6.8	27891	PASS
275	198	10	60	29.0	119651	PASS
365	198	1	100	3.8	15652	PASS
441	198	0.01	100	15.6	64331	PASS
442	442	50	100	100.0	419320	PASS
443	442	15	24	19.3	80792	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070822\
 Data File : BF129172.D
 Acq On : 08 Jul 2022 11:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 09 01:07:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 23:22:06 2022
 Response via : Initial Calibration

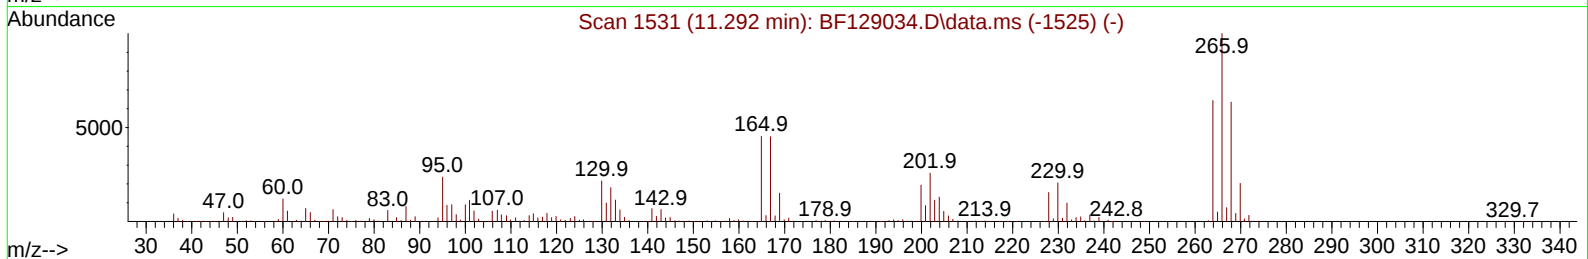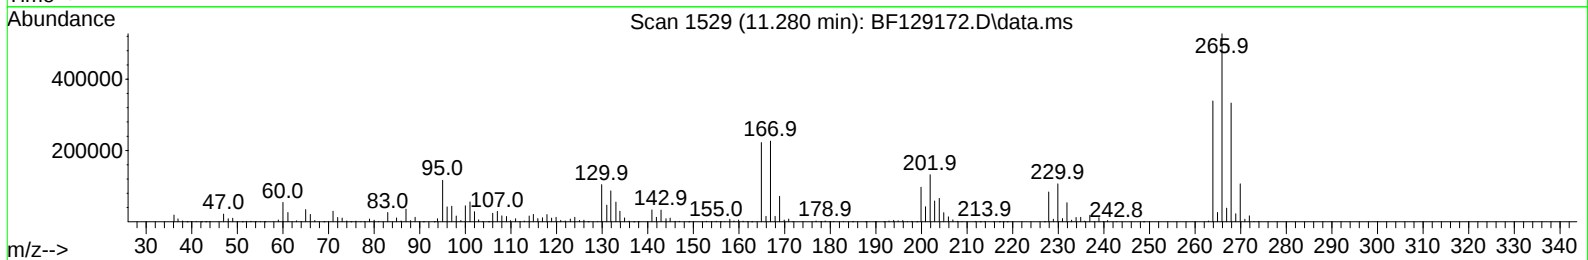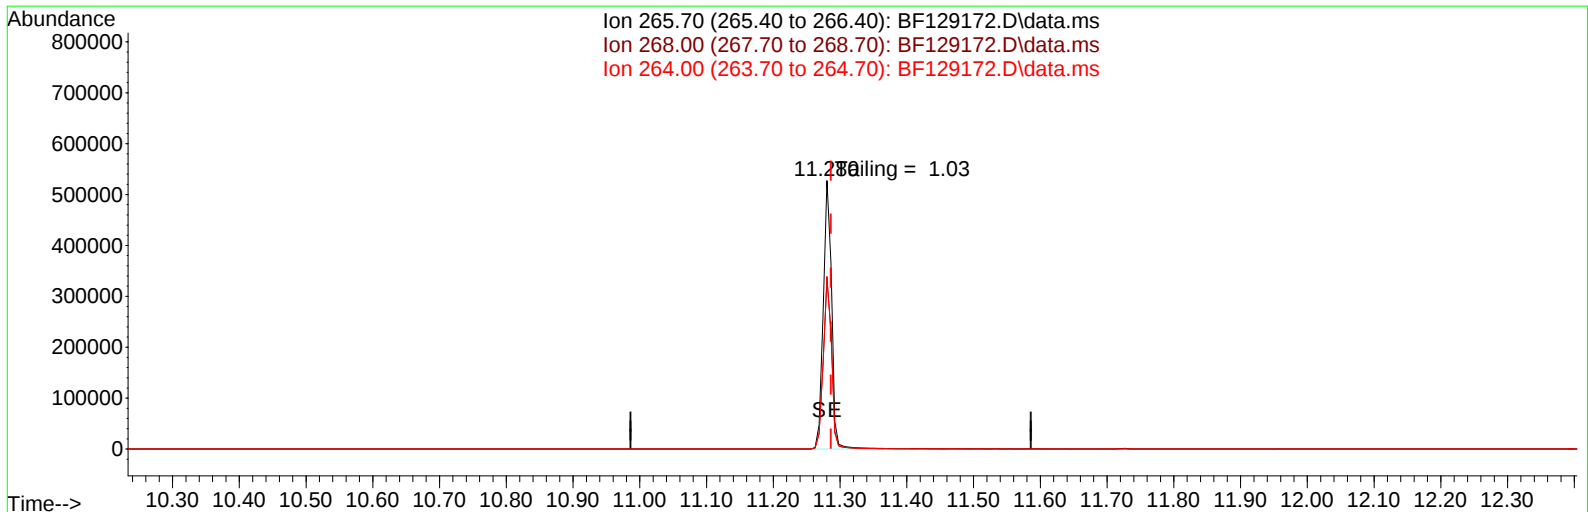

TIC: BF129172.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.006) 433876.01 ng




response 459152

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.16
264.00	61.80	64.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070822\
Data File : BF129172.D
Acq On : 08 Jul 2022 11:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 09 01:07:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 23:22:06 2022
Response via : Initial Calibration

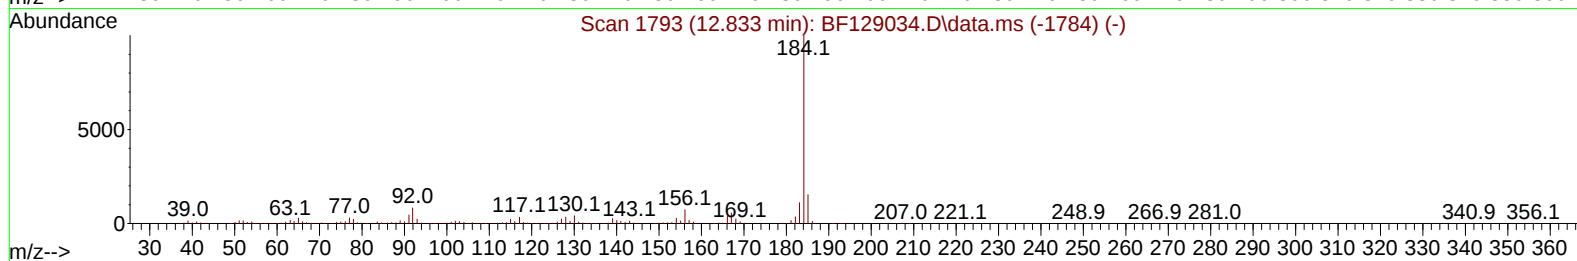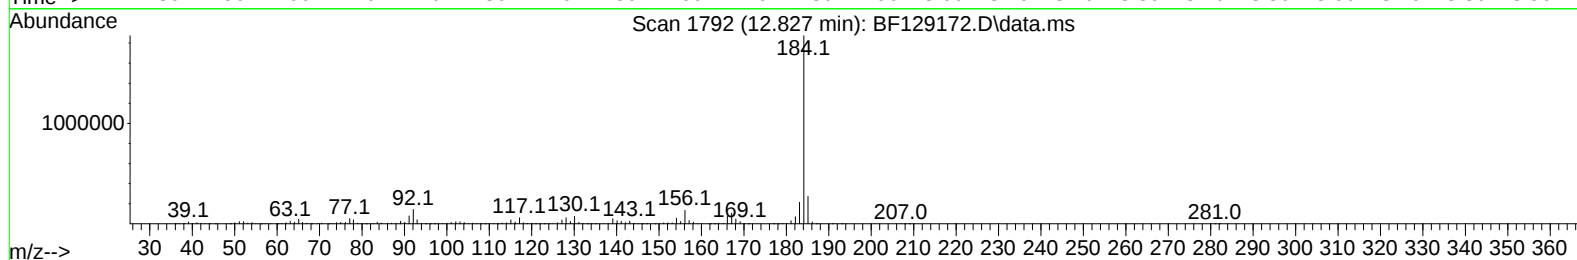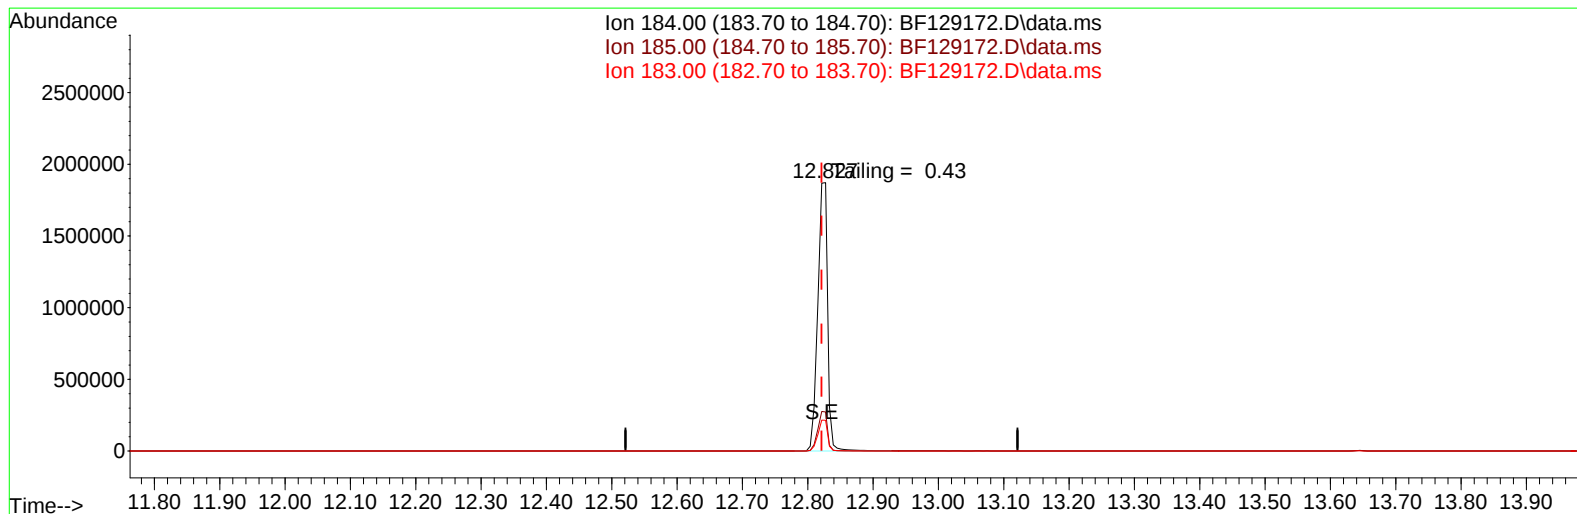

TIC: BF129172.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 45889.86 ng

response 1969284

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.57
183.00	11.60	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/8/2022	BNA_F	<u>BF129172.D</u>
Compound Name	Response	Retention Time
DDT	963843	13.645
DDD	11261	13.339
DDE	1171	13.004
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12432	976275	1.27

Instrument :
BNA_F
ClientSampleId :
DFTPP