


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070824\
Data File : BF138477.D
Acq On : 08 Jul 2024 11:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

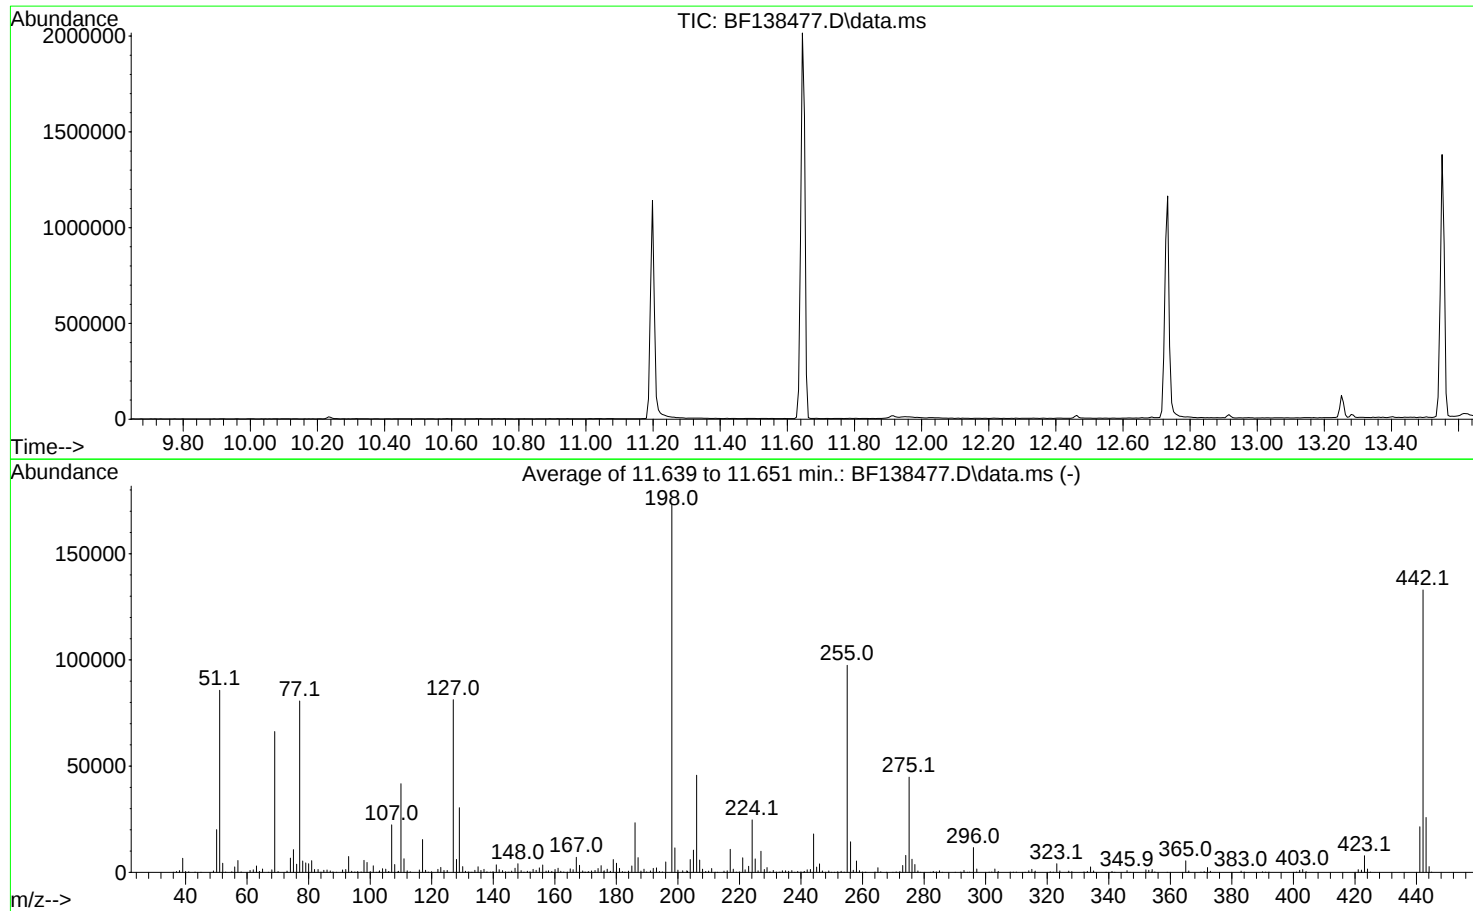

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	85707	PASS
68	69	0.00	2	1.9	1245	PASS
69	198	0.00	100	38.3	66277	PASS
70	69	0.00	2	0.6	414	PASS
127	198	10	80	46.9	81261	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	173171	PASS
199	198	5	9	6.7	11547	PASS
275	198	10	60	25.9	44803	PASS
365	198	1	100	3.1	5420	PASS
441	198	0.01	100	12.4	21468	PASS
442	442	50	100	100.0	132912	PASS
443	442	15	24	19.5	25872	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/8/2024	BNA_F	<u>BF138477.D</u>
Compound Name	Response	Retention Time
DDT	215291	13.551
DDD	21228	13.251
DDE	2118	12.915
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23346	238637	9.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070824\
Data File : BF138477.D
Acq On : 08 Jul 2024 11:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 08 12:34:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

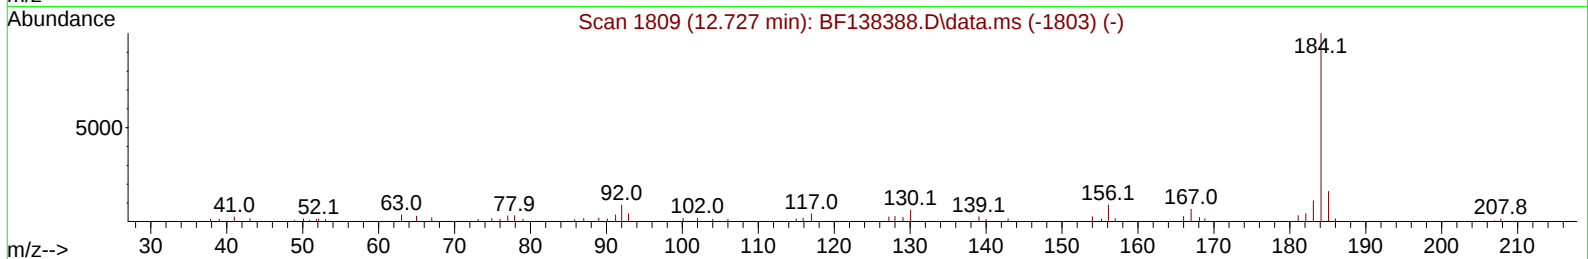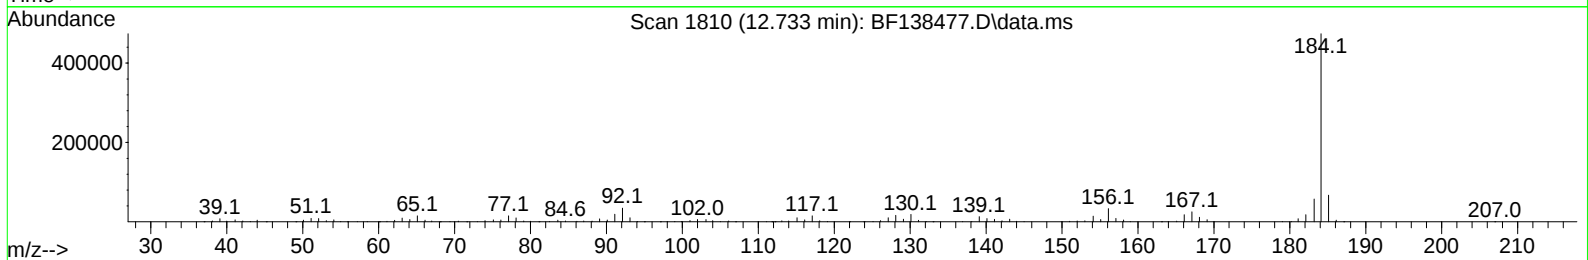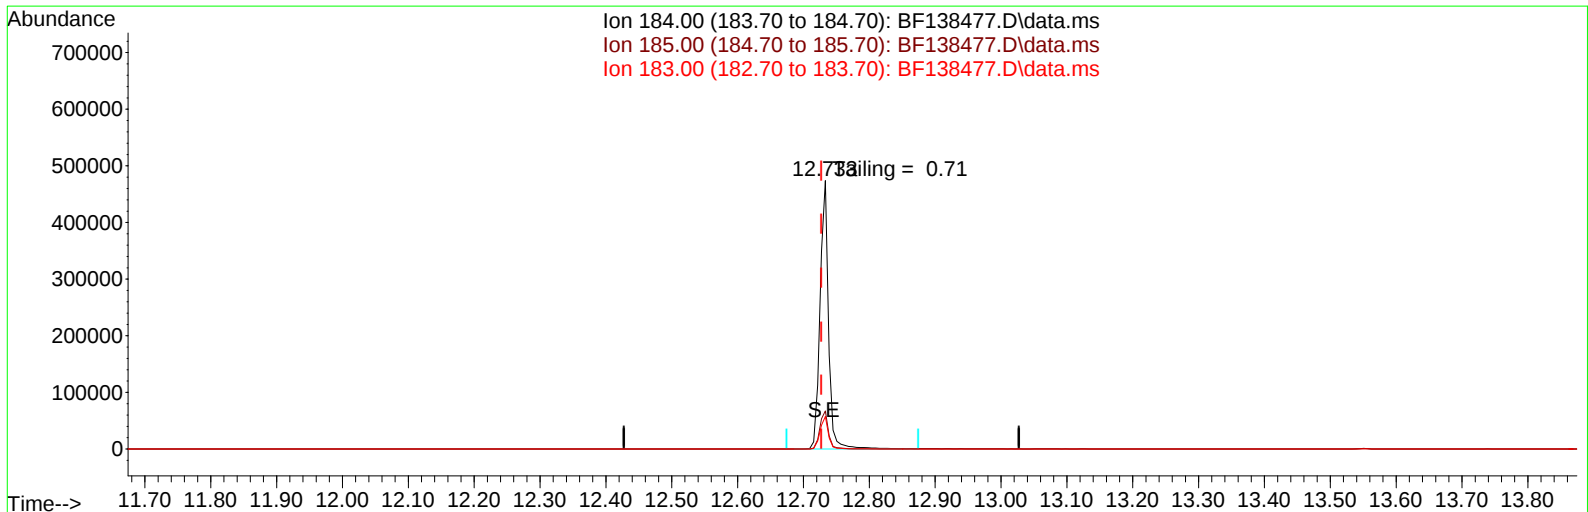

TIC: BF138477.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 427530

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.19
183.00	11.30	12.11
0.00	0.00	0.00