
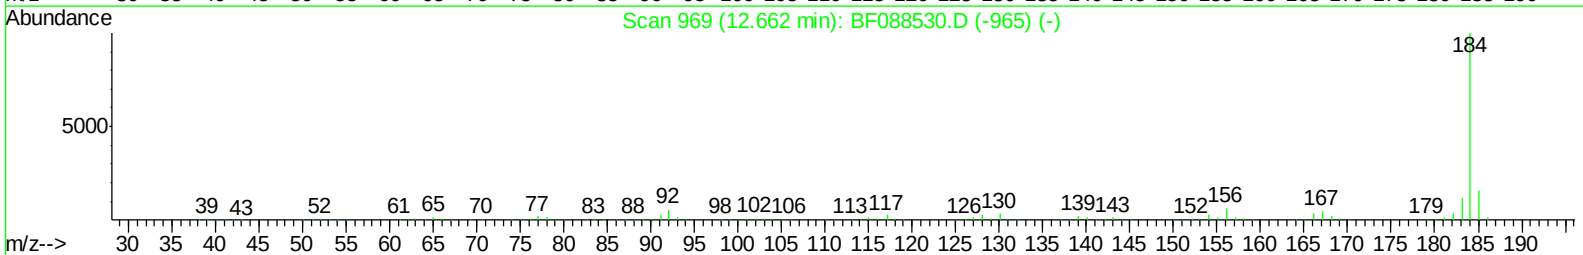
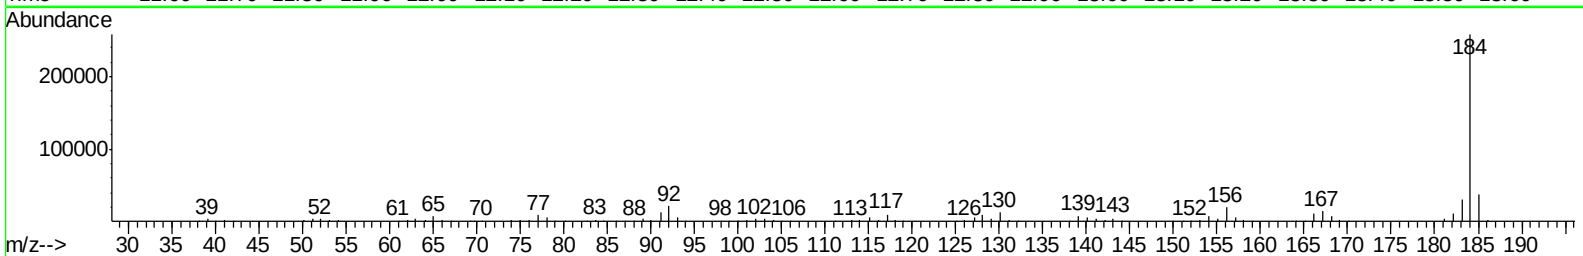


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF070916\  
Data File : BF088889.D  
Acq On : 9 Jul 2016 23:56  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 07:49:05 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF063016.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 08 18:51:20 2016  
Response via : Initial Calibration

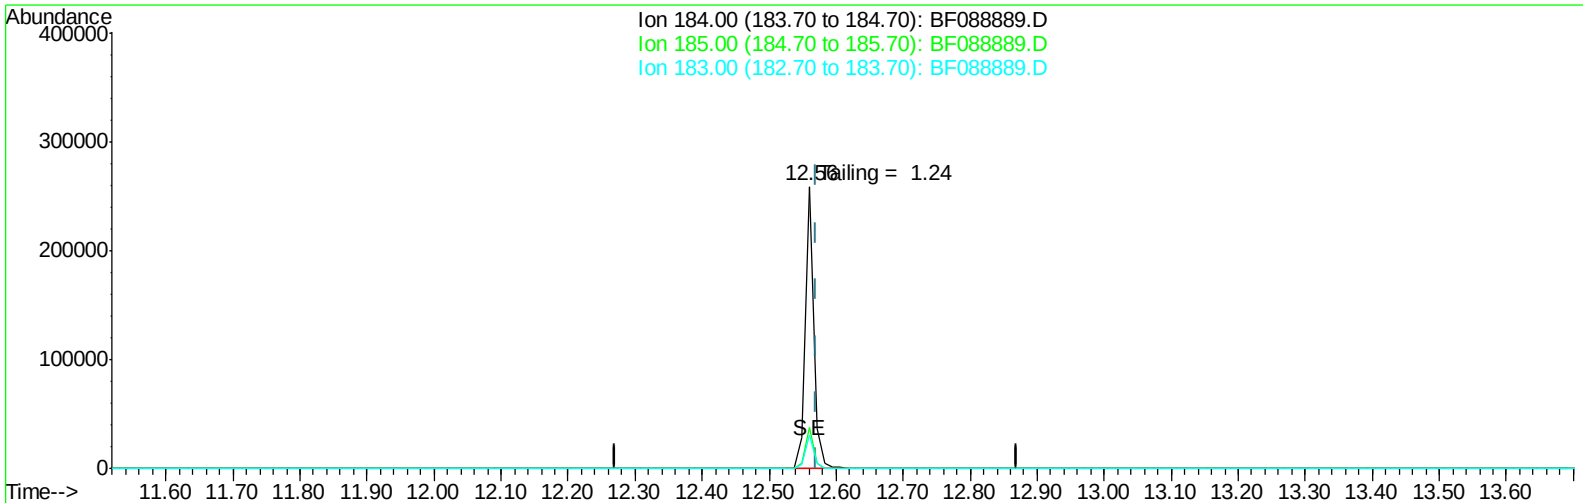

TIC: BF088889.D

(76) Benzidine




12.559min (-0.011) 0.00ng

response 228258

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.60 | 14.75 |
| 183.00 | 11.60 | 11.61 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF070916\  
Data File : BF088889.D  
Acq On : 9 Jul 2016 23:56  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 07:49:05 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF063016.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 08 18:51:20 2016  
Response via : Initial Calibration

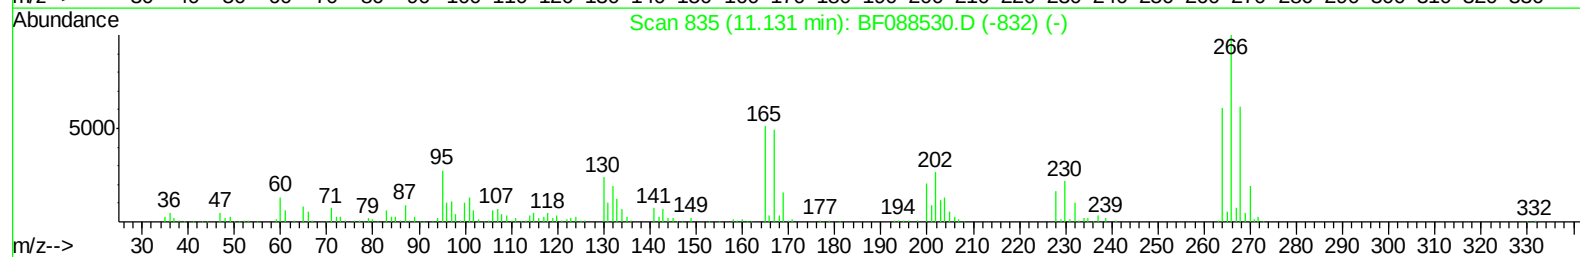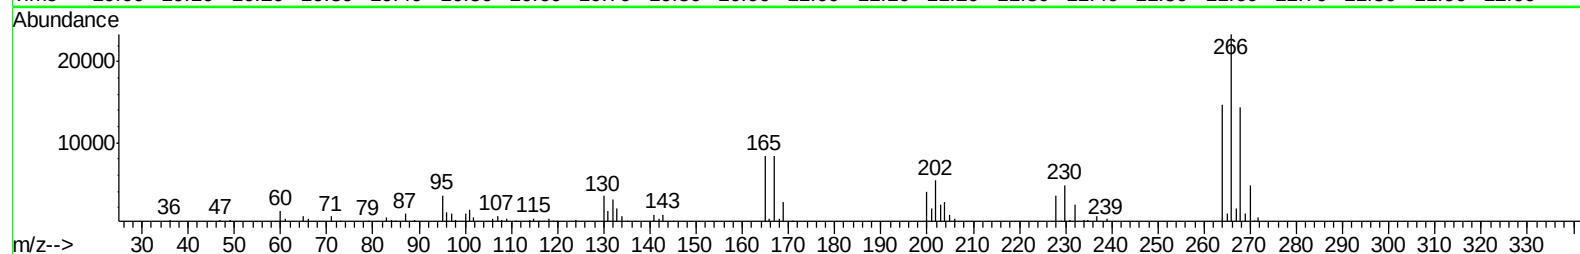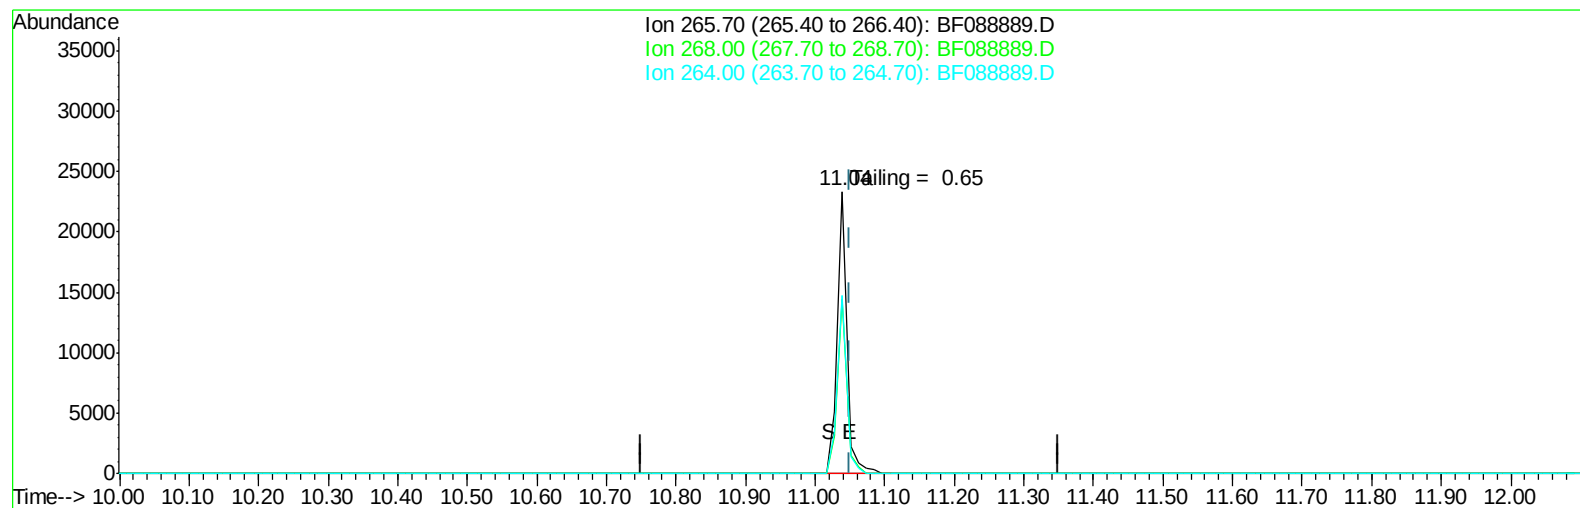

TIC: BF088889.D

(69) Pentachlorophenol (C)

11.039min (-0.011) 0.00ng

response 22096

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.00 | 61.78 |
| 264.00 | 62.00 | 63.02 |
| 0.00   | 0.00  | 0.00  |