

Data Path : V:\HPCHEM1\BNA F\DATA\BF070916\
 Data File : BF088876.D
 Acq On : 9 Jul 2016 17:37
 Operator : UM/SJ
 Sample : H3813-09 25X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-DS001-02

Quant Time: Jul 11 05:46:29 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 18:51:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	70432	20.00	ng	-0.01
21) Naphthalene-d8	8.00	136	264767	20.00	ng	-0.02
38) Acenaphthene-d10	9.75	164	131720	20.00	ng	-0.02
63) Phenanthrene-d10	11.22	188	265648	20.00	ng	-0.02
75) Chrysene-d12	13.85	240	220614	20.00	ng	-0.02
86) Perylene-d12	15.22	264	150981	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	22305	4.75	ng	-0.03
7) Phenol-d6	6.34	99	30150	4.97	ng	-0.03
23) Nitrobenzene-d5	7.28	82	18933	3.75	ng	-0.02
41) 2,4,6-Tribromophenol	10.54	330	5491	4.49	ng	-0.02
44) 2-Fluorobiphenyl	9.07	172	38614	4.63	ng	-0.02
78) Terphenyl-d14	12.81	244	41485	4.19	ng	-0.01


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : V:\HPCHEM1\BNA F\DATA\BF070916\
Data File : BF088876.D
Acq On : 9 Jul 2016 17:37
Operator : UM/SJ
Sample : H3813-09 25X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Quant Time: Jul 11 05:46:29 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 08 18:51:20 2016
Response via : Initial Calibration

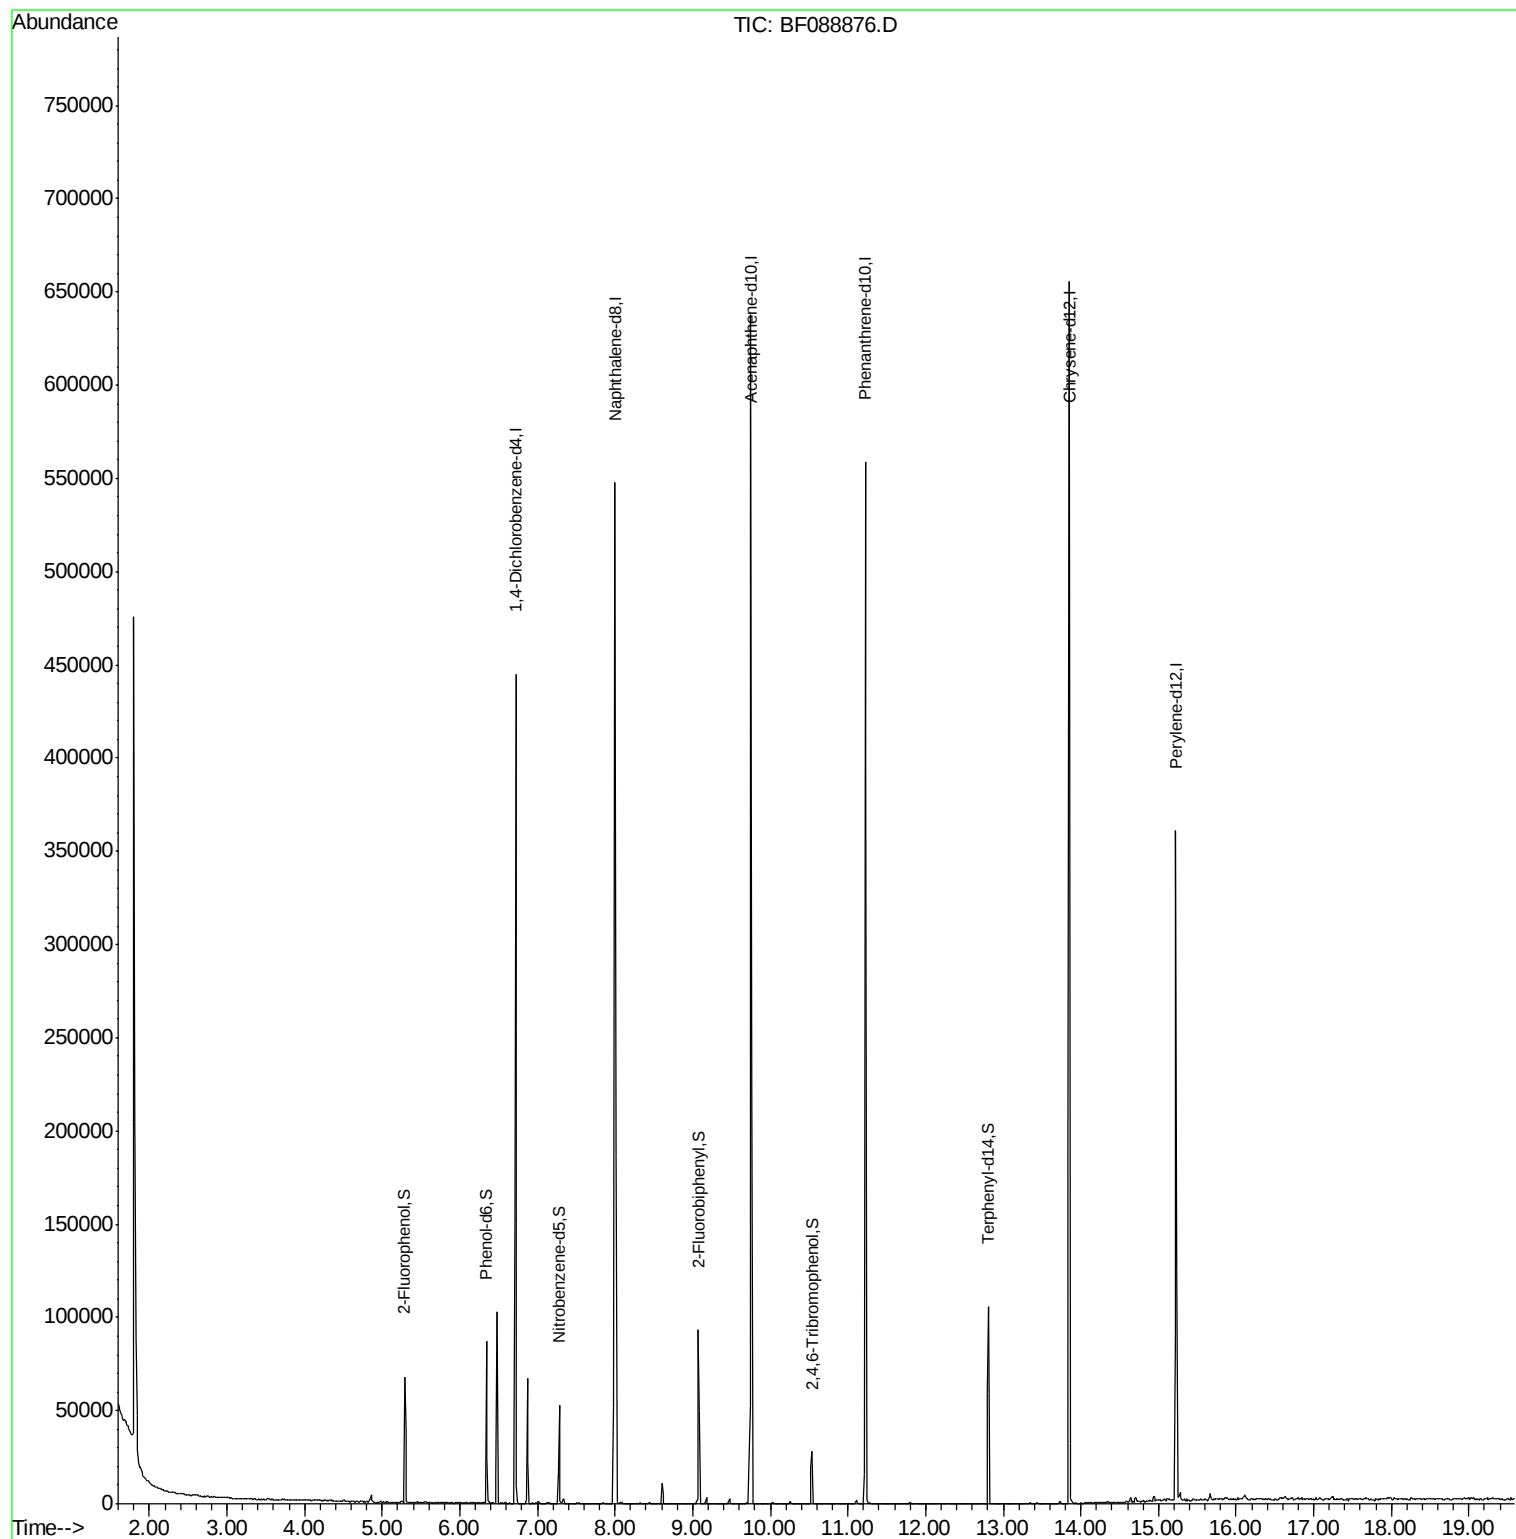




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.72 min Scan# 449
Delta R.T. -0.01 min
Lab File: BF088876.D
Acq: 9 Jul 2016 17:37

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Tot Ion:152 Resp: 70432
Ion Ratio Lower Upper
152 100
150 154.6 123.8 185.6
115 61.4 39.6 59.4#

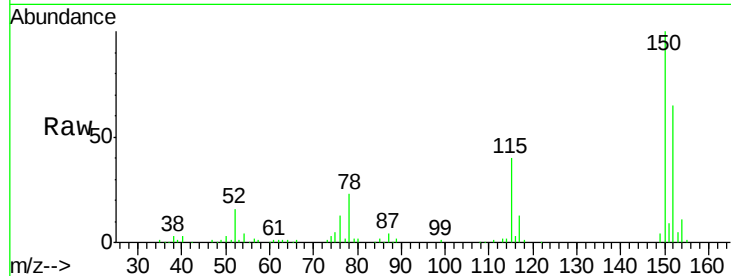


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

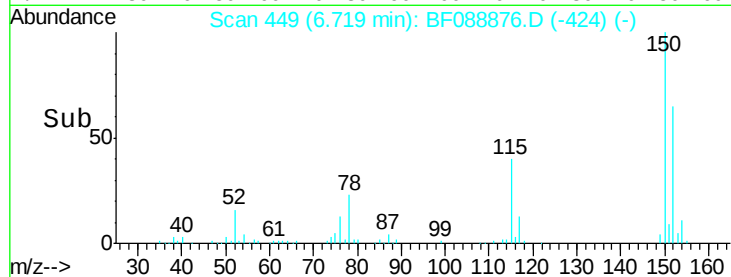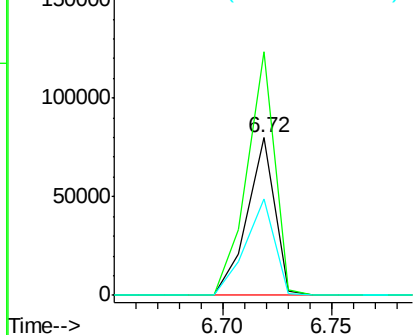



#5


2-Fluorophenol
Concen: 4.75 ng
RT: 5.29 min Scan# 324
Delta R.T. -0.03 min
Lab File: BF088876.D
Acq: 9 Jul 2016 17:37

Tgt Ion:112 Resp: 22305
Ion Ratio Lower Upper
112 100
64 66.6 42.2 63.2#
63 34.6 21.8 32.8#

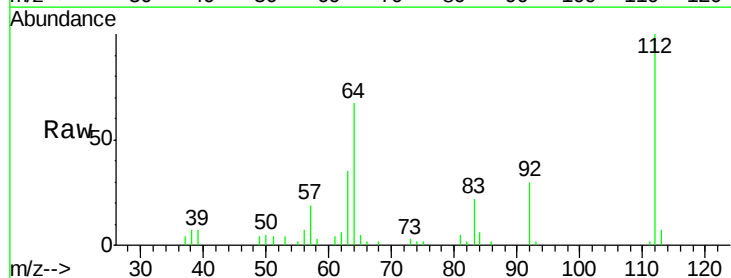

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

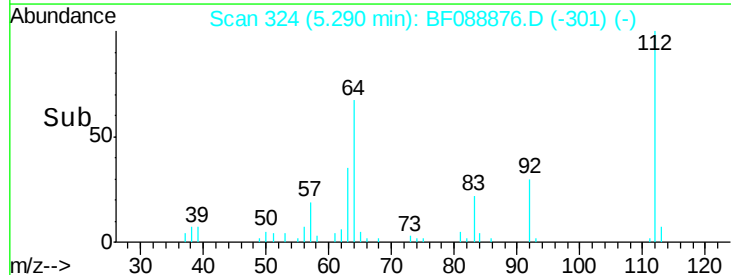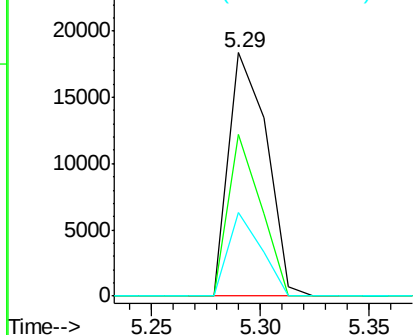

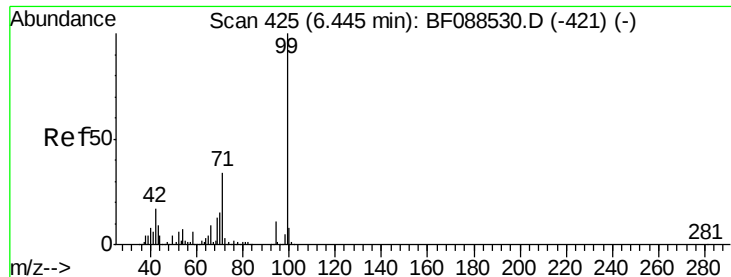

#7

Phenol-d6

Concen: 4.97 ng

RT: 6.34 min Scan# 416

Delta R.T. -0.03 min

Lab File: BF088876.D

Acq: 9 Jul 2016 17:37

Instrument :

BNA_F

ClientSampleId :

P001-DS001-02





Tot Ion: 99 Resp: 30150

Ion Ratio Lower Upper

99 100

42 18.2 12.2 18.2

71 37.9 23.4 35.0#

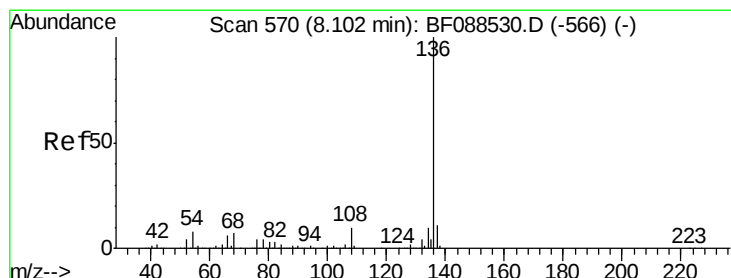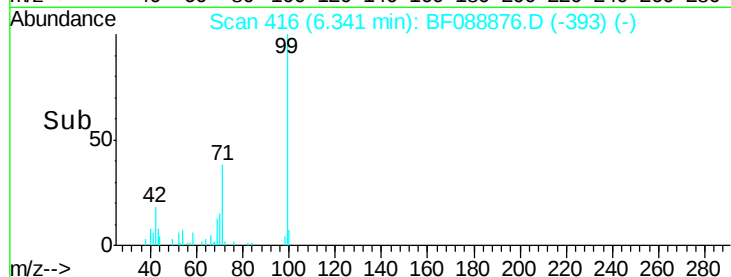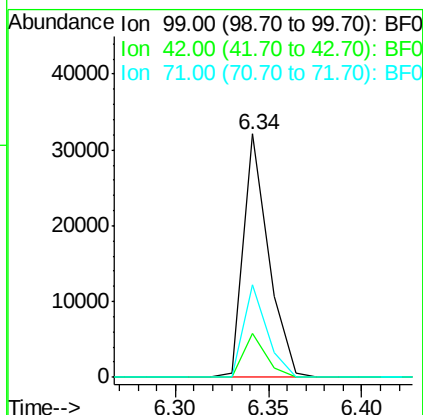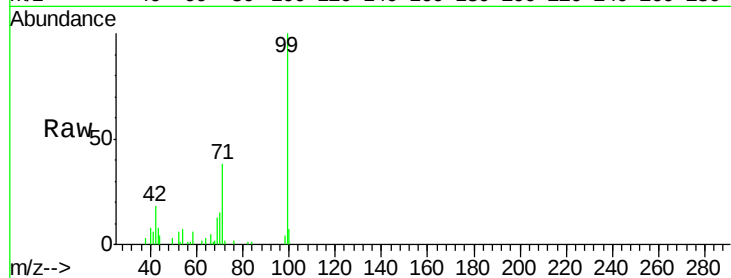

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.00 min Scan# 561

Delta R.T. -0.02 min

Lab File: BF088876.D

Acq: 9 Jul 2016 17:37

Tgt Ion: 136 Resp: 264767




Ion Ratio Lower Upper


136 100

137 11.0 9.1 13.7

54 8.6 6.6 10.0

68 6.9 5.1 7.7

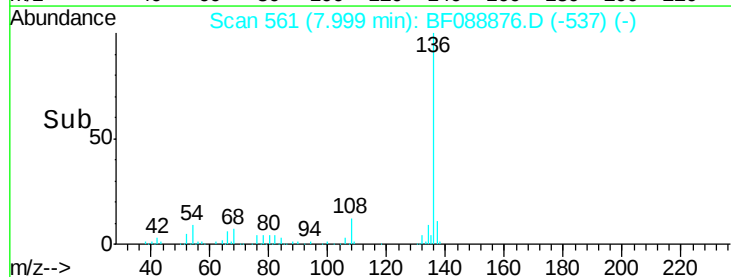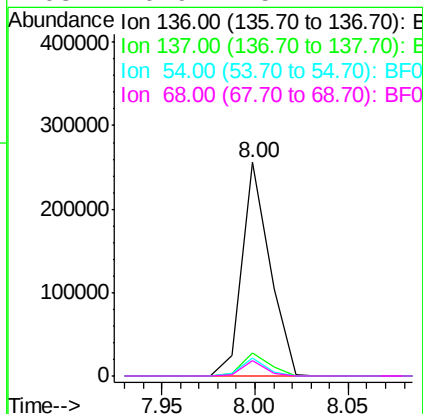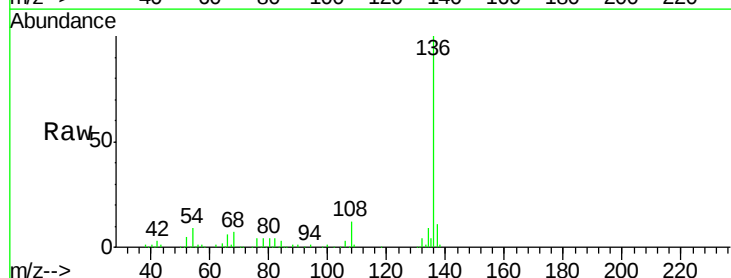

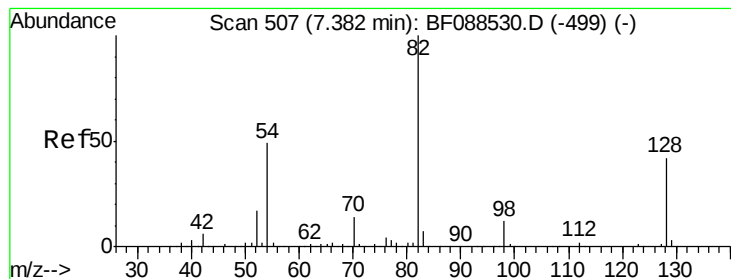

#23

Nitrobenzene-d5

Concen: 3.75 ng

RT: 7.28 min Scan# 498

Delta R.T. -0.02 min

Lab File: BF088876.D

Acq: 9 Jul 2016 17:37

Instrument :

BNA_F

ClientSampleId :

P001-DS001-02


Tot Ion: 82 Resp: 18933

Ion Ratio Lower Upper




82 100

128 45.6 35.9 53.9

54 42.7 40.9 61.3

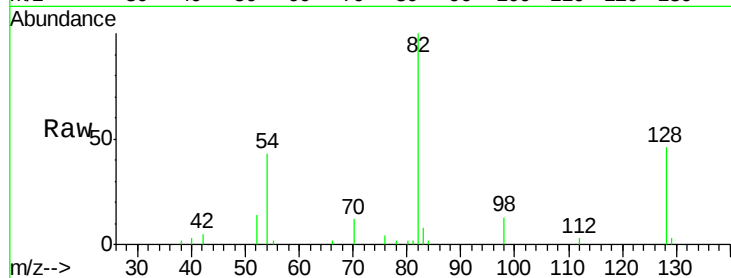

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

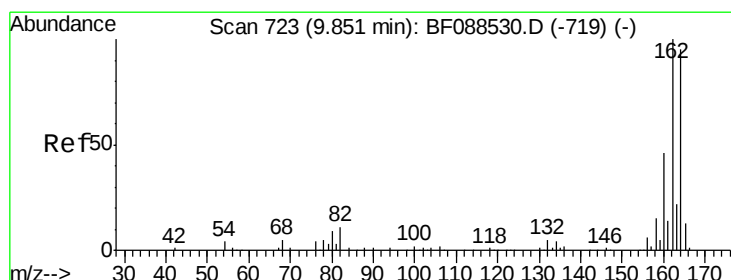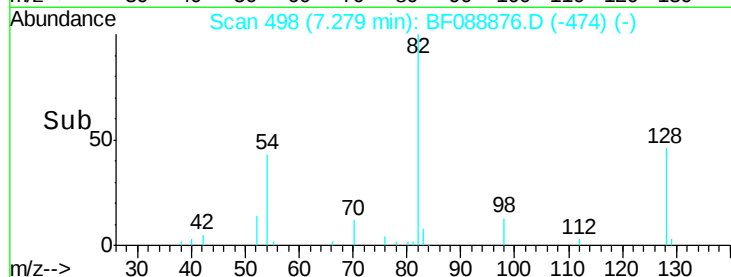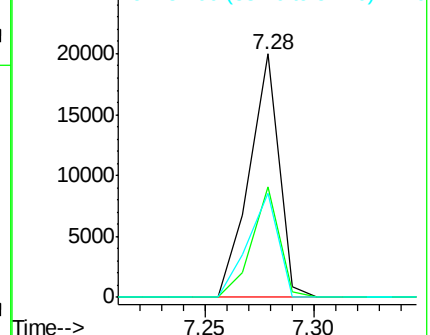

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.75 min Scan# 714

Delta R.T. -0.02 min

Lab File: BF088876.D

Acq: 9 Jul 2016 17:37


Tgt Ion:164 Resp: 131720

Ion Ratio Lower Upper



164 100

162 104.4 85.4 128.2

160 46.4 39.5 59.3

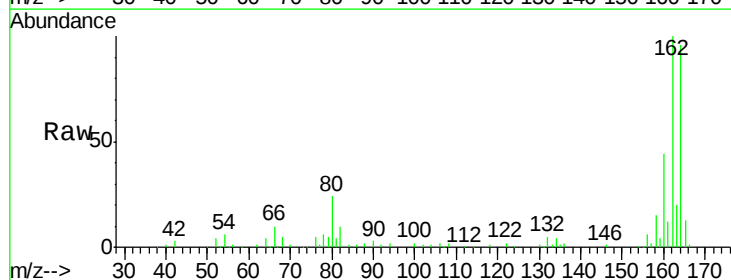

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

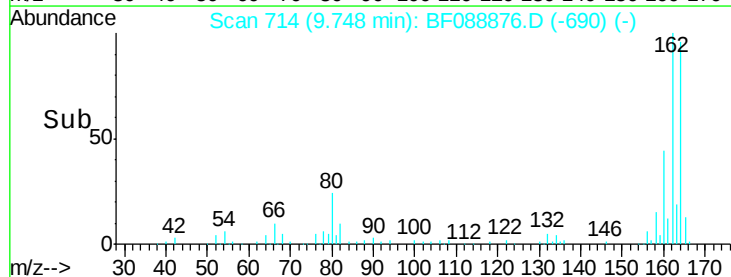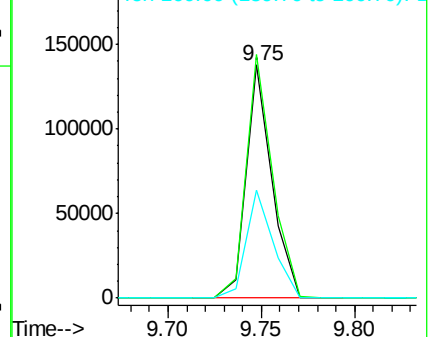






#41
 2,4,6-Tribromophenol
 Concen: 4.49 ng
 RT: 10.54 min Scan# 783
 Delta R.T. -0.02 min
 Lab File: BF088876.D
 Acq: 9 Jul 2016 17:37

Instrument :
 BNA_F
 ClientSampleId :
 P001-DS001-02

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.4	0.0	0.0#
141	34.3	0.0	0.0#

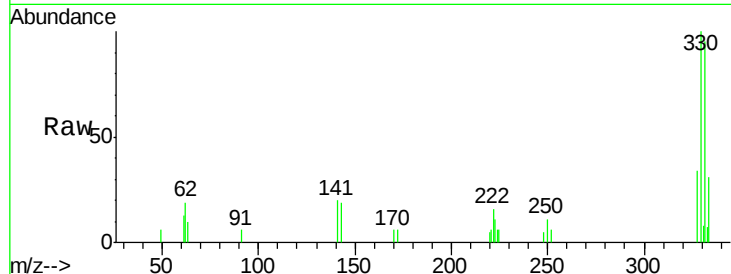


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

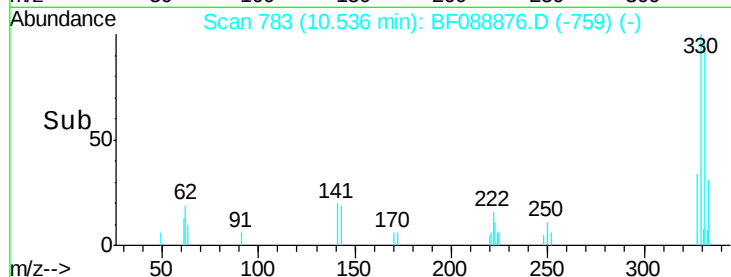
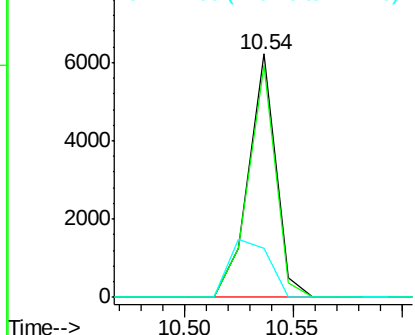



#44
 2-Fluorobiphenyl
 Concen: 4.63 ng
 RT: 9.07 min Scan# 655
 Delta R.T. -0.02 min
 Lab File: BF088876.D
 Acq: 9 Jul 2016 17:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	28.6	43.0
170	23.3	19.2	28.8

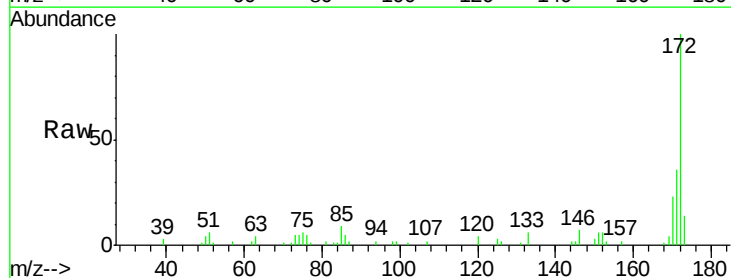

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

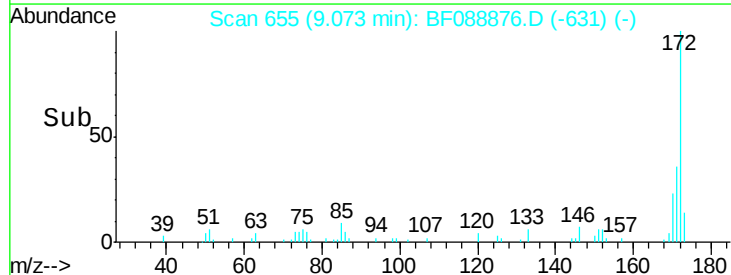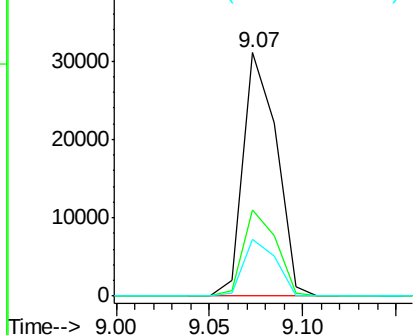


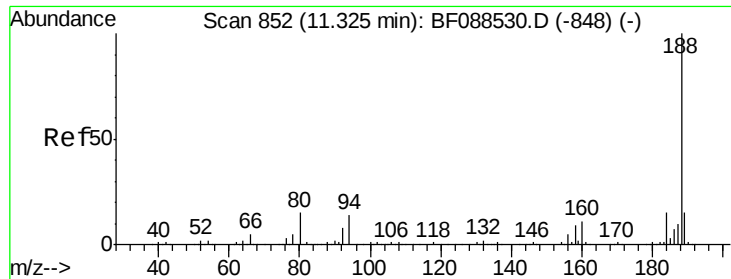




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.22 min Scan# 843
Delta R.T. -0.02 min
Lab File: BF088876.D
Acq: 9 Jul 2016 17:37

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Tot Ion:188 Resp: 265648
Ion Ratio Lower Upper
188 100
94 13.5 9.0 13.6
80 15.4 10.0 15.0#

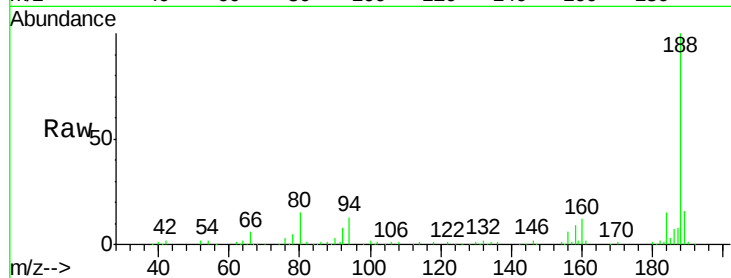


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

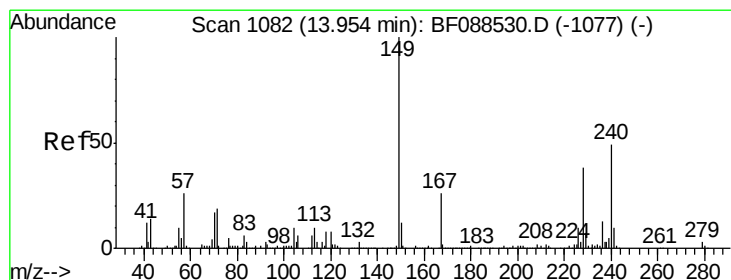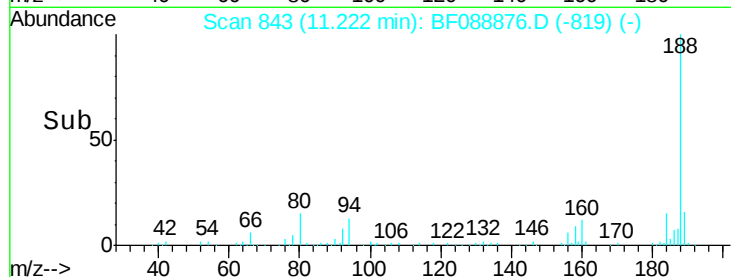
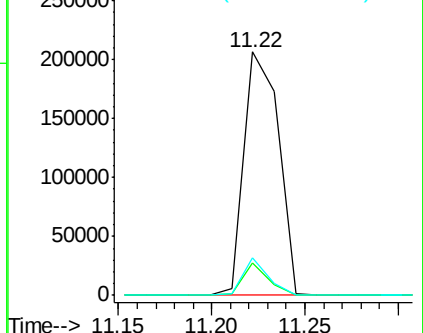


#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.85 min Scan# 1073
Delta R.T. -0.02 min
Lab File: BF088876.D
Acq: 9 Jul 2016 17:37

Tgt Ion:240 Resp: 220614
Ion Ratio Lower Upper
240 100
120 10.4 6.8 10.2#
236 26.0 20.2 30.2

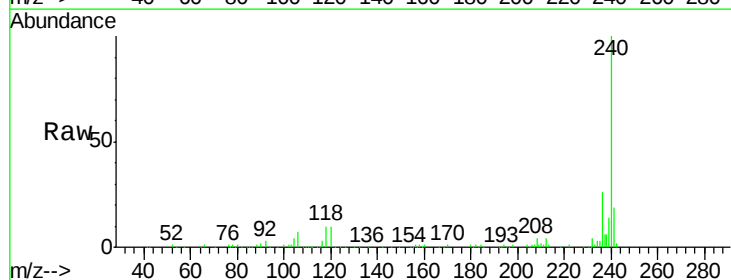

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



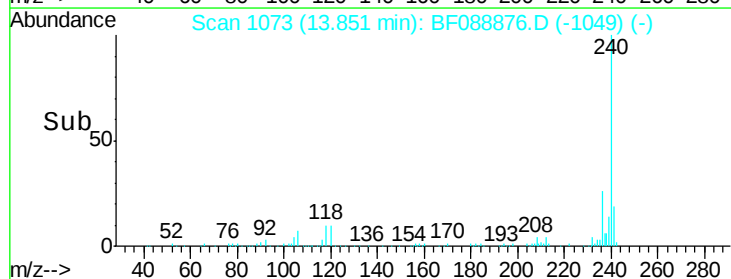
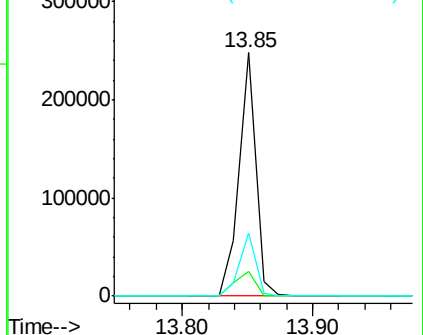




#78
 Terphenyl-d14
 Concen: 4.19 ng
 RT: 12.81 min Scan# 982
 Delta R.T. -0.01 min
 Lab File: BF088876.D
 Acq: 9 Jul 2016 17:37

Instrument :
 BNA_F
 ClientSampleId :
 P001-DS001-02

Tot Ion:244 Resp: 41485
 Ion Ratio Lower Upper
 244 100
 212 6.6 6.0 9.0
 122 7.6 11.2 16.8#

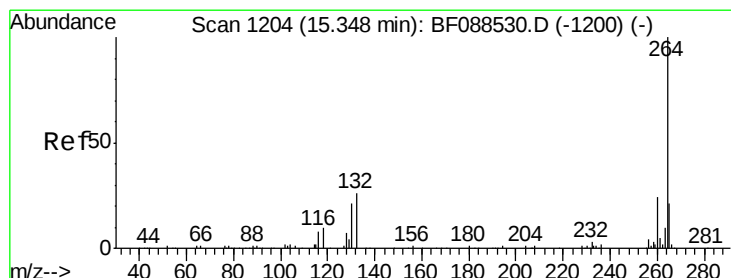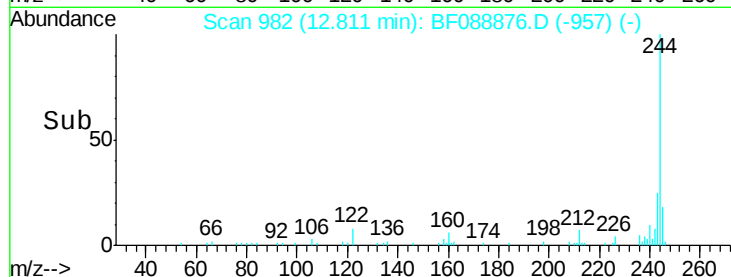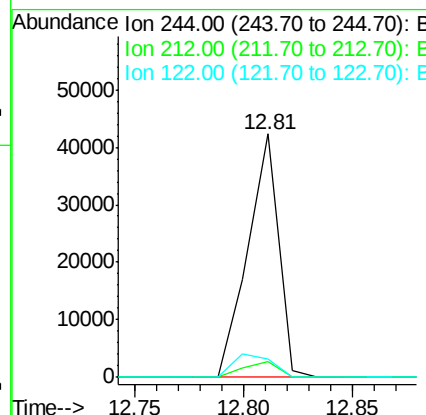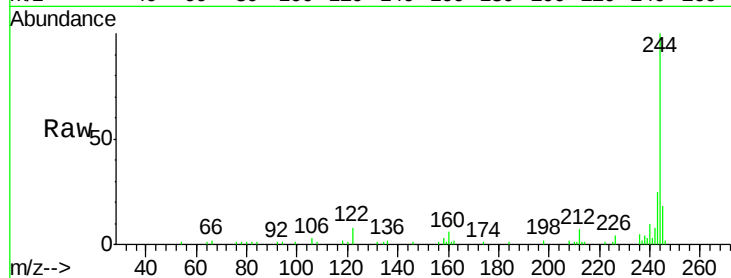

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.22 min Scan# 1193
 Delta R.T. -0.02 min
 Lab File: BF088876.D
 Acq: 9 Jul 2016 17:37

Tgt Ion:264 Resp: 150981
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.2 28.8
 265 21.0 16.9 25.3

