

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088865.D
 Acq On : 9 Jul 2016 12:09
 Operator : UM/SJ
 Sample : PB91808BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB91808BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.678	7	8	17	rVB	82719	149033	5.71%	1.864%
2	1.804	17	19	67	rVB	1358761	2610010	100.00%	32.637%
3	5.301	323	325	327	rBV	246142	219345	8.40%	2.743%
4	6.342	414	416	419	rBV	204117	210582	8.07%	2.633%
5	6.479	426	428	430	rBV	288153	234119	8.97%	2.928%
6	6.719	447	449	451	rBB	478930	417319	15.99%	5.218%
7	6.867	460	462	465	rBB	153273	176482	6.76%	2.207%
8	7.279	496	498	500	rBB	160103	141356	5.42%	1.768%
9	7.999	559	561	564	rBV	475685	528717	20.26%	6.611%
10	9.073	653	655	658	rBV	206262	275845	10.57%	3.449%
11	9.748	712	714	717	rBB	555723	618828	23.71%	7.738%
12	10.536	781	783	785	rBV	146602	158238	6.06%	1.979%
13	11.233	841	844	846	rBV	509857	687065	26.32%	8.591%
14	12.811	980	982	984	rBV	353811	319546	12.24%	3.996%
15	13.851	1070	1073	1075	rBV	748258	658050	25.21%	8.229%
16	15.222	1190	1193	1196	rBV	418200	557687	21.37%	6.974%
17	15.280	1196	1198	1206	rVB	14553	34887	1.34%	0.436%




Sum of corrected areas: 7997109

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088865.D
Acq On : 9 Jul 2016 12:09
Operator : UM/SJ
Sample : PB91808BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91808BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

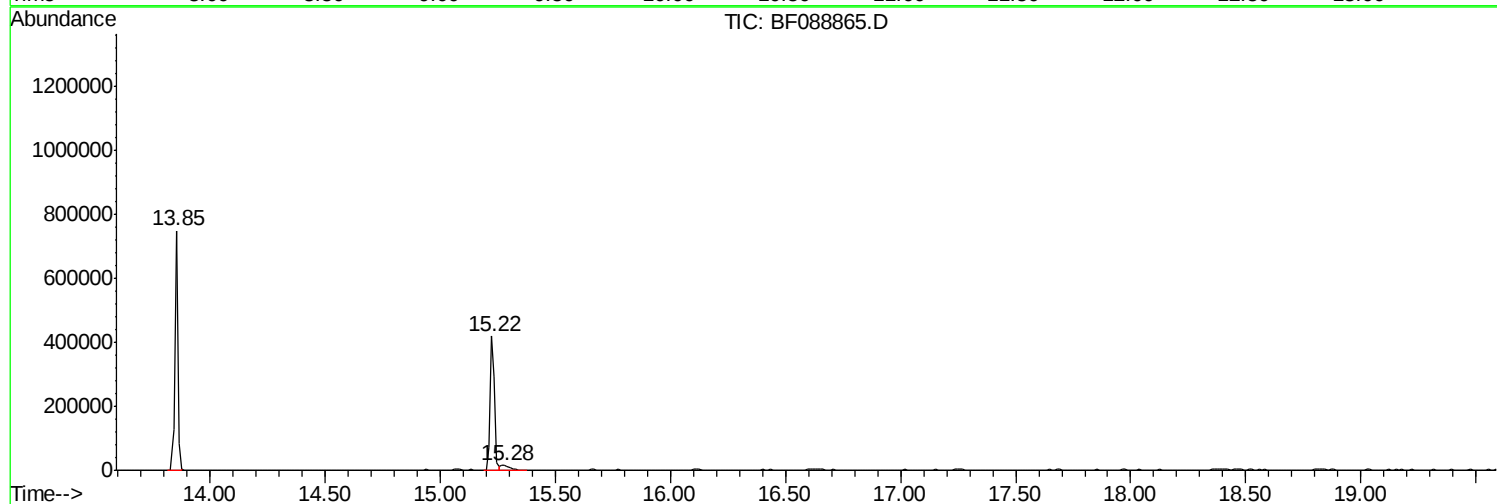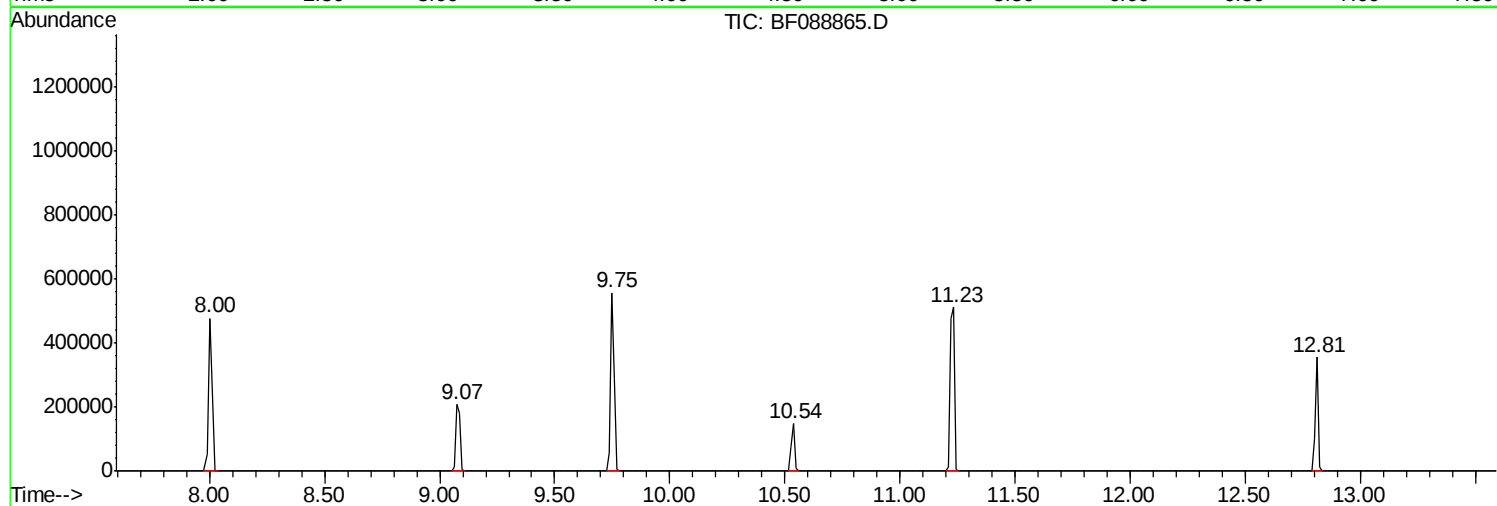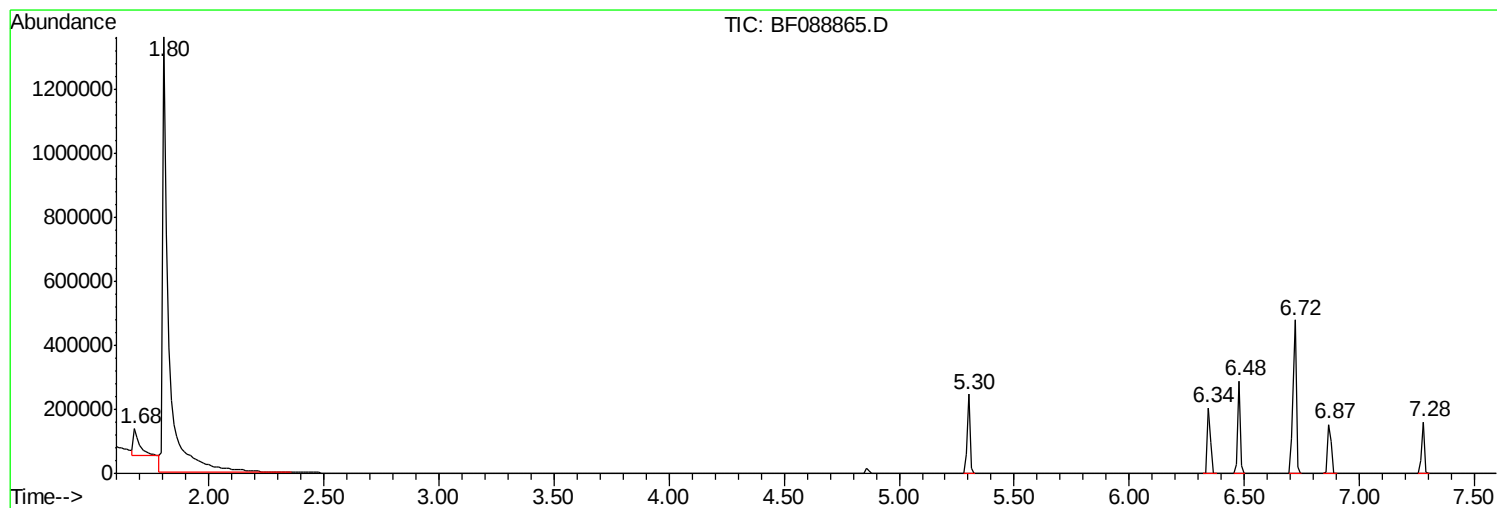

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088865.D
Acq On : 9 Jul 2016 12:09
Operator : UM/SJ
Sample : PB91808BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91808BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown11.22 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	11.22 ng	234119	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3	Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2	5	Aminoindole	132	C8H8N2	005192-03-0	12
3	4	Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4	5	Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5	(E)-3	Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

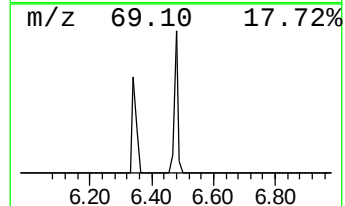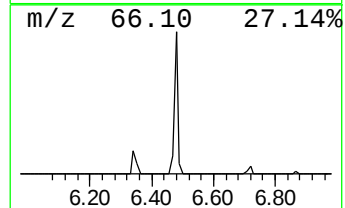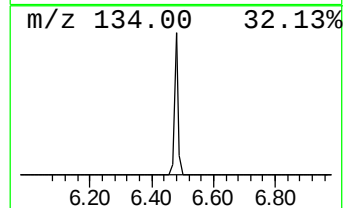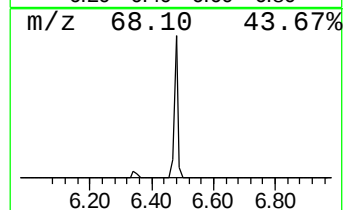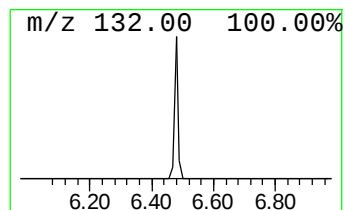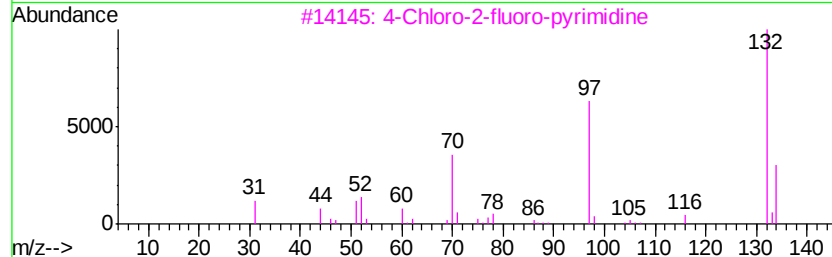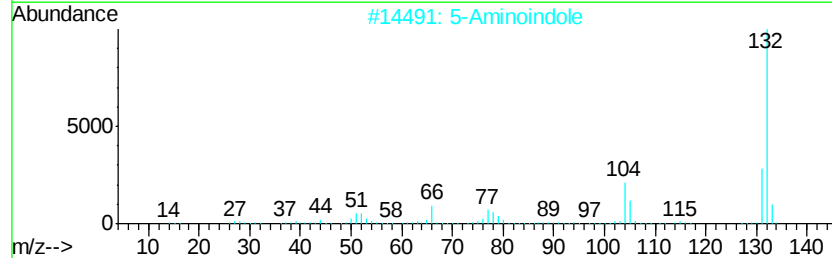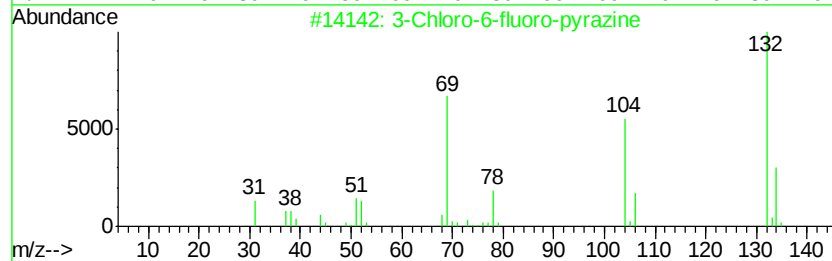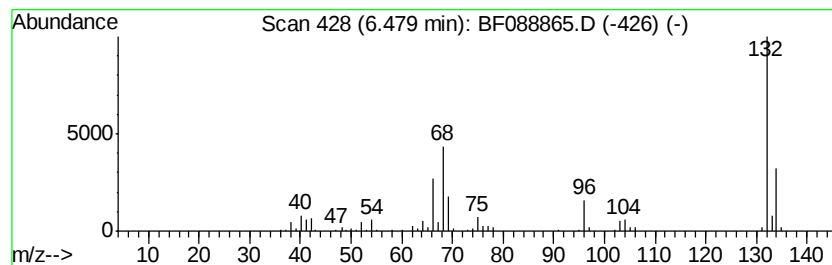

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088865.D
Acq On : 9 Jul 2016 12:09
Operator : UM/SJ
Sample : PB91808BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91808BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown11.22	6.48	11.2	ng	234119	1	6.72	417319	20.0