

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088873.D
 Acq On : 9 Jul 2016 16:09
 Operator : UM/SJ
 Sample : H3813-06 25X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-DS001-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.804	17	19	37	rVB	428764	551954	84.04%	13.062%
2	5.290	323	324	327	rVB	39481	55027	8.38%	1.302%
3	6.342	415	416	418	rBV	73879	65638	9.99%	1.553%
4	6.479	426	428	430	rBB	82666	65277	9.94%	1.545%
5	6.719	447	449	451	rBB	450726	408906	62.26%	9.677%
6	6.867	461	462	464	rBB	48937	44967	6.85%	1.064%
7	7.279	496	498	500	rBB	41488	38348	5.84%	0.908%
8	7.999	559	561	564	rBV	537573	525444	80.00%	12.435%
9	8.605	613	614	616	rBB	12686	13213	2.01%	0.313%
10	9.073	653	655	658	rBV	79290	86267	13.13%	2.042%
11	9.748	712	714	717	rBB	605759	614002	93.48%	14.531%
12	10.536	781	783	785	rBB	22490	28724	4.37%	0.680%
13	11.222	841	843	846	rBV2	611087	656814	100.00%	15.544%
14	12.811	980	982	984	rBB	79764	99366	15.13%	2.352%
15	13.851	1070	1073	1075	rBV	634466	593121	90.30%	14.037%
16	15.223	1190	1193	1196	rBV	345684	378492	57.63%	8.957%


Sum of corrected areas: 4225560

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088873.D
Acq On : 9 Jul 2016 16:09
Operator : UM/SJ
Sample : H3813-06 25X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

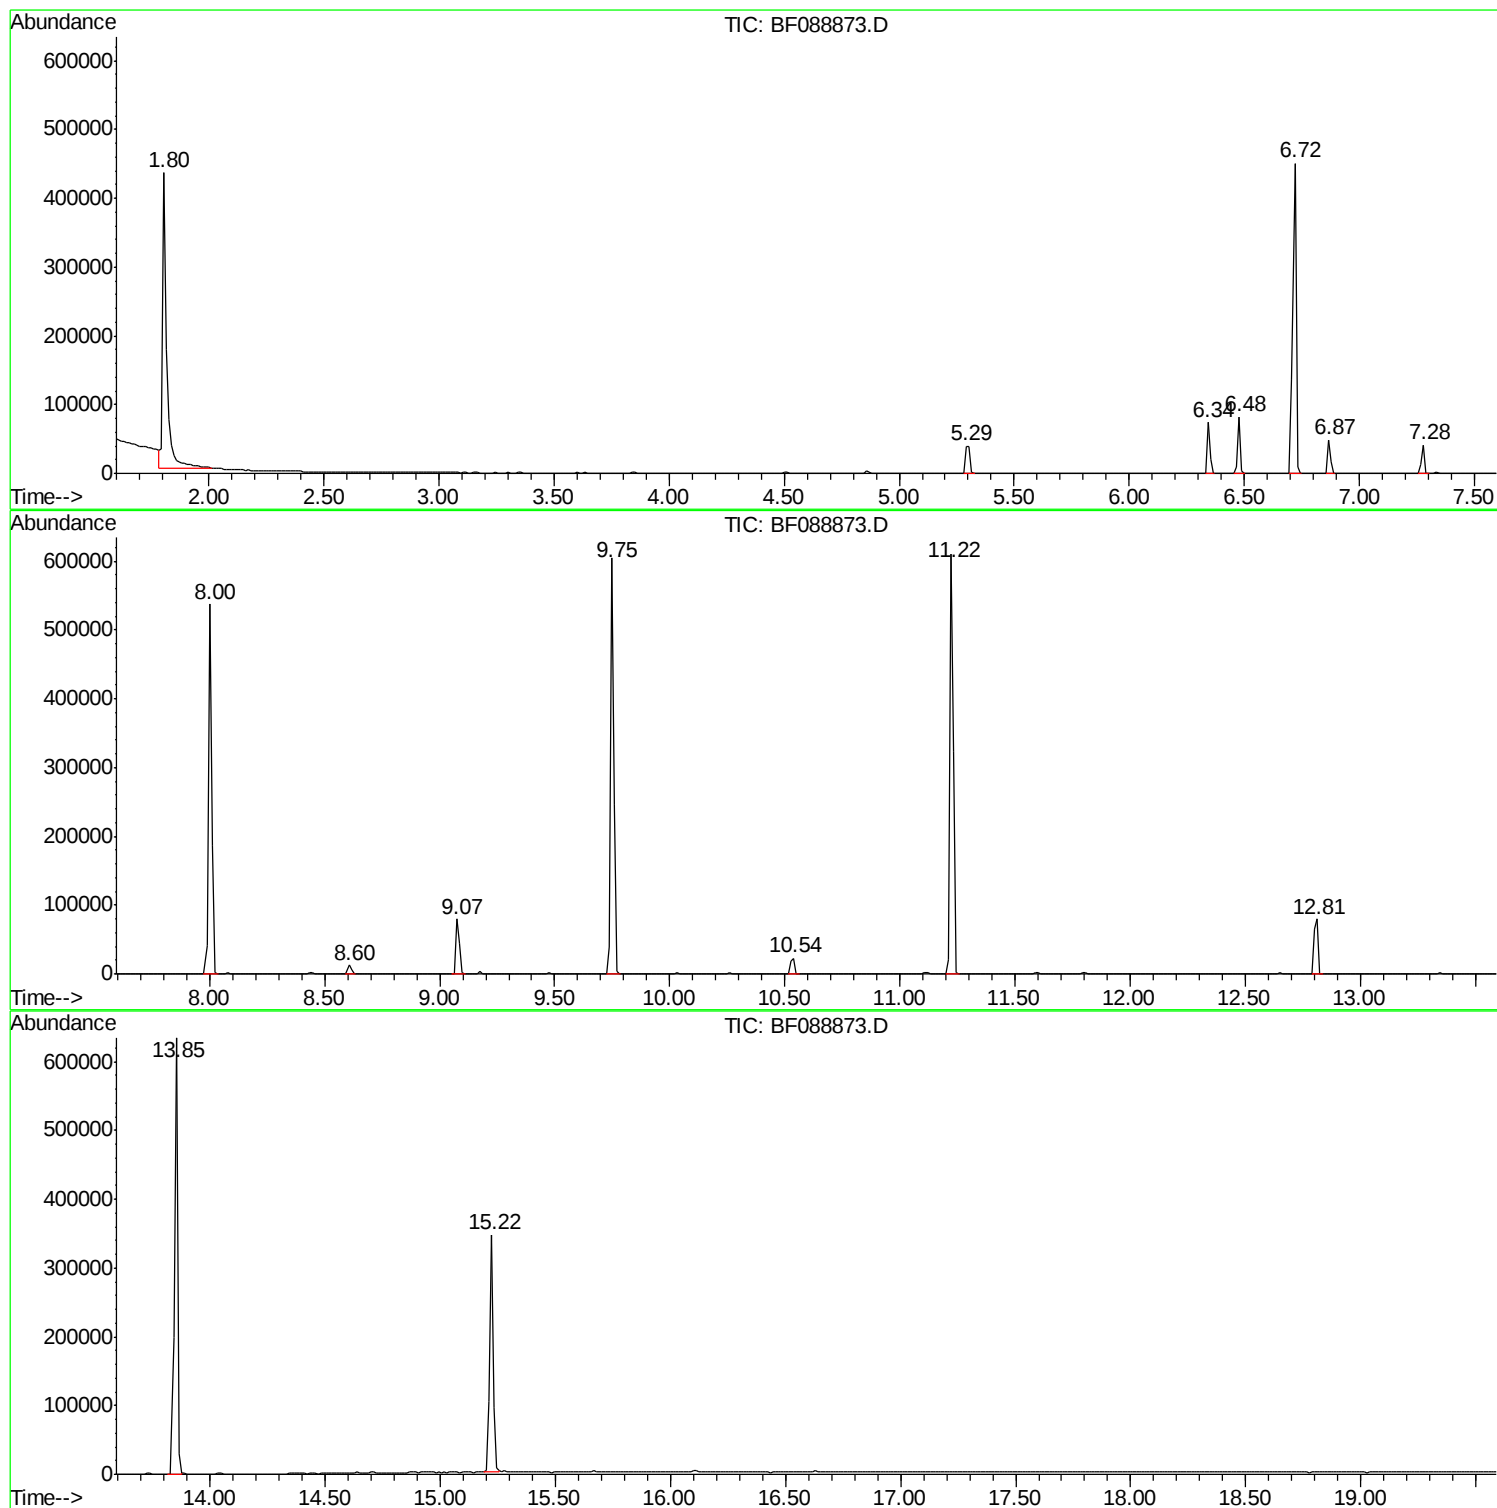

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088873.D
Acq On : 9 Jul 2016 16:09
Operator : UM/SJ
Sample : H3813-06 25X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	3.19 ng	65277	1,4-Dichlorobenzene-d4	6.72

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

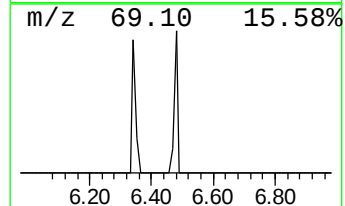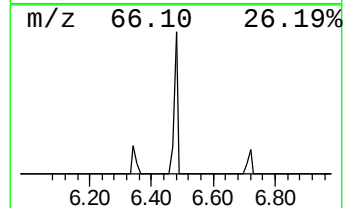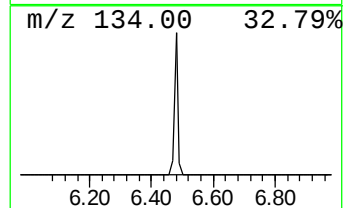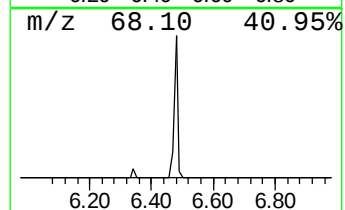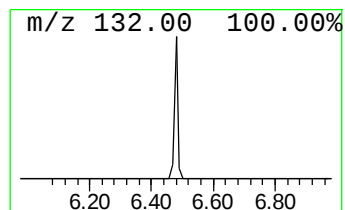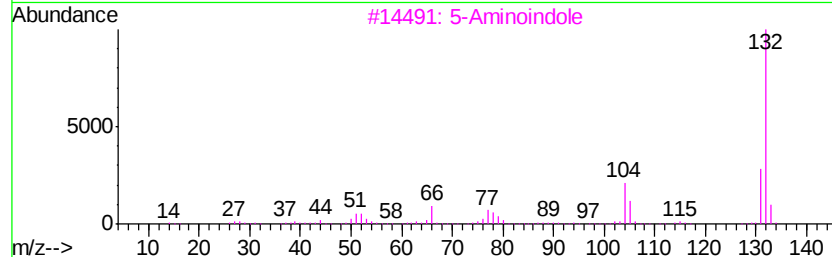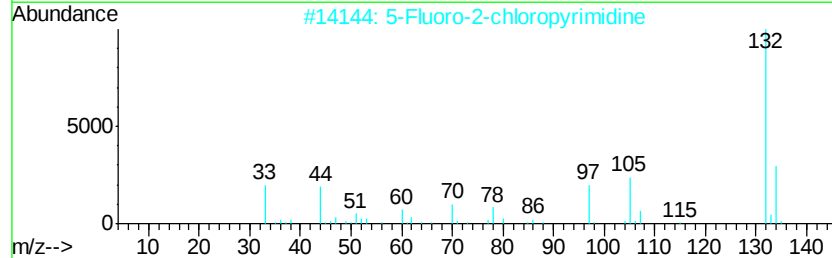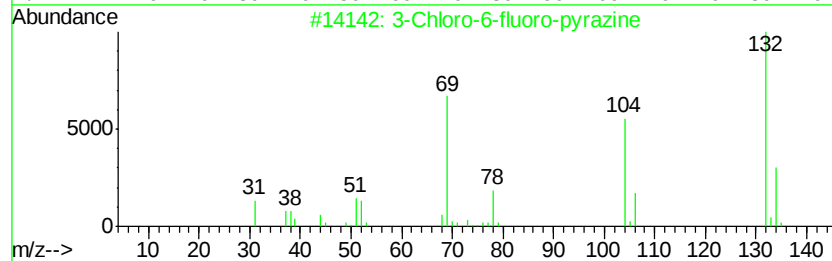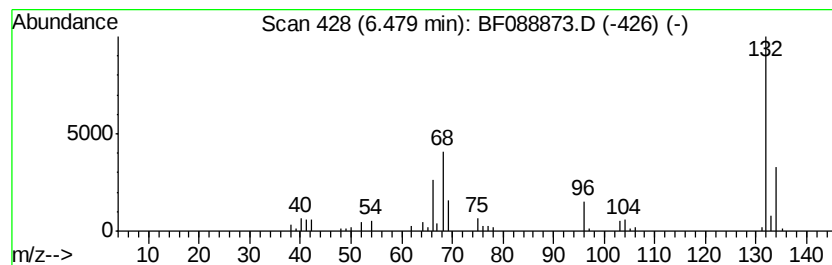

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088873.D
Acq On : 9 Jul 2016 16:09
Operator : UM/SJ
Sample : H3813-06 25X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	3.2	ng	65277	1	6.72	408906	20.0