

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088876.D
 Acq On : 9 Jul 2016 17:37
 Operator : UM/SJ
 Sample : H3813-09 25X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-DS001-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.804	17	19	25	rVB	456350	528233	79.29%	12.009%
2	5.290	323	324	327	rBV	67364	72251	10.85%	1.643%
3	6.341	415	416	419	rBV	86713	76884	11.54%	1.748%
4	6.479	425	428	430	rBV	102647	83359	12.51%	1.895%
5	6.719	447	449	451	rBV	445222	415794	62.42%	9.453%
6	6.867	460	462	464	rVB	66845	62388	9.37%	1.418%
7	7.279	495	498	500	rBV	53244	50168	7.53%	1.141%
8	7.999	559	561	564	rBV	547817	540731	81.17%	12.293%
9	8.605	613	614	616	rBB	11256	11006	1.65%	0.250%
10	9.073	653	655	658	rBB	93210	101254	15.20%	2.302%
11	9.748	712	714	717	rBB	637623	629885	94.55%	14.320%
12	10.536	781	783	785	rBB	28264	33154	4.98%	0.754%
13	11.222	841	843	846	rBV2	558722	666166	100.00%	15.145%
14	12.811	980	982	984	rBB	105958	114155	17.14%	2.595%
15	13.851	1071	1073	1075	rBV	655362	602989	90.52%	13.709%
16	15.222	1190	1193	1196	rBV	358752	396518	59.52%	9.015%
17	15.668	1229	1232	1234	rBV2	3704	6803	1.02%	0.155%
18	16.114	1268	1271	1275	rVB2	2768	6798	1.02%	0.155%


Sum of corrected areas: 4398536

Data Path : V:\HPCHEM1\BNA F\DATA\BF070916\
Data File : BF088876.D
Acq On : 9 Jul 2016 17:37
Operator : UM/SJ
Sample : H3813-09 25X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

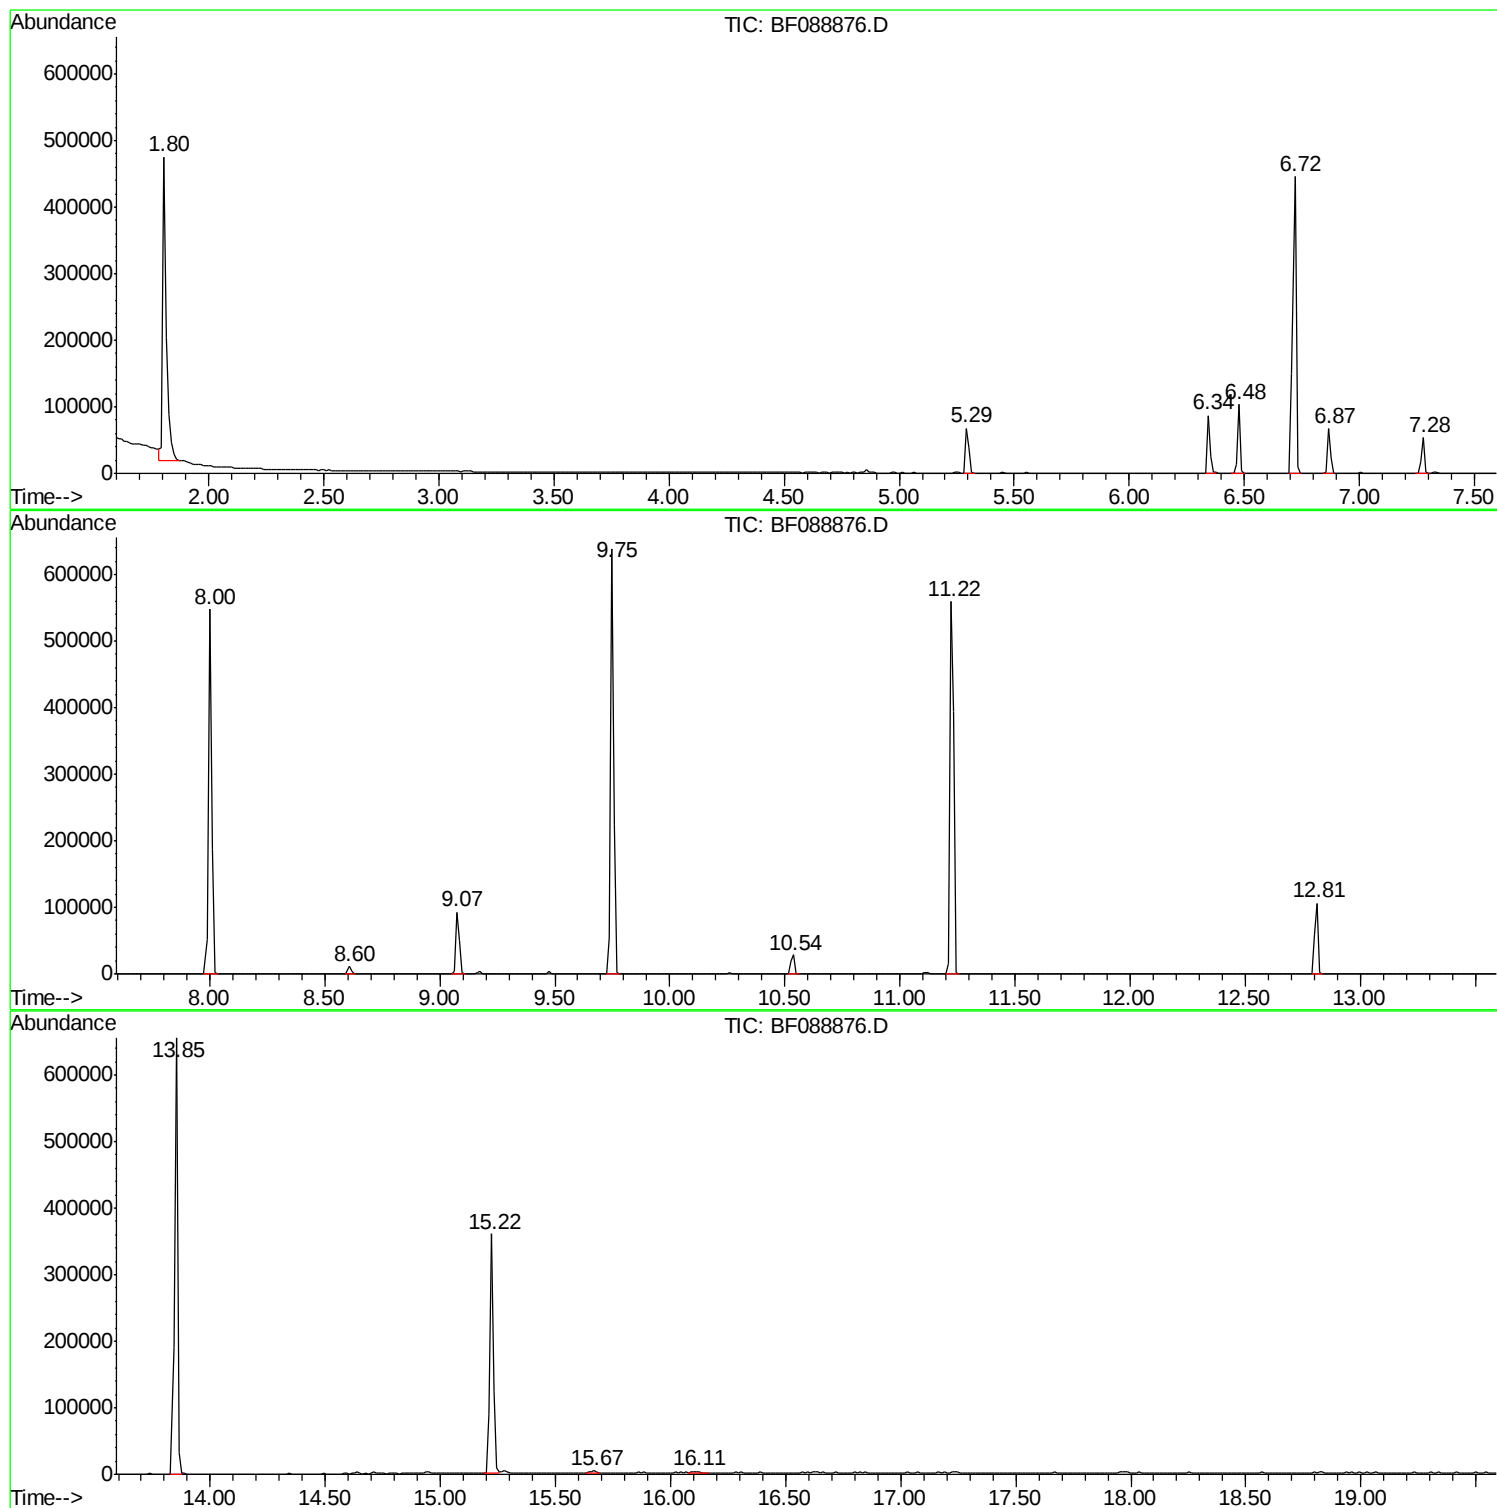

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088876.D
Acq On : 9 Jul 2016 17:37
Operator : UM/SJ
Sample : H3813-09 25X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	4.01 ng	83359	1,4-Dichlorobenzene-d4	6.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4			1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

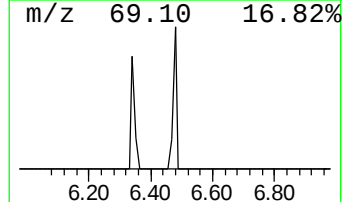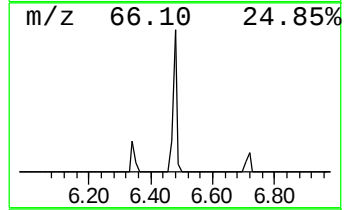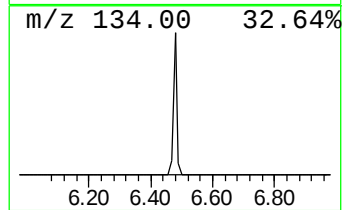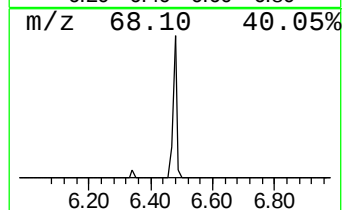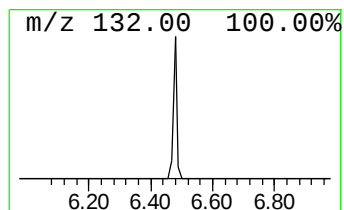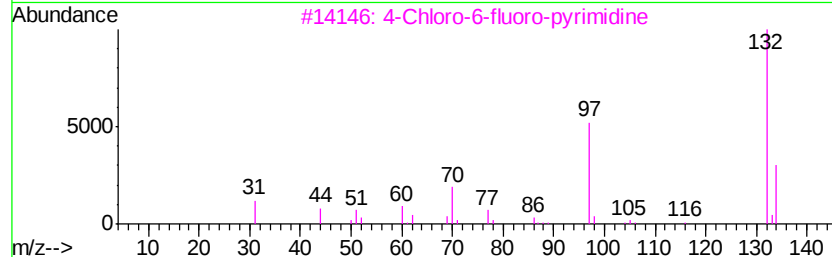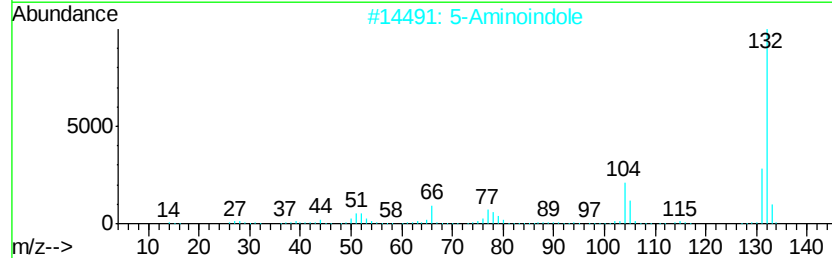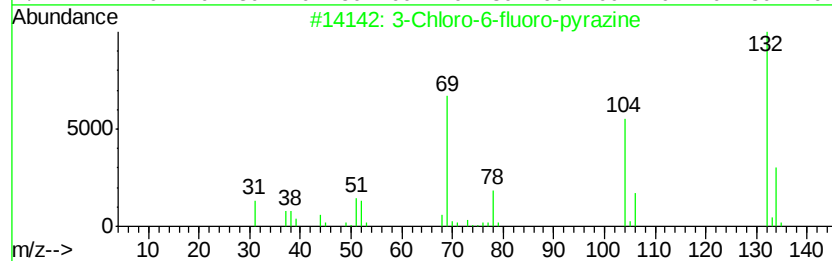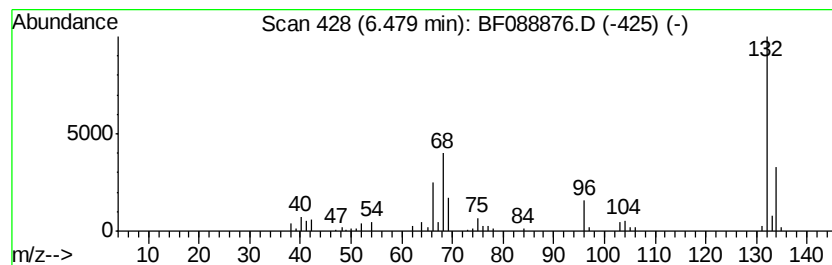

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088876.D
Acq On : 9 Jul 2016 17:37
Operator : UM/SJ
Sample : H3813-09 25X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-DS001-02

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	4.0	ng	83359	1	6.72	415794	20.0