

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088877.D
 Acq On : 9 Jul 2016 18:06
 Operator : UM/SJ
 Sample : H3813-10 25X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS001-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.804	17	19	54	rVB	898285	1342673	100.00%	26.908%
2	5.290	322	324	327	rBV	66914	71323	5.31%	1.429%
3	6.341	414	416	419	rBV	82681	77579	5.78%	1.555%
4	6.479	426	428	430	rBV	101650	81350	6.06%	1.630%
5	6.719	447	449	451	rBB	460703	412453	30.72%	8.266%
6	6.867	461	462	464	rVB	59823	58092	4.33%	1.164%
7	7.279	496	498	500	rBV	55475	49275	3.67%	0.988%
8	7.999	559	561	564	rBV	491343	515979	38.43%	10.341%
9	9.073	653	655	658	rBV	71118	85905	6.40%	1.722%
10	9.748	712	714	717	rBV	575839	623034	46.40%	12.486%
11	10.536	781	783	785	rBB	63739	60518	4.51%	1.213%
12	11.222	841	843	846	rBV2	544627	643493	47.93%	12.896%
13	12.811	980	982	984	rBB	77298	80209	5.97%	1.607%
14	13.851	1070	1073	1075	rBV	552729	526765	39.23%	10.557%
15	15.222	1190	1193	1196	rBV	334779	361171	26.90%	7.238%




Sum of corrected areas: 4989819

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088877.D
Acq On : 9 Jul 2016 18:06
Operator : UM/SJ
Sample : H3813-10 25X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS001-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

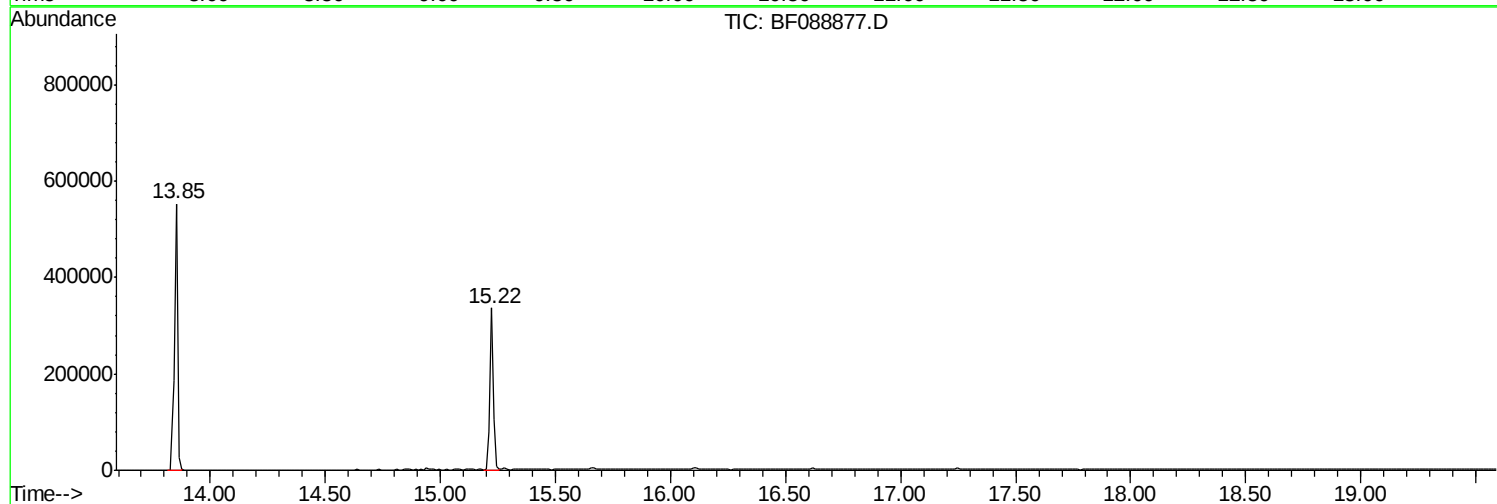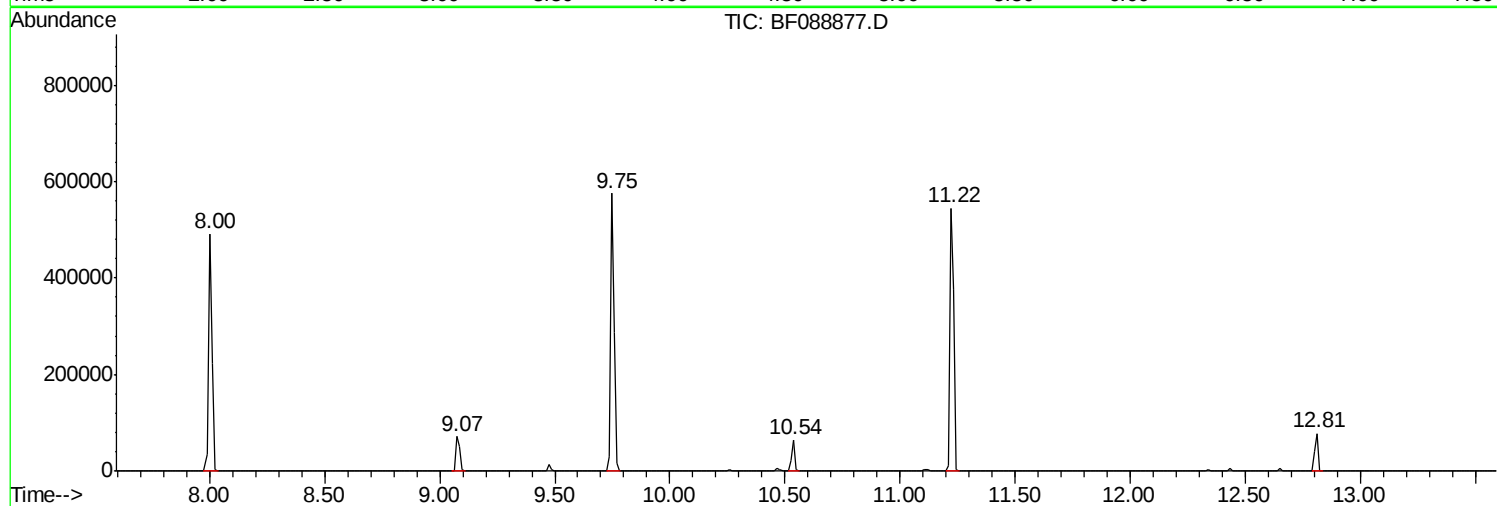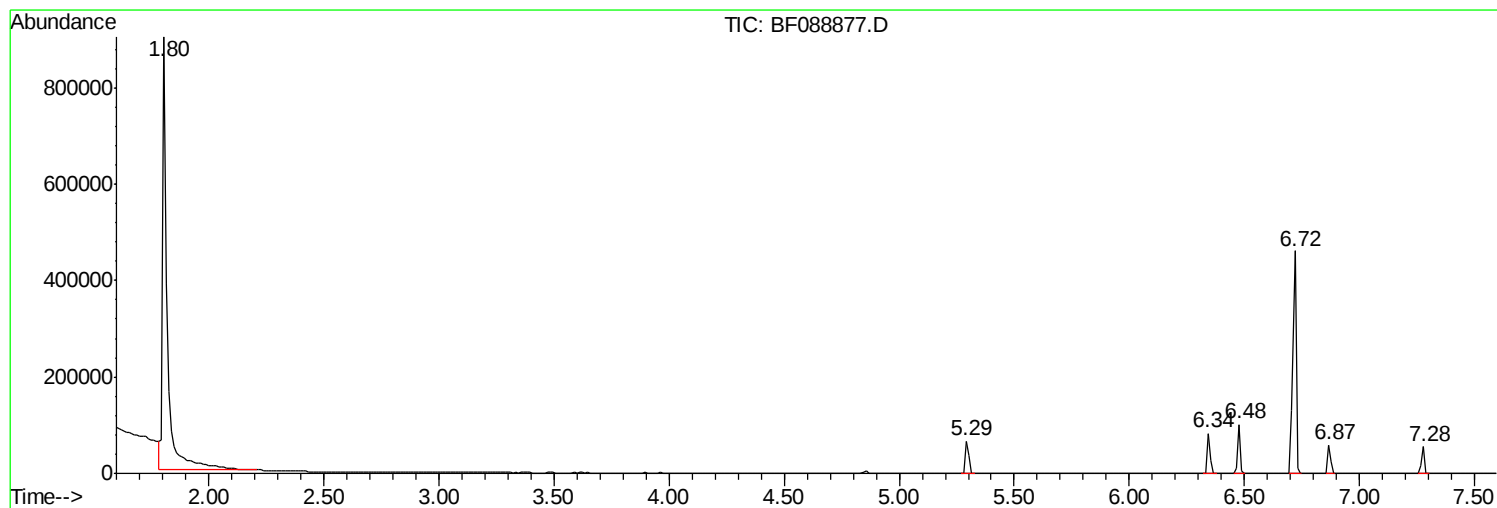

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088877.D
Acq On : 9 Jul 2016 18:06
Operator : UM/SJ
Sample : H3813-10 25X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS001-0006-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	3.94 ng	81350	1,4-Dichlorobenzene-d4	6.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			5-Aminoindole	132	C8H8N2	005192-03-0	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

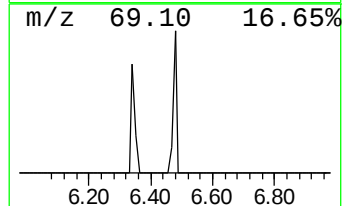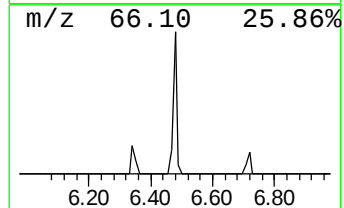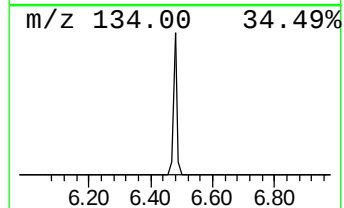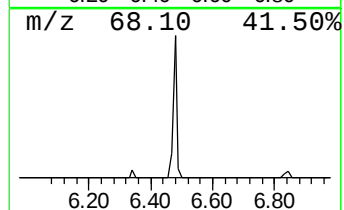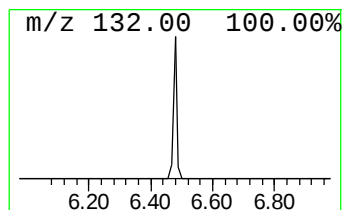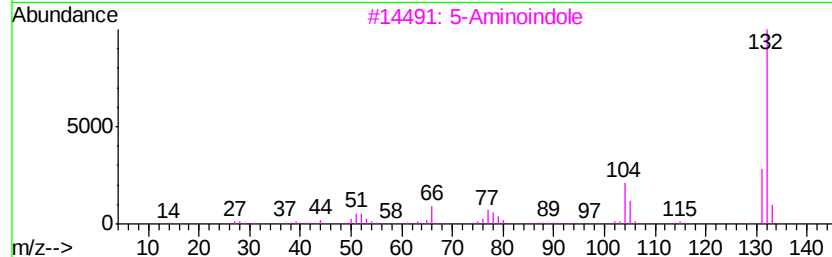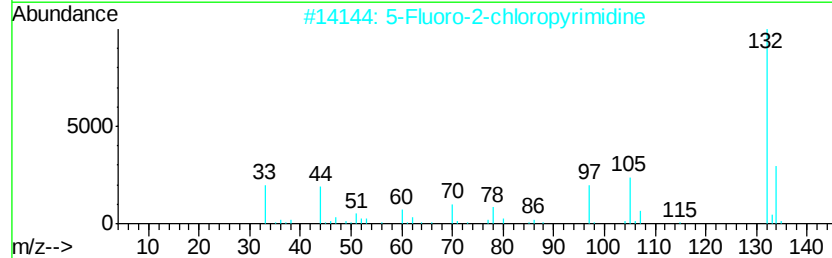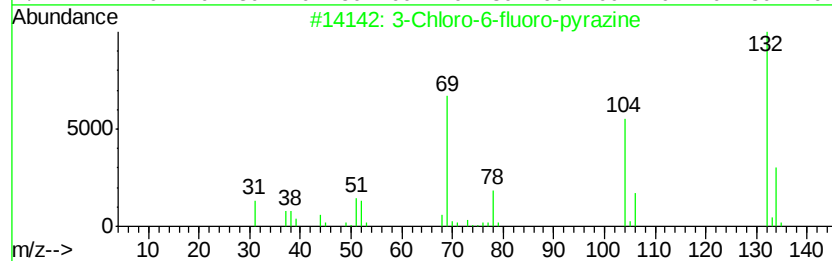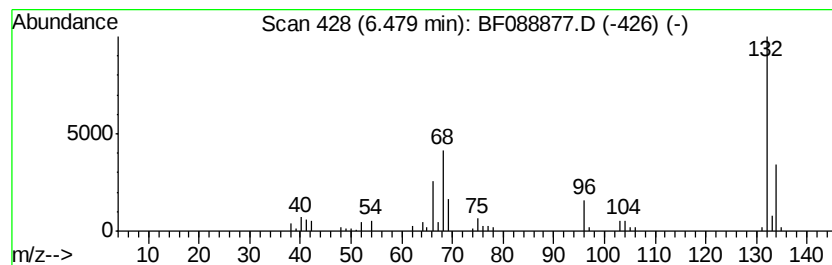

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088877.D
Acq On : 9 Jul 2016 18:06
Operator : UM/SJ
Sample : H3813-10 25X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS001-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	3.9	ng	81350	1	6.72	412453	20.0