

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088878.D
 Acq On : 9 Jul 2016 18:35
 Operator : UM/SJ
 Sample : H3813-11 25X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS002-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.804	17	19	52	rVB	297414	425327	62.39%	9.788%
2	5.290	322	324	327	rBB	67770	69395	10.18%	1.597%
3	6.342	414	416	419	rBV	84605	75239	11.04%	1.731%
4	6.479	426	428	430	rBB	96786	77513	11.37%	1.784%
5	6.719	447	449	451	rBB	483386	437829	64.23%	10.075%
6	6.867	460	462	464	rBB	62185	57719	8.47%	1.328%
7	7.279	496	498	500	rBB	51825	46636	6.84%	1.073%
8	7.999	559	561	564	rBV	562954	556888	81.69%	12.815%
9	9.073	653	655	658	rBV	92704	93163	13.67%	2.144%
10	9.748	712	714	717	rBB2	657928	662503	97.18%	15.245%
11	10.536	781	783	785	rBB	27273	37192	5.46%	0.856%
12	11.222	841	843	846	rBV2	637199	681710	100.00%	15.687%
13	12.811	980	982	984	rBB	78411	93900	13.77%	2.161%
14	13.851	1070	1073	1075	rBV	656695	603807	88.57%	13.895%
15	15.223	1190	1193	1196	rBV	360309	389548	57.14%	8.964%
16	15.280	1196	1198	1204	rVB	7624	11680	1.71%	0.269%
17	15.668	1229	1232	1236	rBV	5274	9381	1.38%	0.216%
18	16.114	1268	1271	1274	rVB	4361	8626	1.27%	0.199%
19	17.246	1366	1370	1375	rVB3	2596	7512	1.10%	0.173%


Sum of corrected areas: 4345568

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088878.D
Acq On : 9 Jul 2016 18:35
Operator : UM/SJ
Sample : H3813-11 25X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS002-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

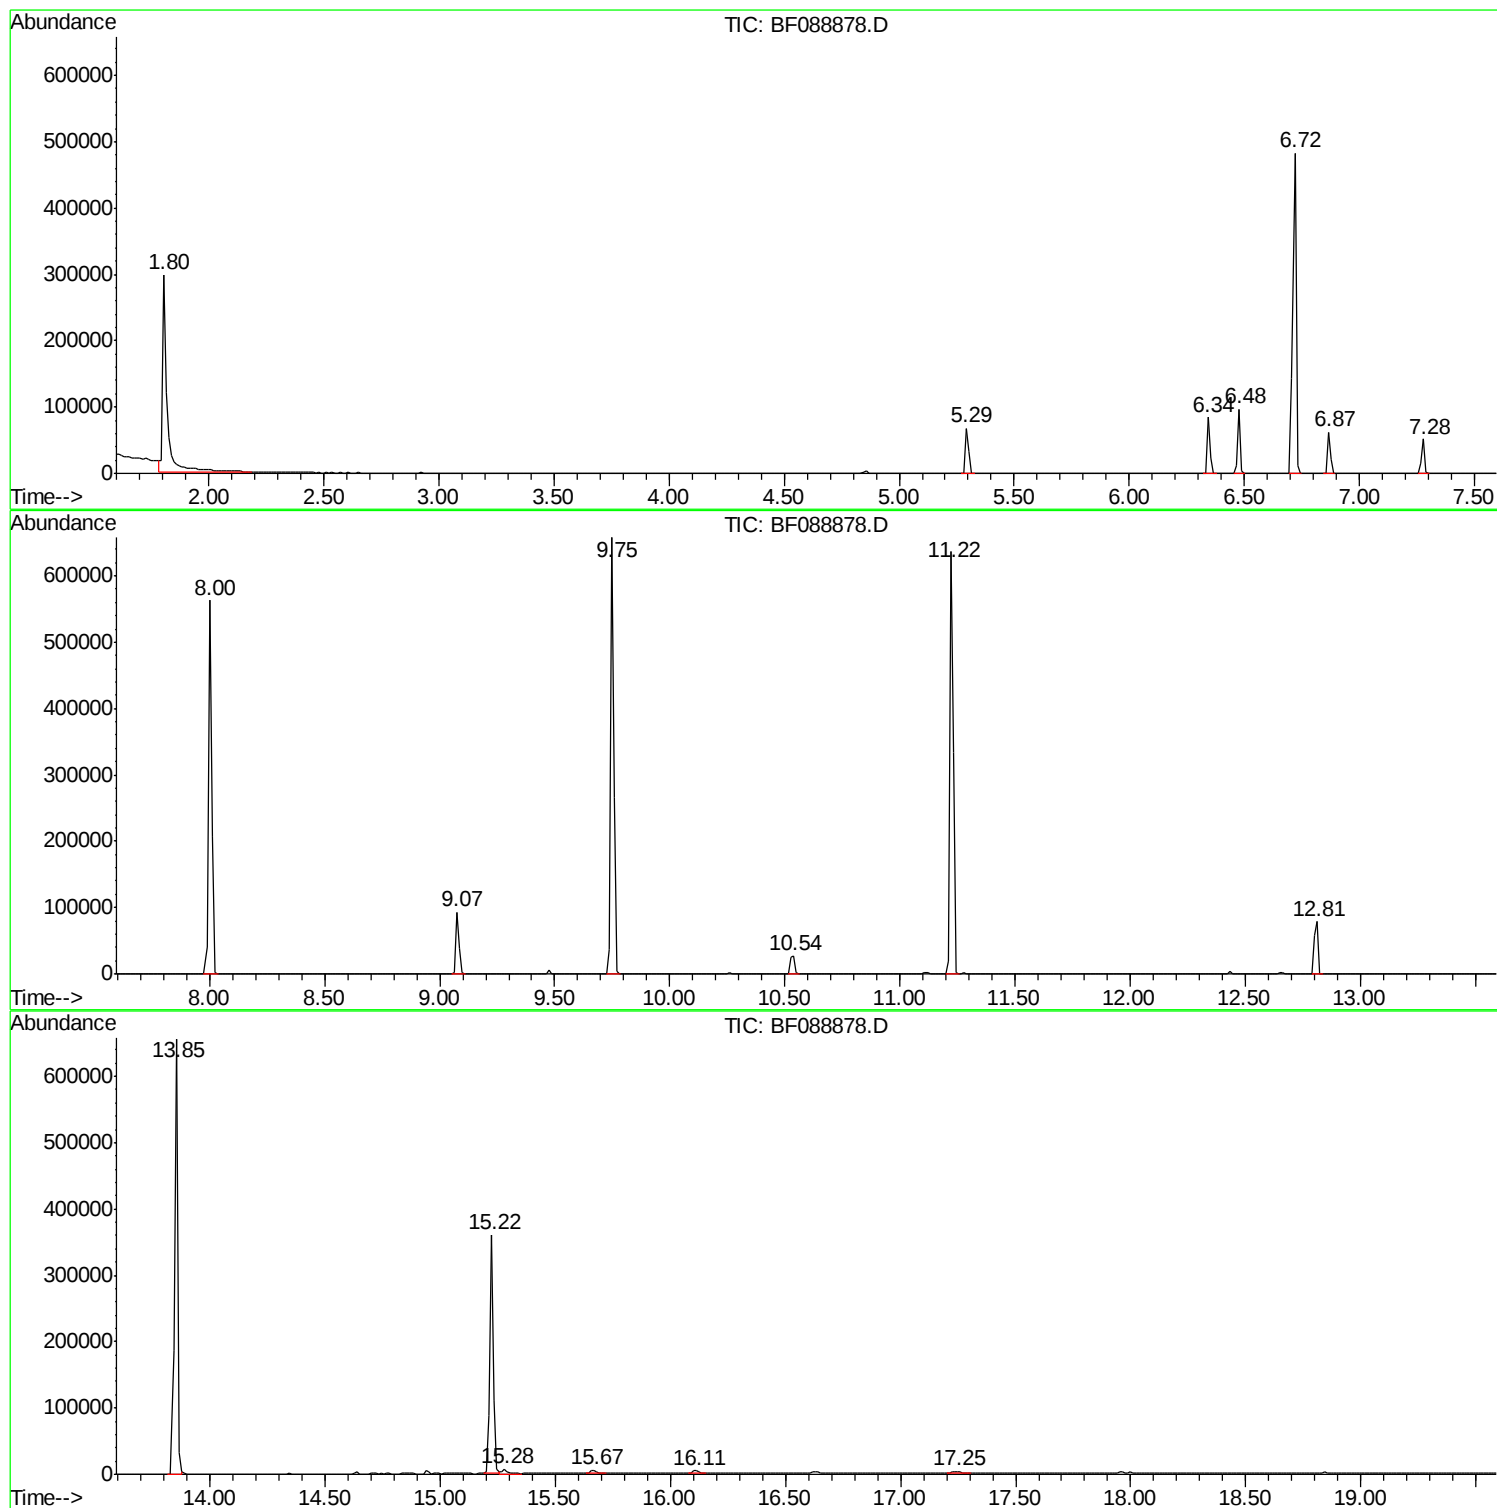

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088878.D
Acq On : 9 Jul 2016 18:35
Operator : UM/SJ
Sample : H3813-11 25X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS002-0006-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	3.54 ng	77513	1,4-Dichlorobenzene-d4	6.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			5-Aminoindole	132	C8H8N2	005192-03-0	10
2			(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	9
3			1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

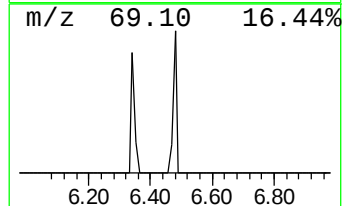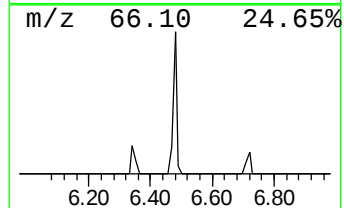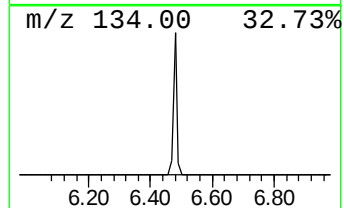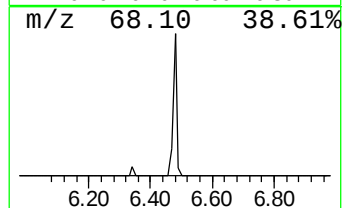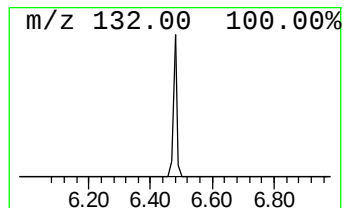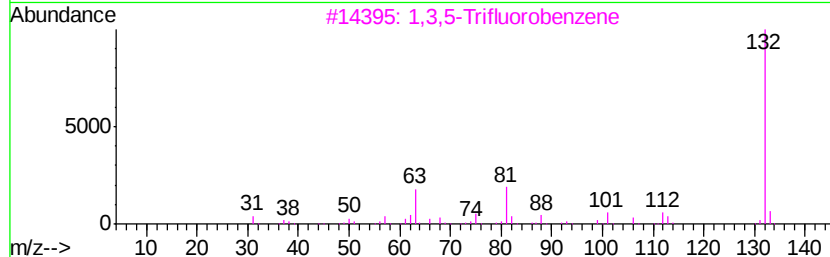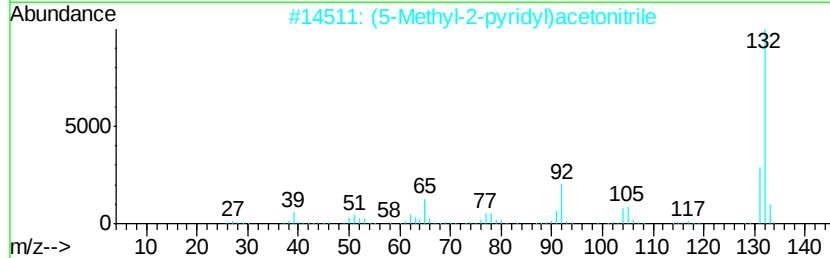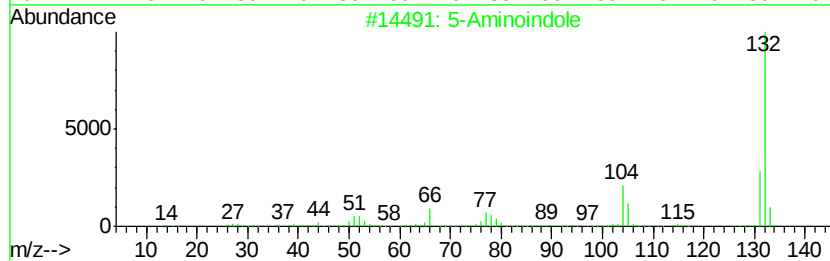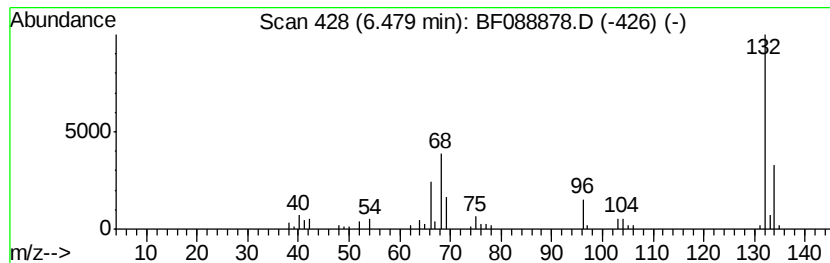

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088878.D
Acq On : 9 Jul 2016 18:35
Operator : UM/SJ
Sample : H3813-11 25X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS002-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	3.5	ng	77513	1	6.72	437829	20.0