

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088884.D
 Acq On : 9 Jul 2016 21:30
 Operator : UM/SJ
 Sample : H3813-17 25X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS005-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.804	17	19	49	rVB	506463	718563	100.00%	15.596%
2	5.301	323	325	327	rBB	54571	70789	9.85%	1.536%
3	6.342	415	416	420	rBB	73158	82434	11.47%	1.789%
4	6.479	426	428	430	rBB	106199	83711	11.65%	1.817%
5	6.719	447	449	451	rBB	537388	444710	61.89%	9.652%
6	6.867	461	462	464	rBB	46352	57779	8.04%	1.254%
7	7.279	496	498	500	rBB	64097	51771	7.20%	1.124%
8	8.010	559	562	564	rBV	464259	590370	82.16%	12.814%
9	9.085	653	656	658	rBV	77761	86052	11.98%	1.868%
10	9.759	712	715	717	rBV	575293	675770	94.04%	14.668%
11	10.536	781	783	785	rBB	46277	40681	5.66%	0.883%
12	11.108	831	833	837	rBV2	5718	8088	1.13%	0.176%
13	11.233	841	844	846	rBV	674721	689144	95.91%	14.958%
14	12.434	947	949	951	rBV	8183	9096	1.27%	0.197%
15	12.662	966	969	970	rBV3	7187	12151	1.69%	0.264%
16	12.697	970	972	974	rVV3	4960	8106	1.13%	0.176%
17	12.811	980	982	984	rBV	89577	74627	10.39%	1.620%
18	12.971	984	996	997	rBV7	13244	62075	8.64%	1.347%
19	13.851	1071	1073	1076	rBV	468617	447020	62.21%	9.703%
20	15.234	1191	1194	1196	rBV	261315	394292	54.87%	8.558%


Sum of corrected areas: 4607229

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088884.D
Acq On : 9 Jul 2016 21:30
Operator : UM/SJ
Sample : H3813-17 25X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS005-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

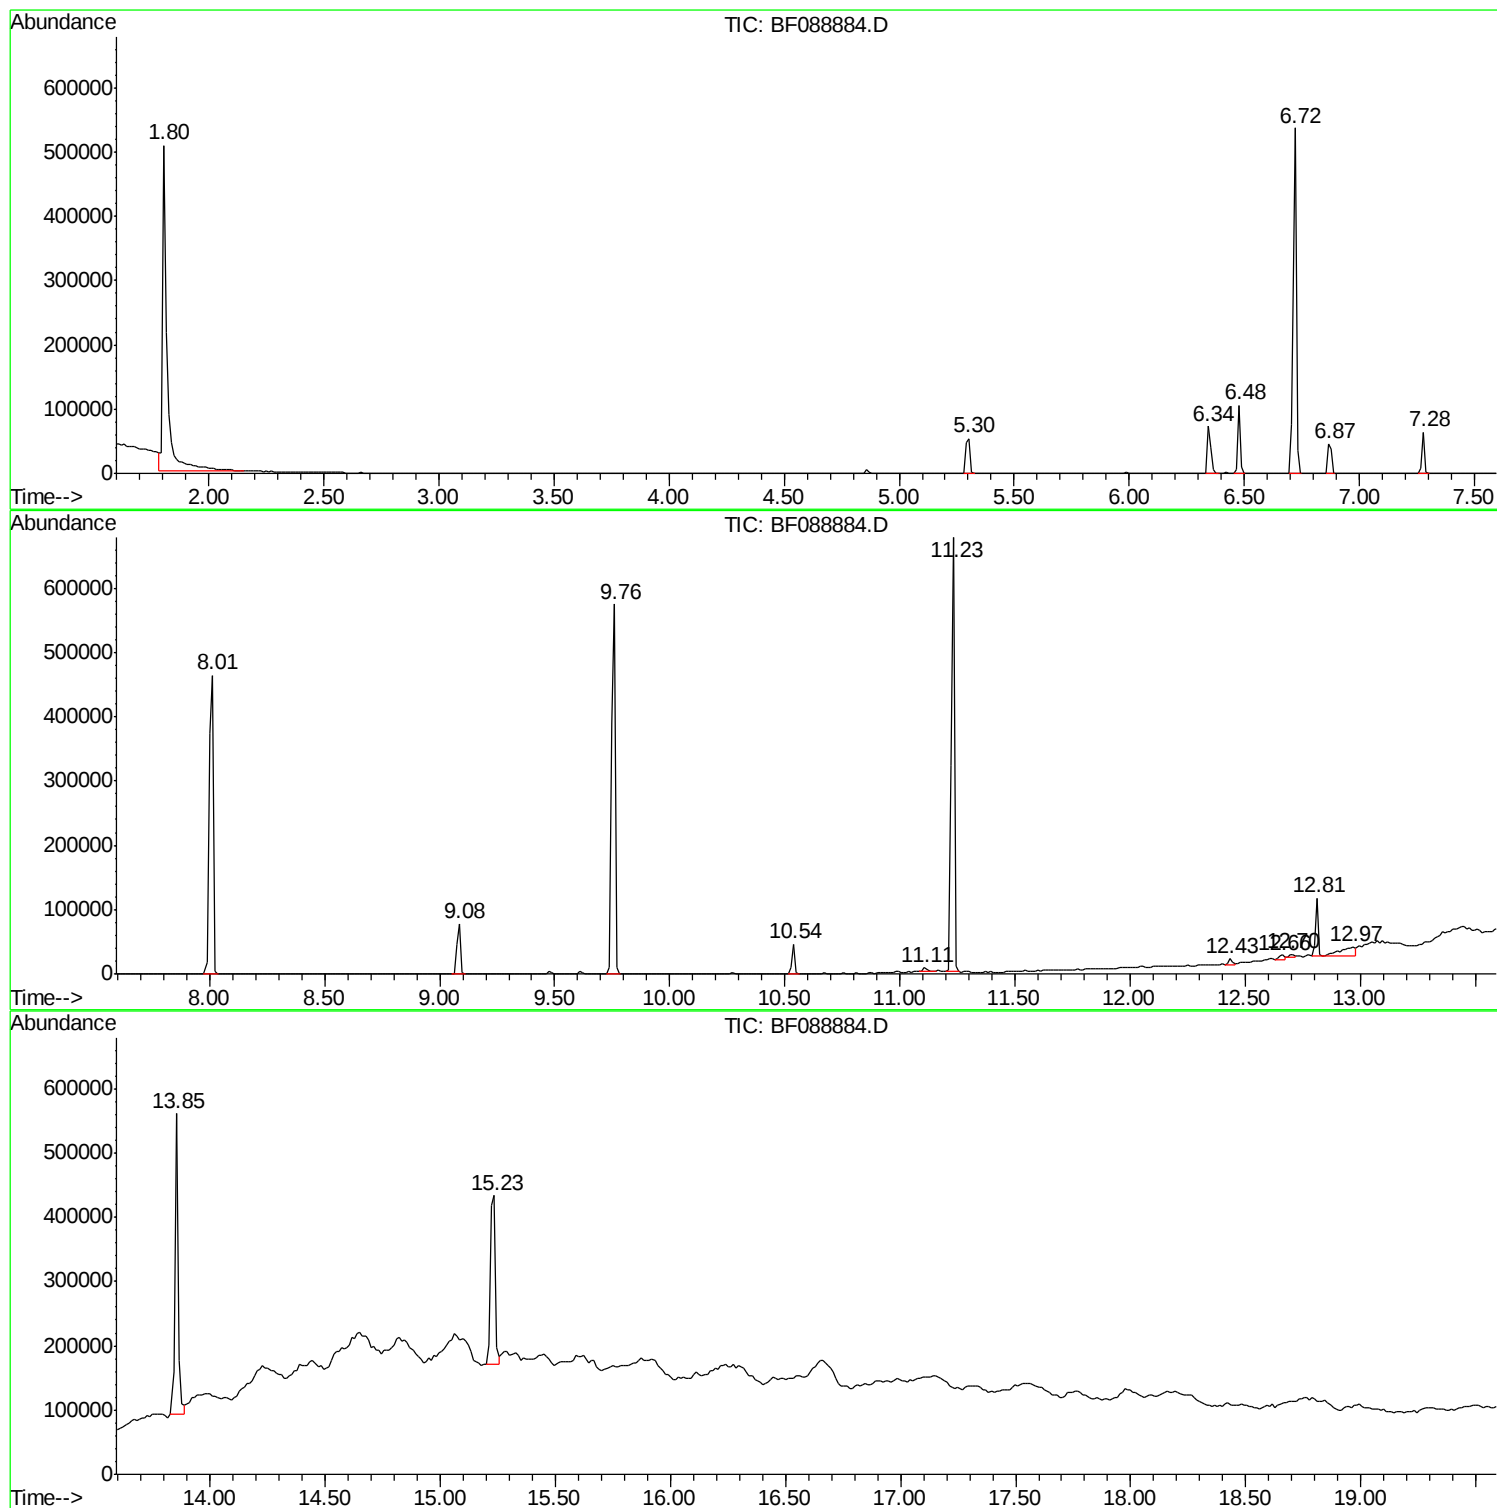

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088884.D
Acq On : 9 Jul 2016 21:30
Operator : UM/SJ
Sample : H3813-17 25X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS005-0006-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.48 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	3.76 ng	83711	1,4-Dichlorobenzene-d4	6.72

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	10
3			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
4			Xenon	132	Xe	007440-63-3	9
5			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

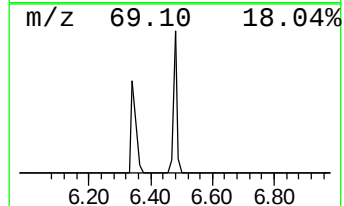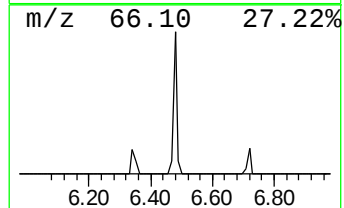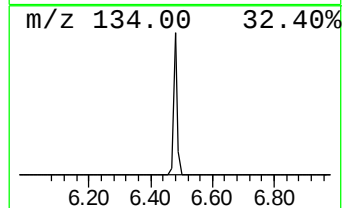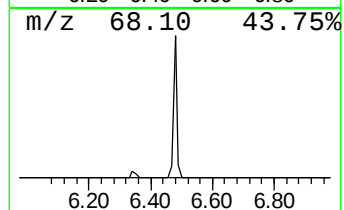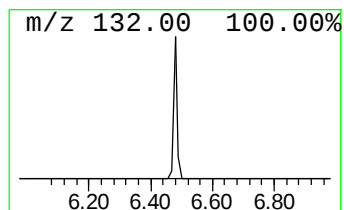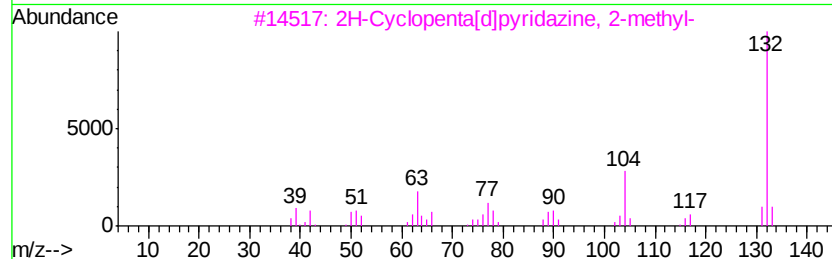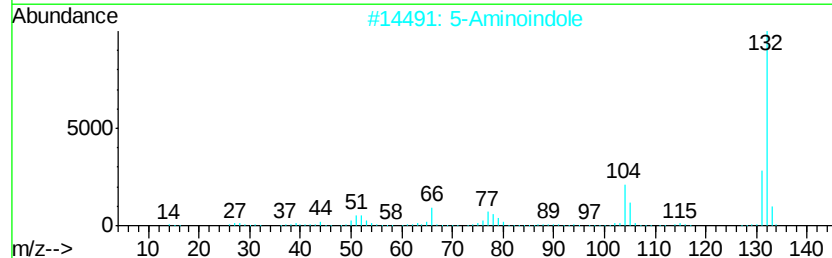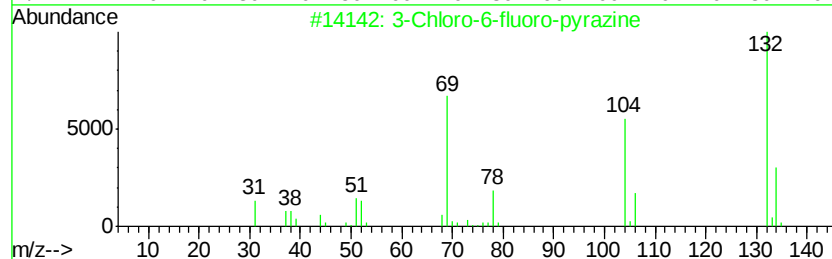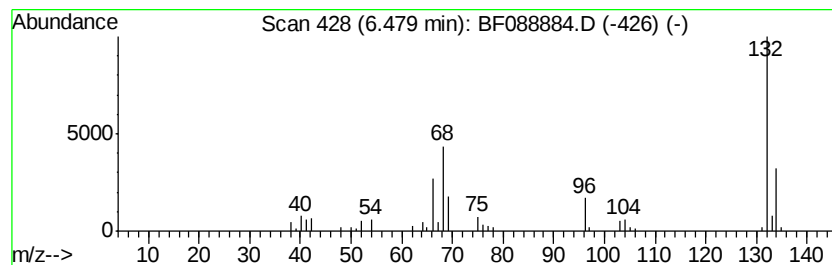

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088884.D
Acq On : 9 Jul 2016 21:30
Operator : UM/SJ
Sample : H3813-17 25X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS005-0006-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown12.97 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.97	2.78 ng	62075	Chrysene-d12	13.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Hydroxy-5-isopropyl-6-methyl-h...	182	C11H18O2	1000187-15-9	22
2		5-Bromopentanoic acid, 1-(cyclop...	276	C12H21BrO2	1000293-35-4	12
3		1-Heptanal, 3,5,5-triethyl-	198	C13H26O	1000160-77-0	10
4		Ethanol, 2-bromo-	124	C2H5BrO	000540-51-2	10
5		Tetratriacontyl heptafluorobutyrate	691	C38H69F7O2	1000351-84-1	9

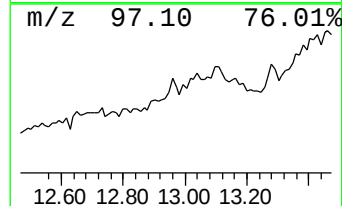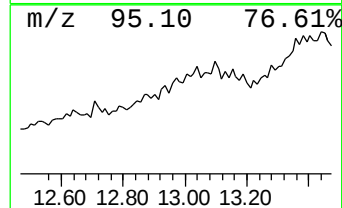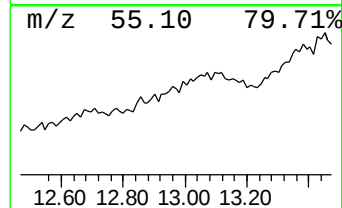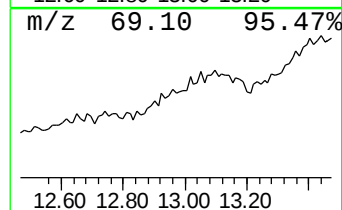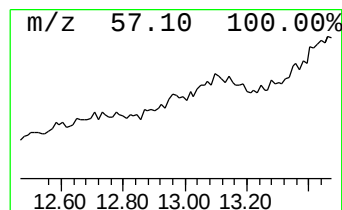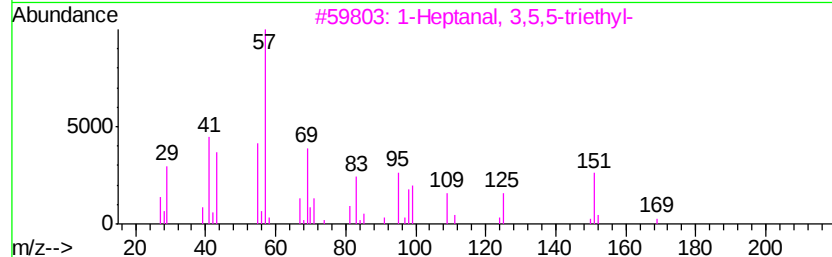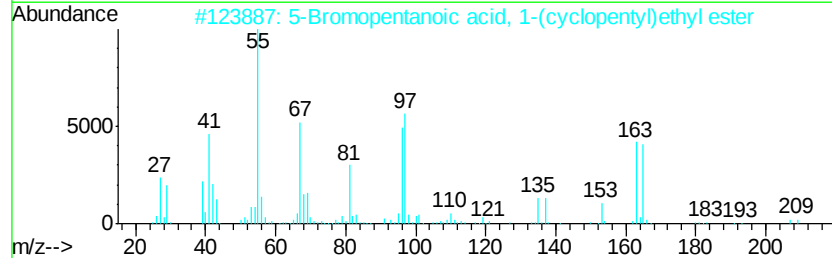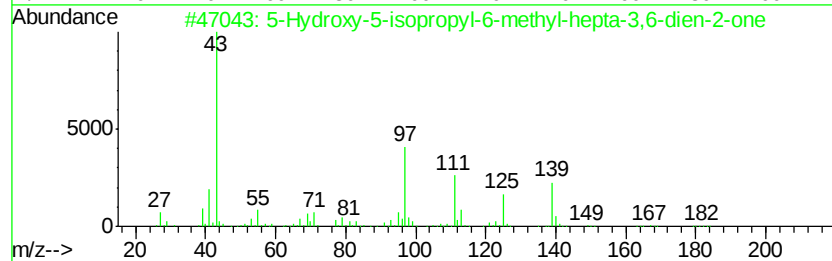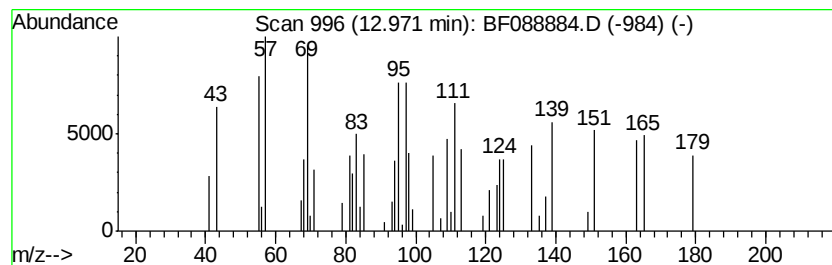

Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
Data File : BF088884.D
Acq On : 9 Jul 2016 21:30
Operator : UM/SJ
Sample : H3813-17 25X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS005-0006-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	3.8	ng	83711	1	6.72	444710	20.0
unknown12.97	12.97	2.8	ng	62075	5	13.85	447020	20.0