


Data Path : V:\HPCHEM1\BNA_F\DATA\BF070916\
 Data File : BF088889.D
 Acq On : 9 Jul 2016 23:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 08 18:51:20 2016

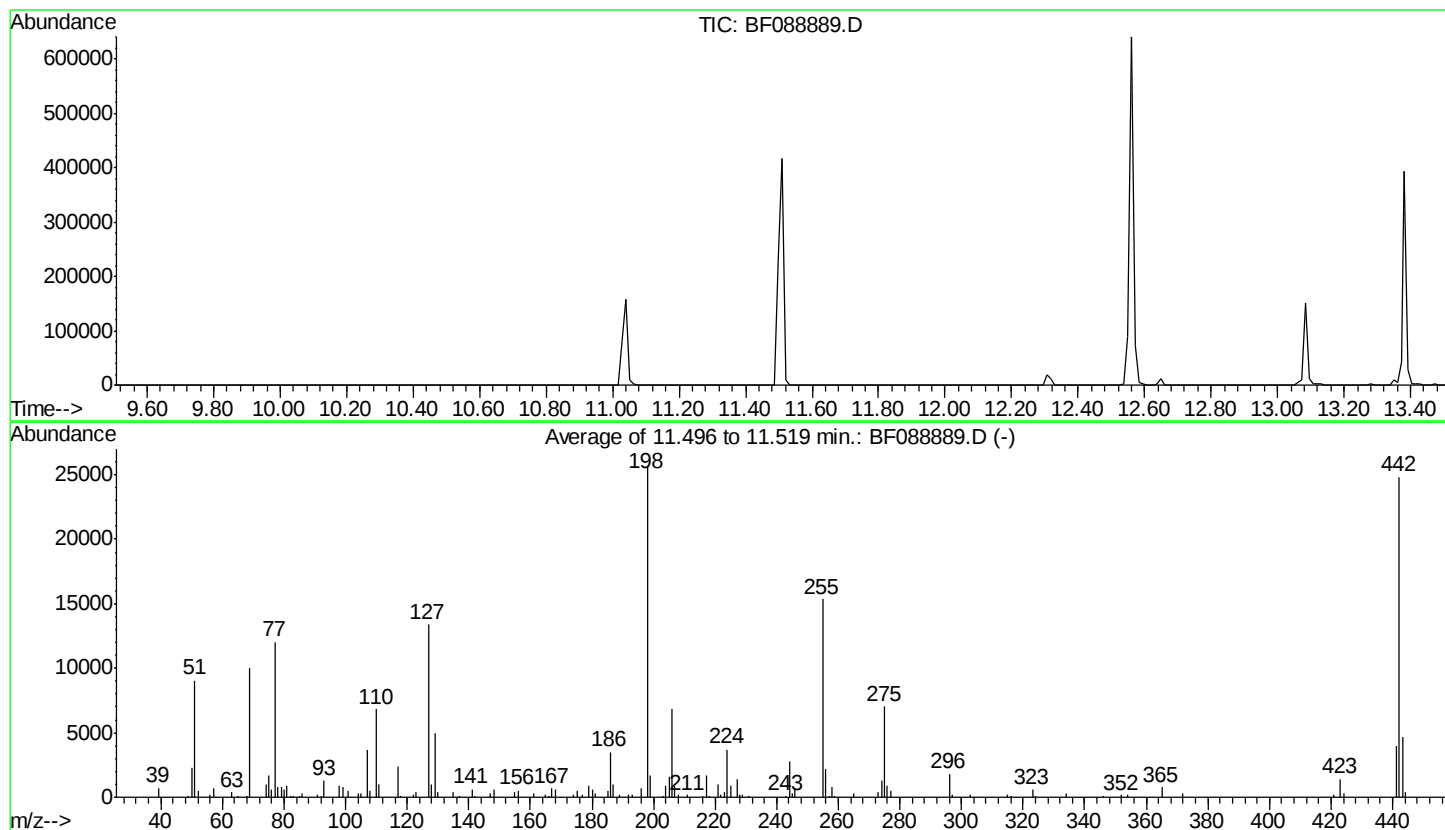

AutoFind: Scans 867, 868, 869; Background Corrected with Scan 864

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	9079	PASS
68	69	0.00	2	1.2	124	PASS
69	198	0.00	100	39.0	10026	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	13386	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25706	PASS
199	198	5	9	6.7	1729	PASS
275	198	10	60	27.4	7033	PASS
365	198	1	100	2.9	751	PASS
441	442	0.01	24	16.1	3988	PASS
442	198	50	100	96.6	24829	PASS
443	442	15	24	19.0	4714	PASS