
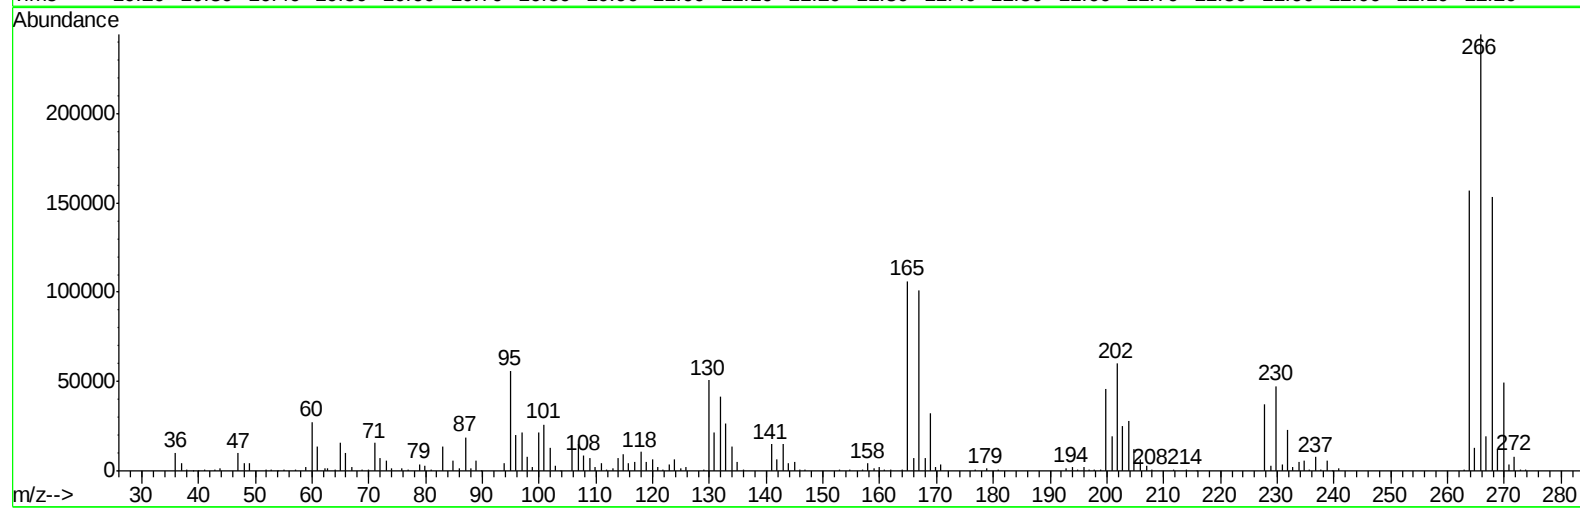


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070919\  
Data File : BF115432.D  
Acq On : 9 Jul 2019 13:51  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 06:29:06 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 09 16:29:09 2019  
Response via : Initial Calibration

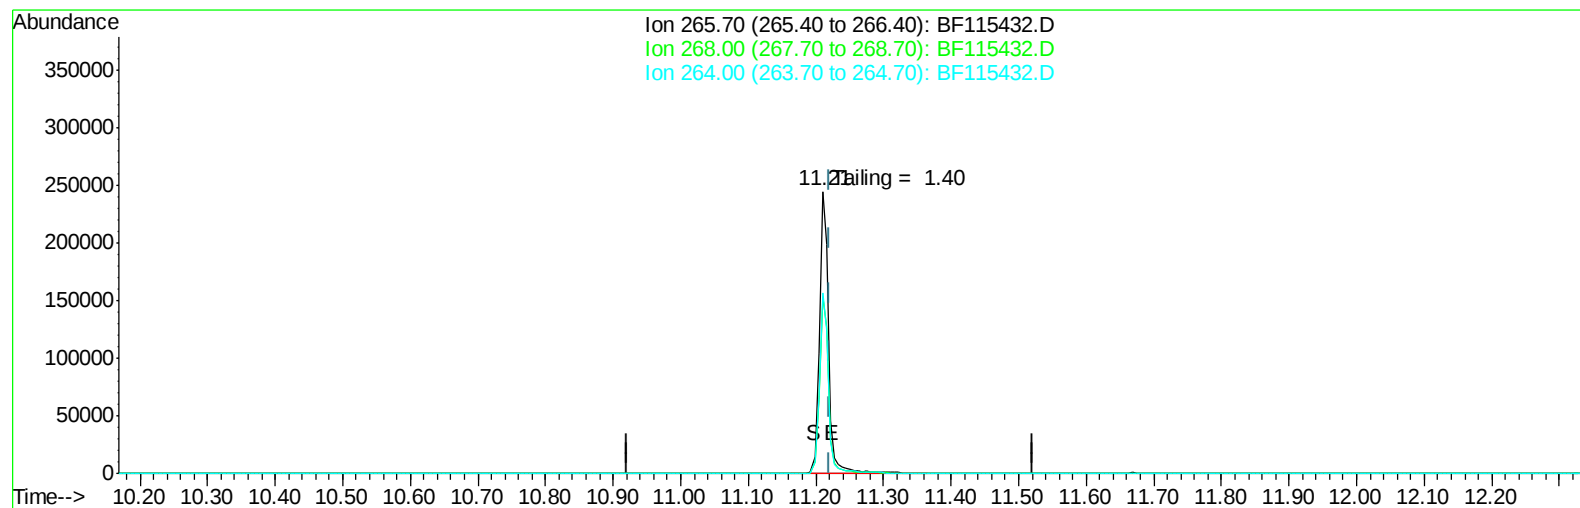

TIC: BF115432.D

(70) Pentachlorophenol (C)



11.210min (-0.012) 28542.04ng

response 233031

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.50 | 62.81 |
| 264.00 | 63.10 | 64.25 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070919\  
Data File : BF115432.D  
Acq On : 9 Jul 2019 13:51  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 06:29:06 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 09 16:29:09 2019  
Response via : Initial Calibration

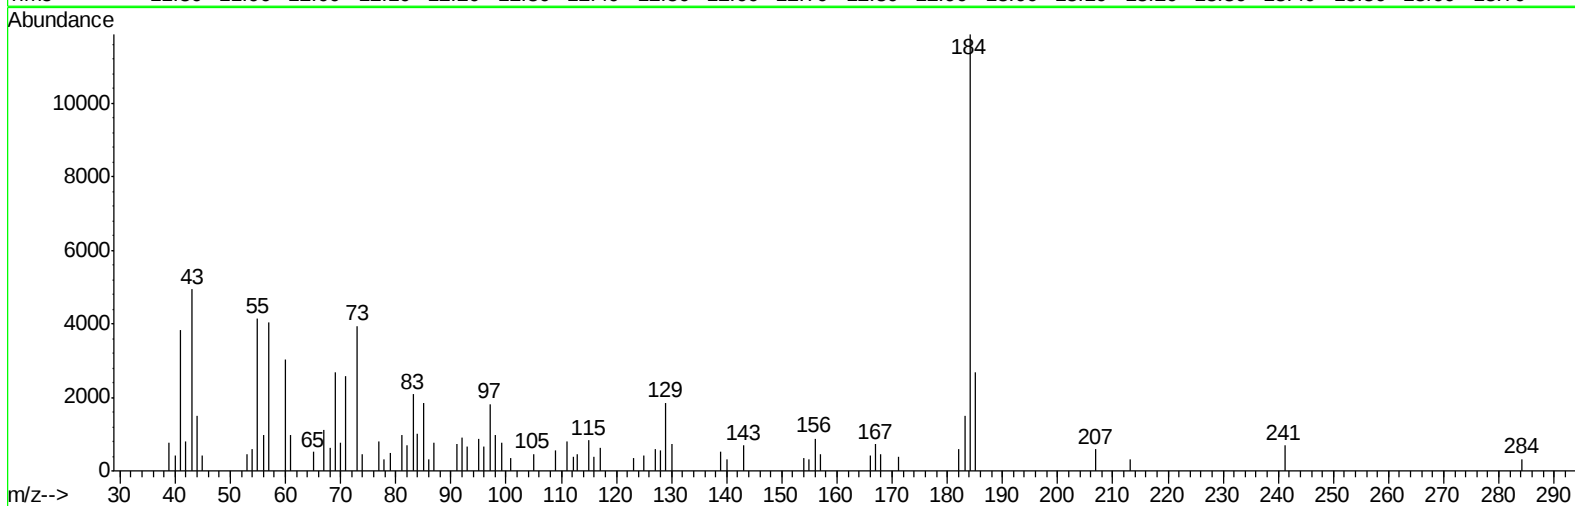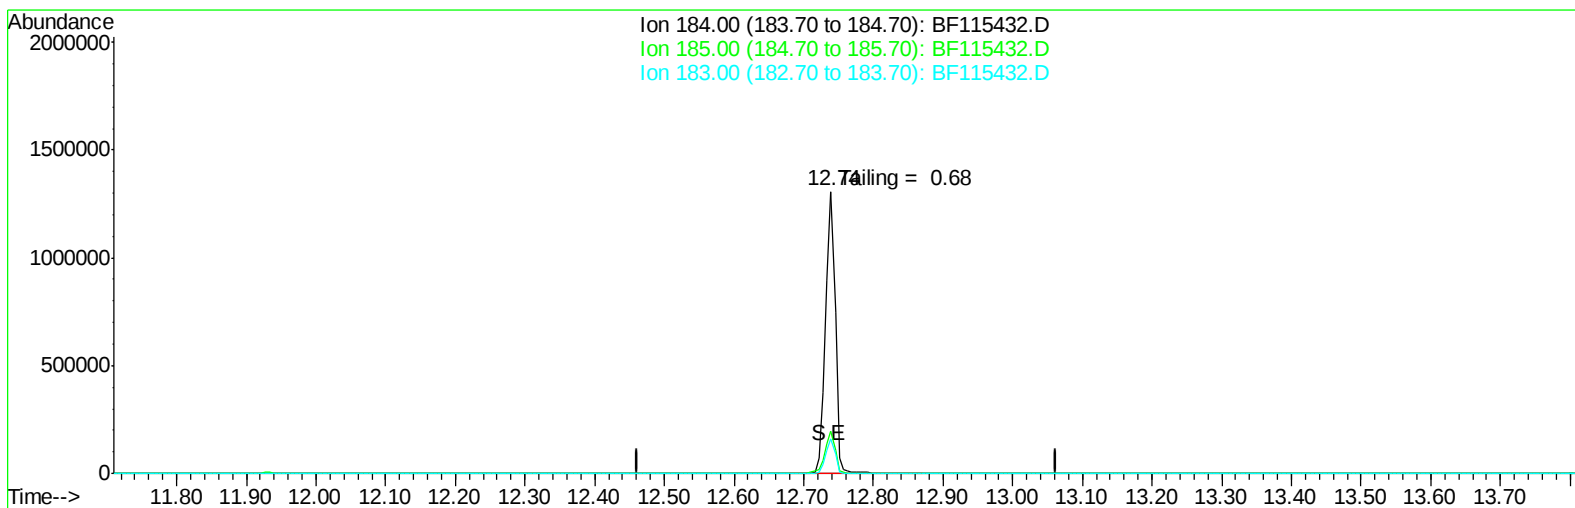

TIC: BF115432.D

(77) Benzidine

12.763min (-12.763) 0.00ng

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 0.00  |
| 185.00 | 16.80 | 0.00# |
| 183.00 | 11.70 | 0.00# |
| 0.00   | 0.00  | 0.00  |