


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070919\
 Data File : BF115432.D
 Acq On : 9 Jul 2019 13:51
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 09 16:29:09 2019

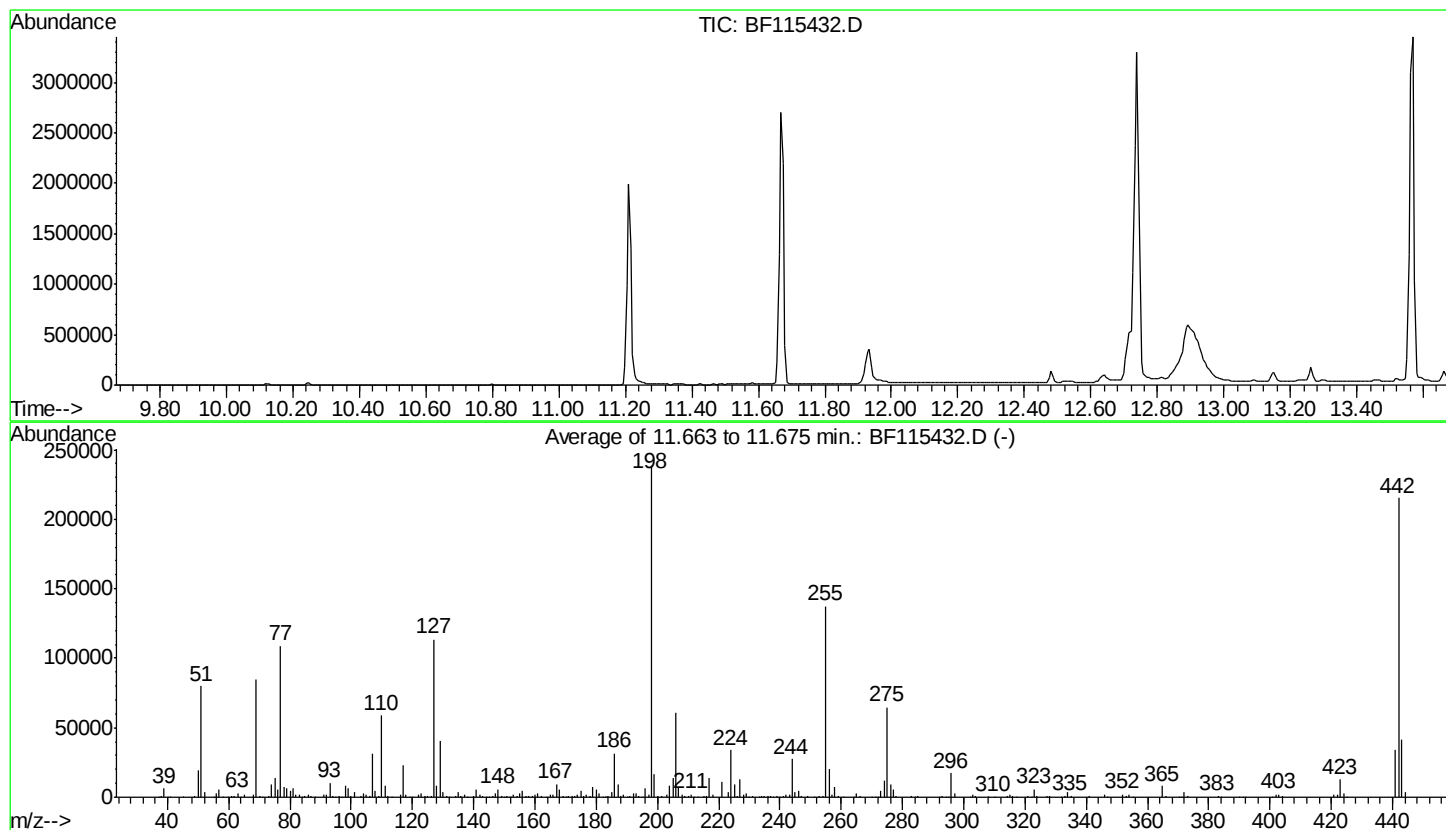

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	79930	PASS
68	69	0.00	2	1.9	1605	PASS
69	198	0.00	100	35.5	84715	PASS
70	69	0.00	2	0.8	686	PASS
127	198	10	80	47.5	113389	PASS
197	198	0.00	2	0.7	1560	PASS
198	198	100	100	100.0	238570	PASS
199	198	5	9	6.8	16251	PASS
275	198	10	60	27.2	64832	PASS
365	198	1	100	3.3	7953	PASS
441	198	0.01	100	14.2	33793	PASS
442	198	50	100	90.2	215106	PASS
443	442	15	24	19.3	41621	PASS