


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070920\
 Data File : BF120805.D
 Acq On : 9 Jul 2020 8:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 18:51:52 2020

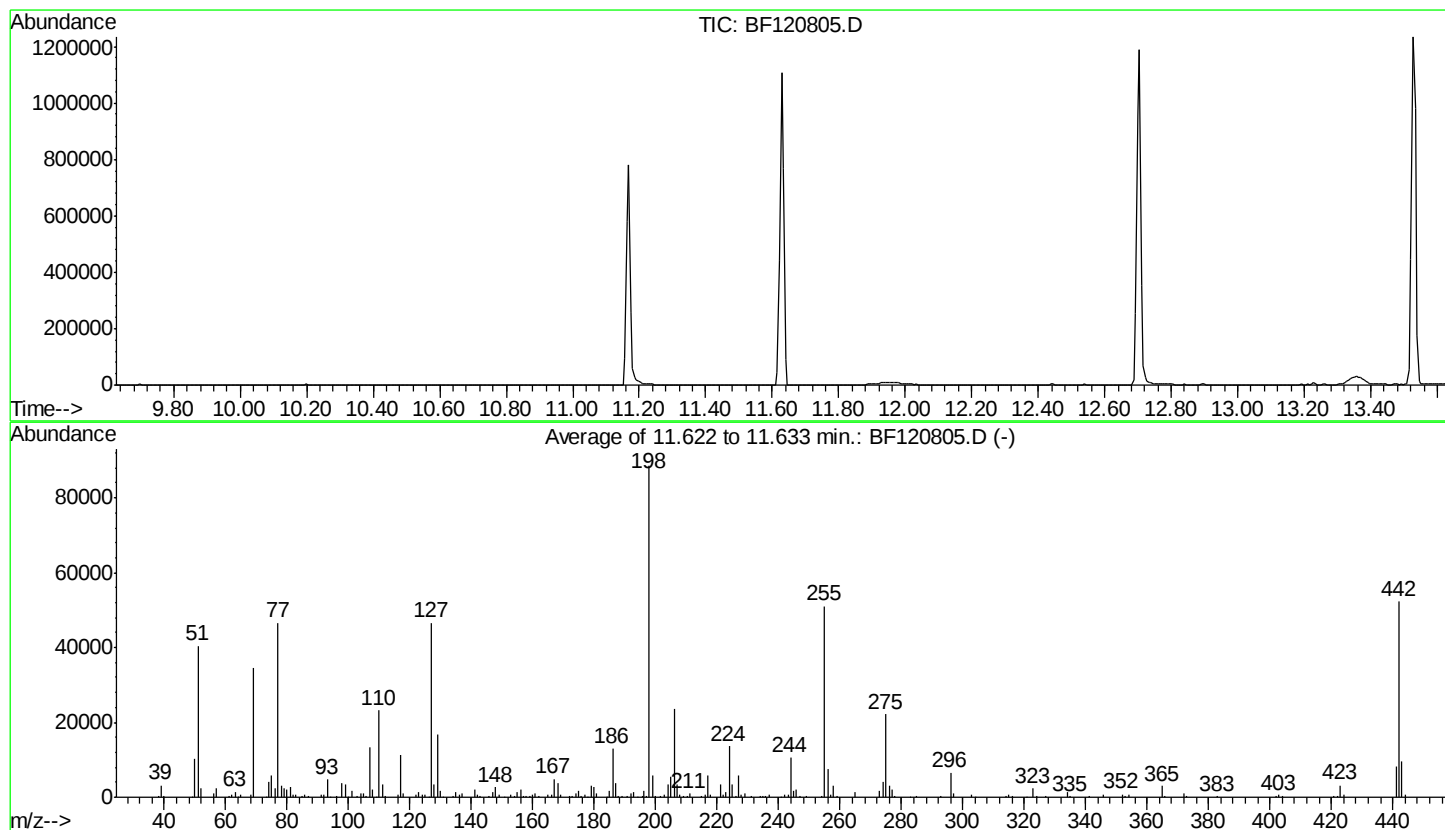

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	40474	PASS
68	69	0.00	2	1.5	531	PASS
69	198	0.00	100	38.9	34461	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	46562	PASS
197	198	0.00	2	0.5	425	PASS
198	198	100	100	100.0	88602	PASS
199	198	5	9	6.7	5938	PASS
275	198	10	60	24.9	22092	PASS
365	198	1	100	3.4	3031	PASS
441	198	0.01	100	9.3	8216	PASS
442	198	50	100	59.1	52322	PASS
443	442	15	24	18.7	9759	PASS