
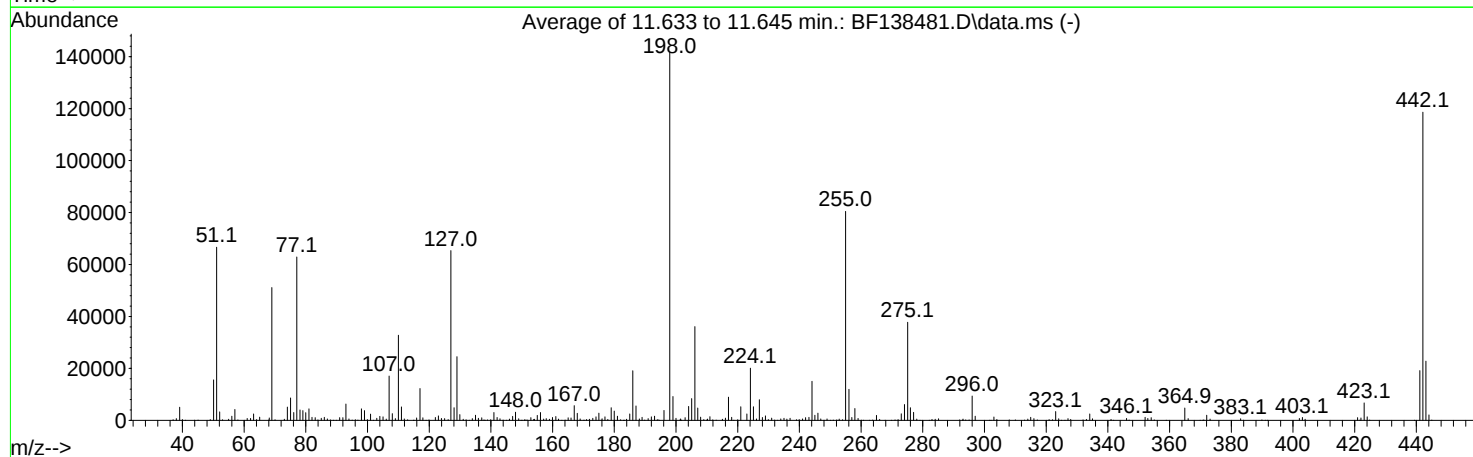


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070924\
Data File : BF138481.D
Acq On : 09 Jul 2024 11:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

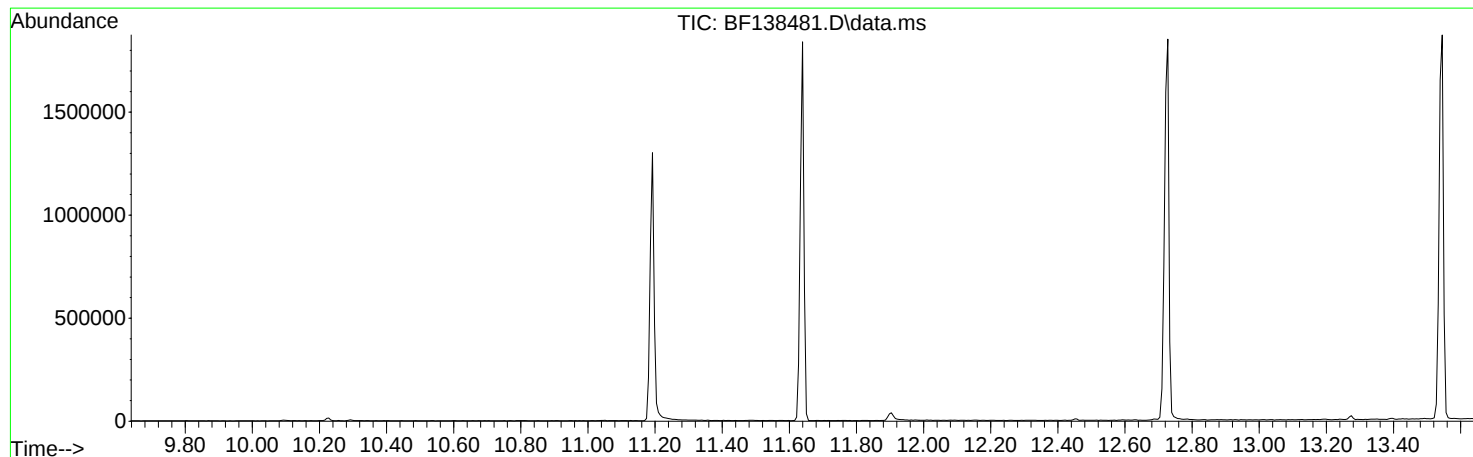




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	66621	PASS
68	69	0.00	2	1.8	935	PASS
69	198	0.00	100	36.1	51097	PASS
70	69	0.00	2	0.5	231	PASS
127	198	10	80	46.2	65381	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141605	PASS
199	198	5	9	6.5	9160	PASS
275	198	10	60	26.7	37776	PASS
365	198	1	100	3.4	4753	PASS
441	198	0.01	100	13.5	19185	PASS
442	442	50	100	100.0	118605	PASS
443	442	15	24	19.2	22798	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070924\
Data File : BF138481.D
Acq On : 09 Jul 2024 11:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 09 13:04:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

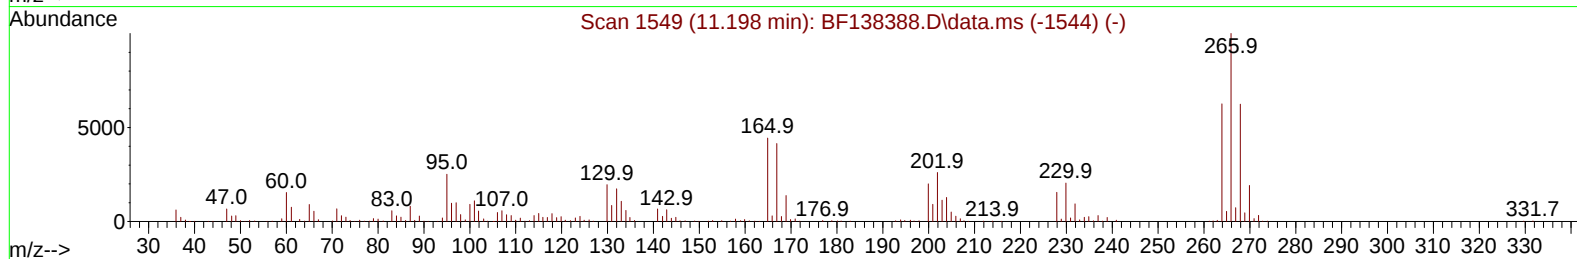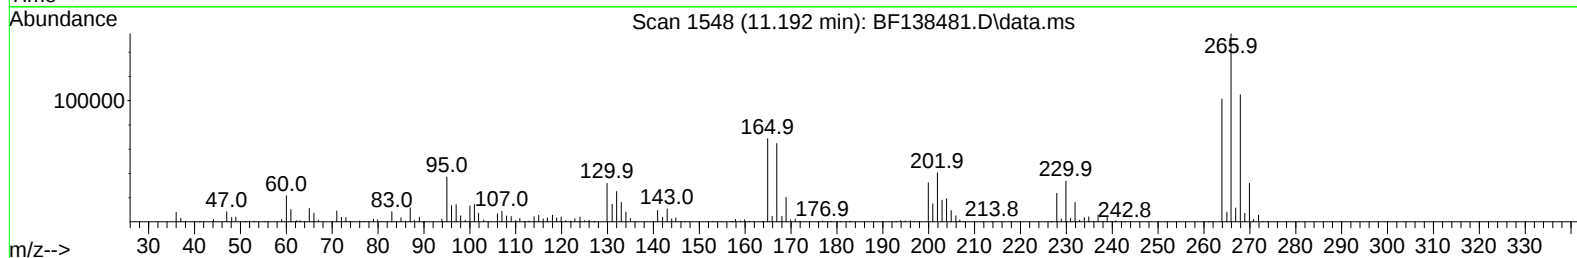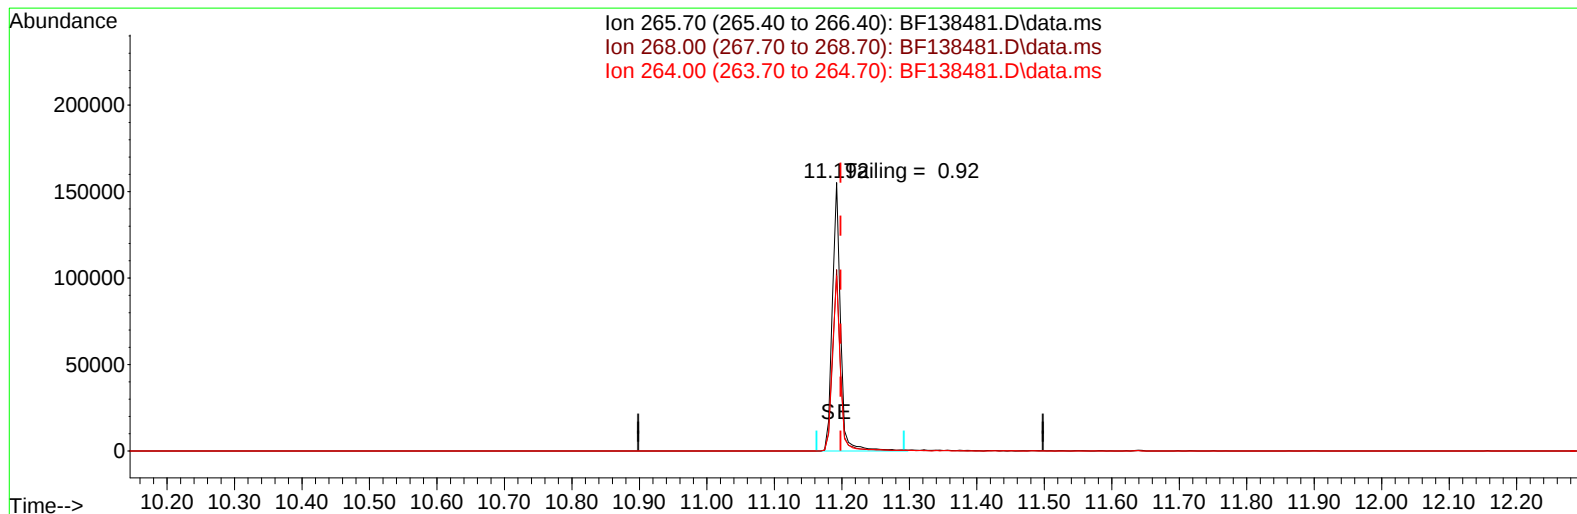

TIC: BF138481.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 39076.74 ng




response 131113

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	67.57
264.00	62.50	65.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070924\
Data File : BF138481.D
Acq On : 09 Jul 2024 11:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 09 13:04:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

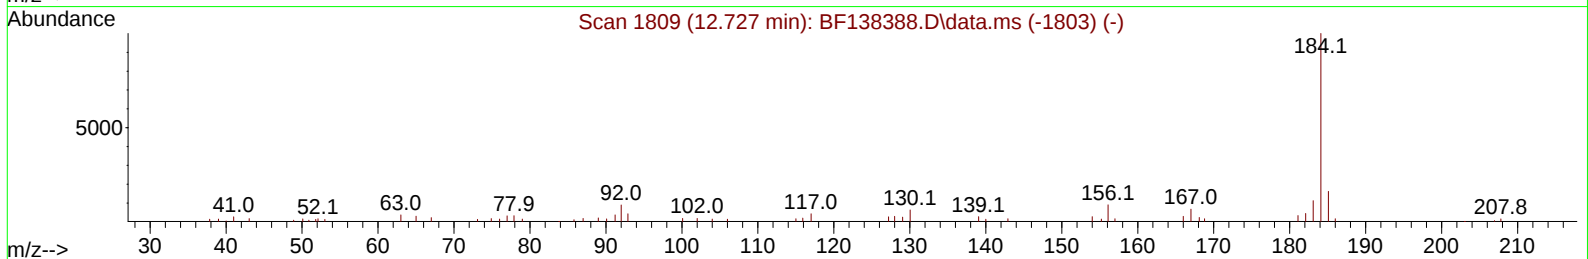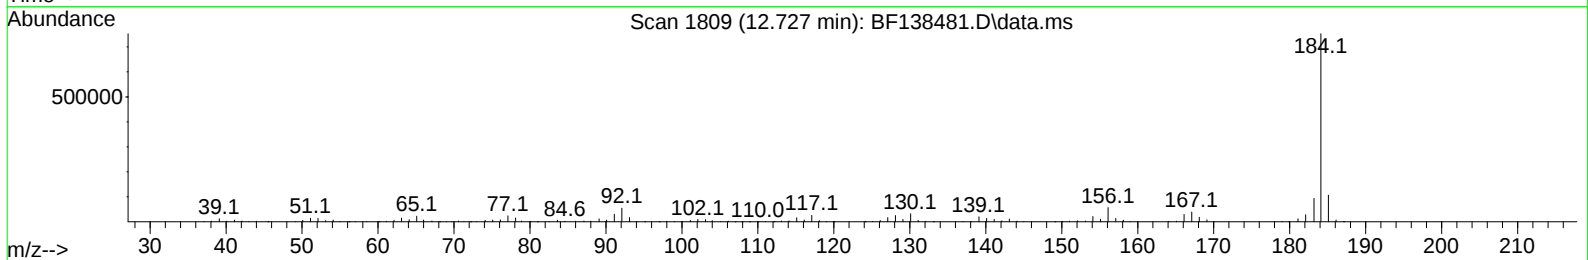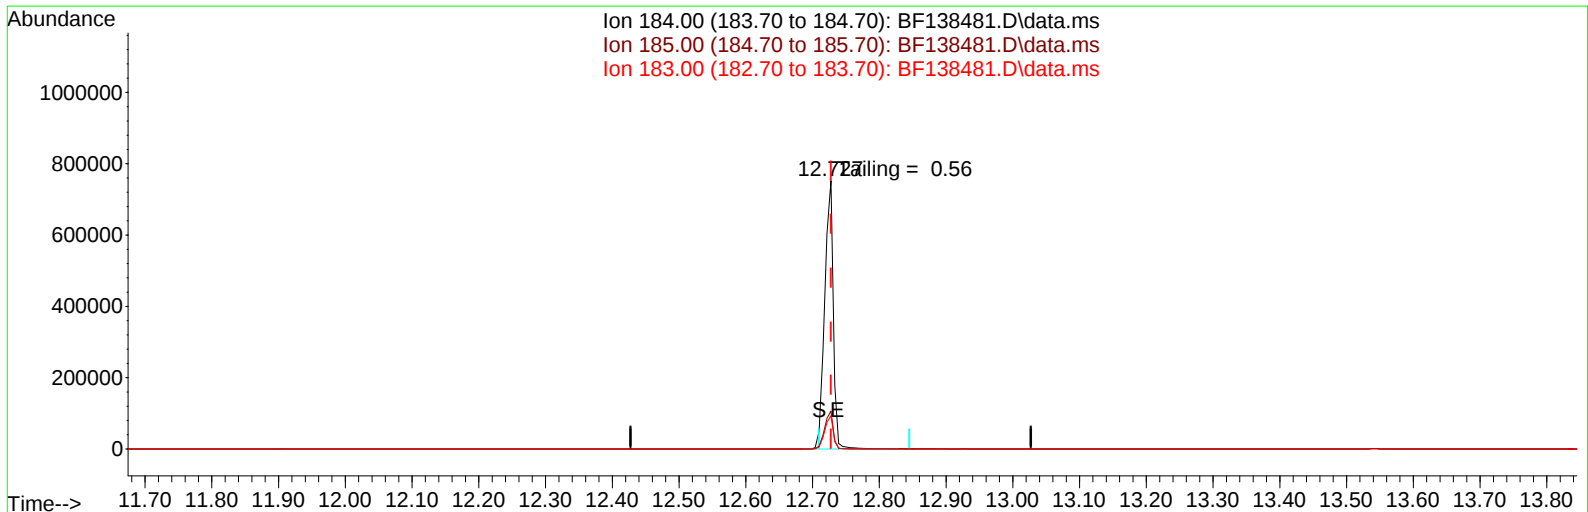

TIC: BF138481.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 1511119.34 ng

response 652509

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.15
183.00	11.30	12.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/9/2024	BNA_F	<u>BF138481.D</u>
Compound Name	Response	Retention Time
DDT	312473	13.545
DDD	3931	13.274
DDE	188	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4119	316592	1.30

Instrument :
BNA_F
ClientSampleId :
DFTPP