
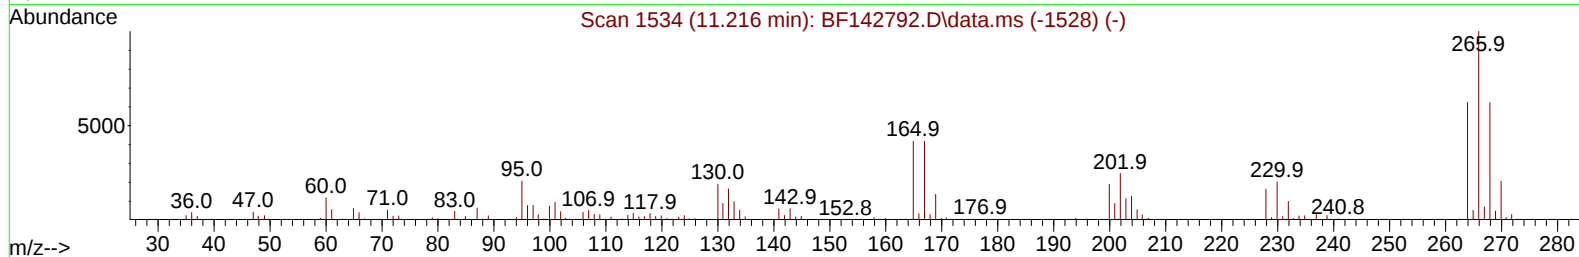
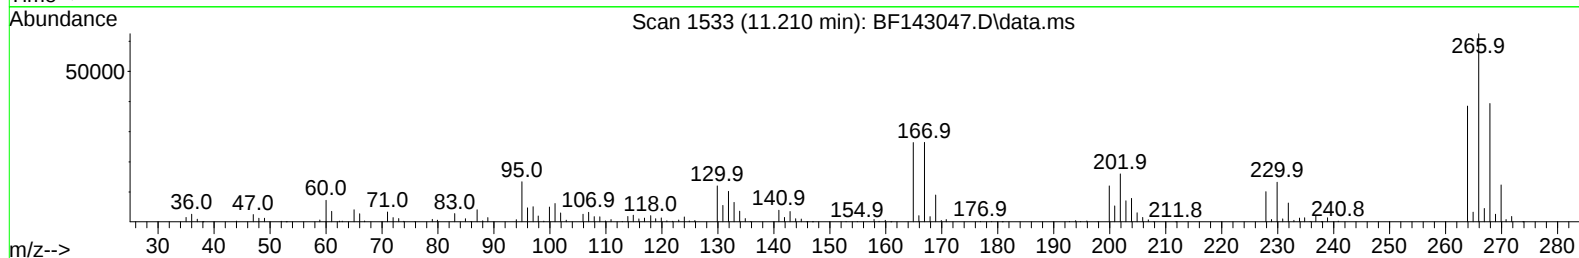


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
Data File : BF143047.D
Acq On : 09 Jul 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 11:29:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

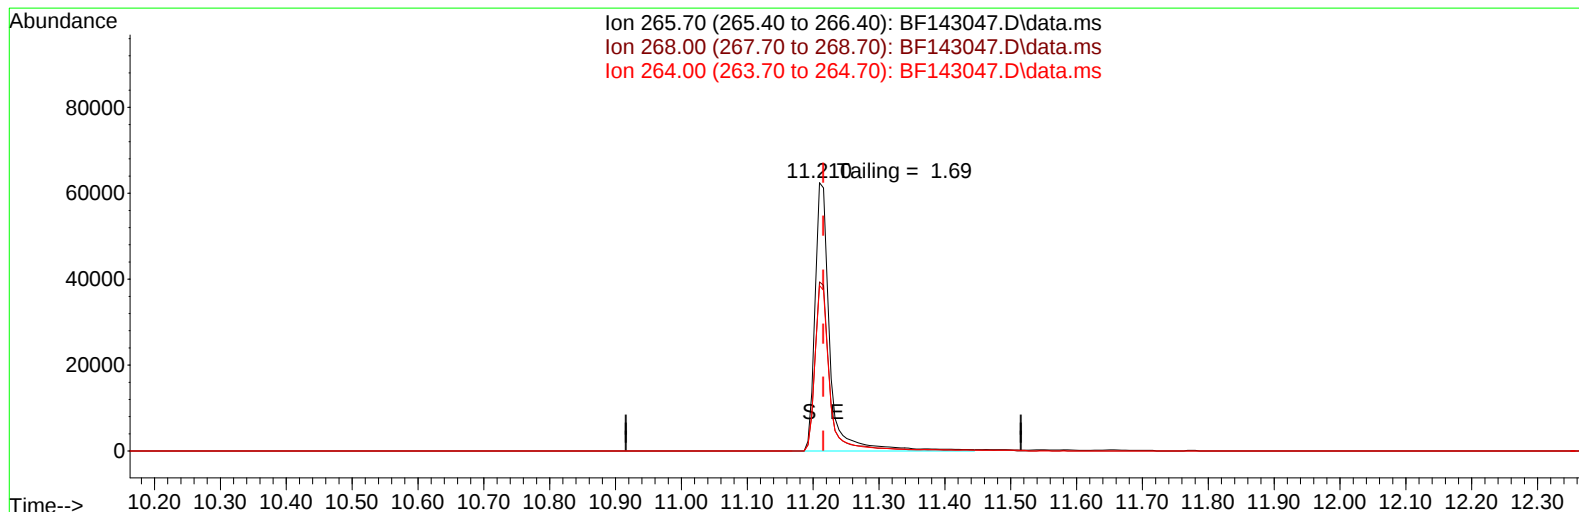

TIC: BF143047.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 48733.15 ng

response 96735

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.02
264.00	62.40	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
Data File : BF143047.D
Acq On : 09 Jul 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 11:29:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 24 05:28:21 2025
Response via : Initial Calibration

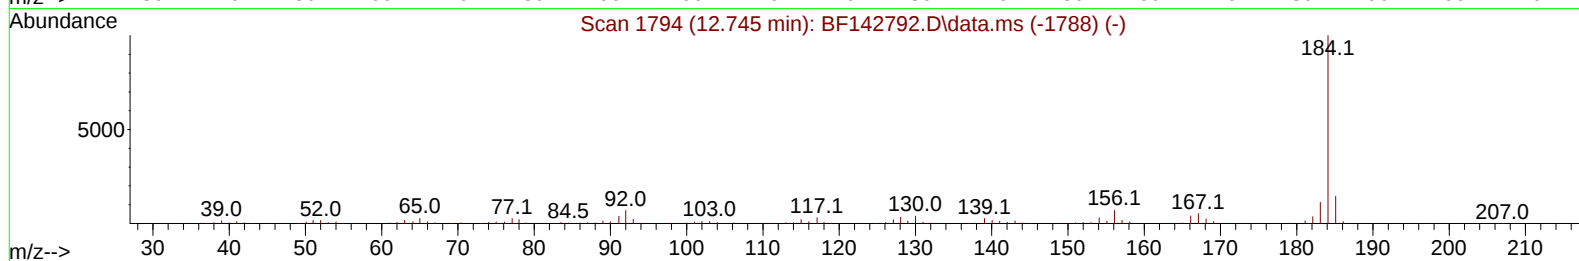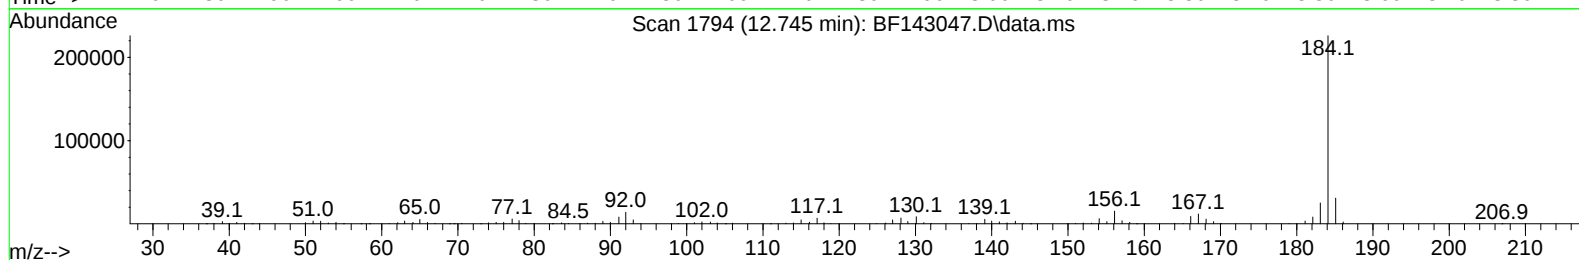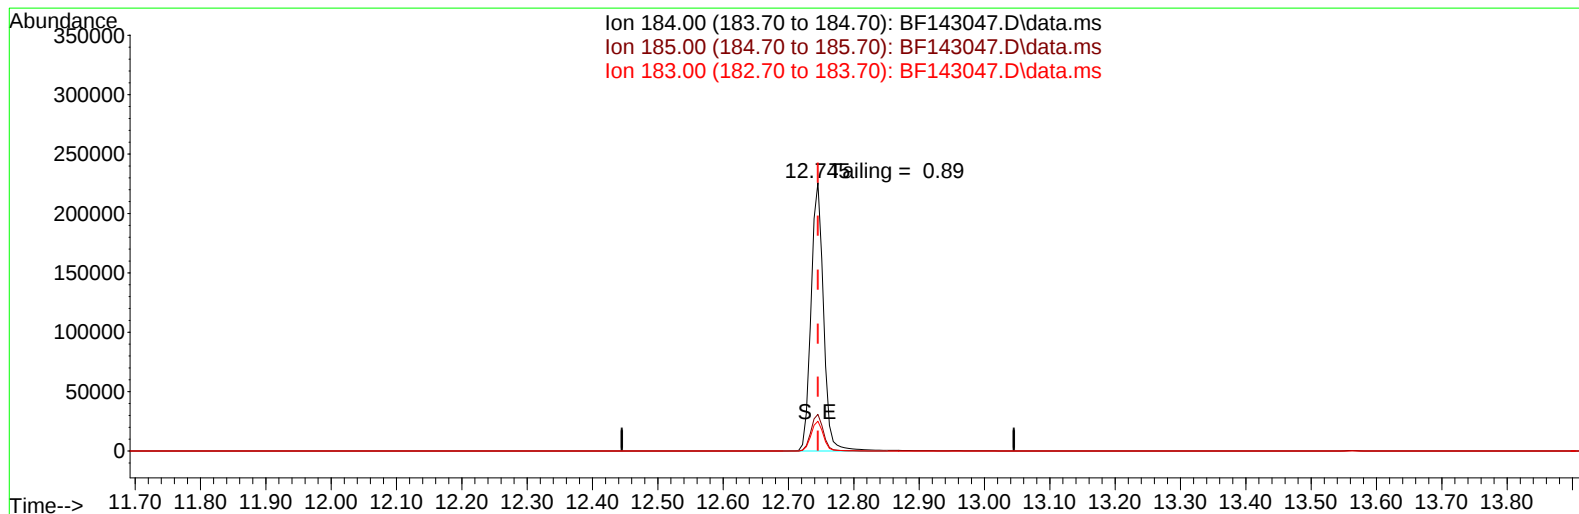

TIC: BF143047.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 301867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.67
183.00	11.20	11.11
0.00	0.00	0.00