

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
 Data File : BF143051.D
 Acq On : 09 Jul 2025 12:24
 Operator : RC/JU
 Sample : PB168750BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB168750BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	489	495	507	rBV	86696	145859	7.32%	1.285%
2	5.504	557	563	590	rBV	1103137	1500623	75.31%	13.220%
3	6.504	727	733	752	rBV	1065058	1482743	74.41%	13.063%
4	6.869	790	795	802	rBV	265000	321828	16.15%	2.835%
5	7.434	885	891	906	rBV	701839	968008	48.58%	8.528%
6	8.157	1008	1014	1038	rVB	324356	424016	21.28%	3.736%
7	9.233	1190	1197	1202	rBV	1550945	1992558	100.00%	17.554%
8	9.916	1307	1313	1325	rVB	368746	486203	24.40%	4.283%
9	10.704	1442	1447	1468	rBV	858331	1149411	57.69%	10.126%
10	11.404	1561	1566	1574	rBV	392252	488158	24.50%	4.301%
11	12.992	1830	1836	1841	rBV	1374809	1763136	88.49%	15.533%
12	14.051	2011	2016	2025	rBV	217237	281839	14.14%	2.483%
13	15.545	2264	2270	2281	rBV	184765	300992	15.11%	2.652%
14	17.139	2535	2541	2551	rVB6	8701	24549	1.23%	0.216%
15	18.027	2686	2692	2703	rVB8	6381	20966	1.05%	0.185%




Sum of corrected areas: 11350889

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
Data File : BF143051.D
Acq On : 09 Jul 2025 12:24
Operator : RC/JU
Sample : PB168750BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168750BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

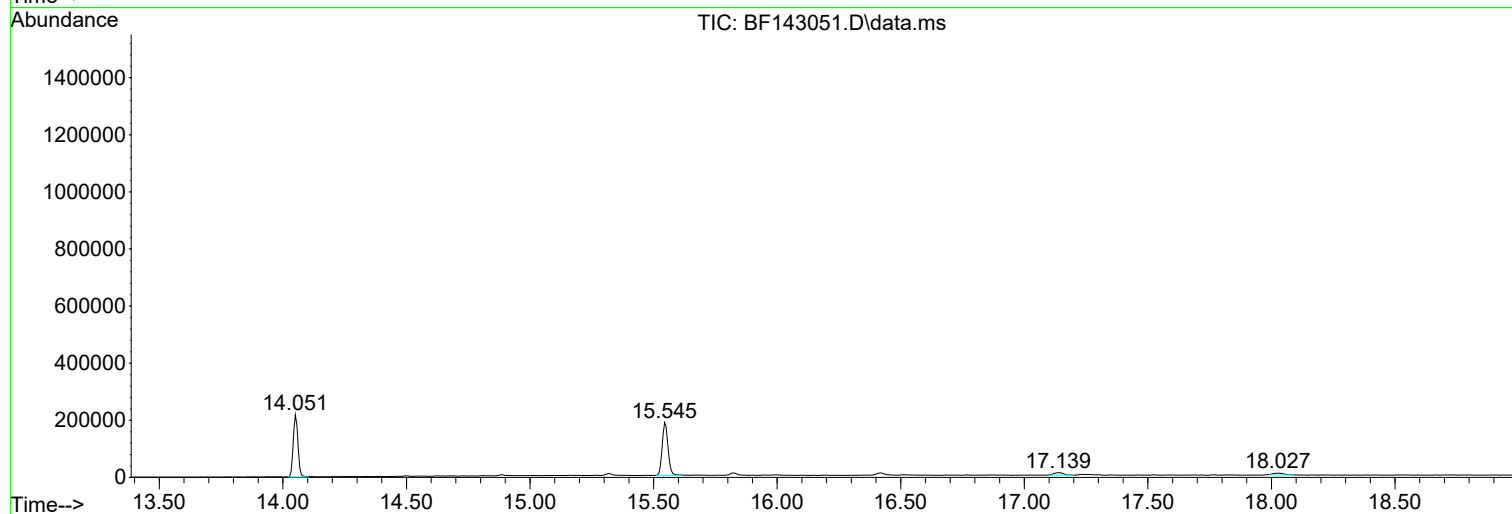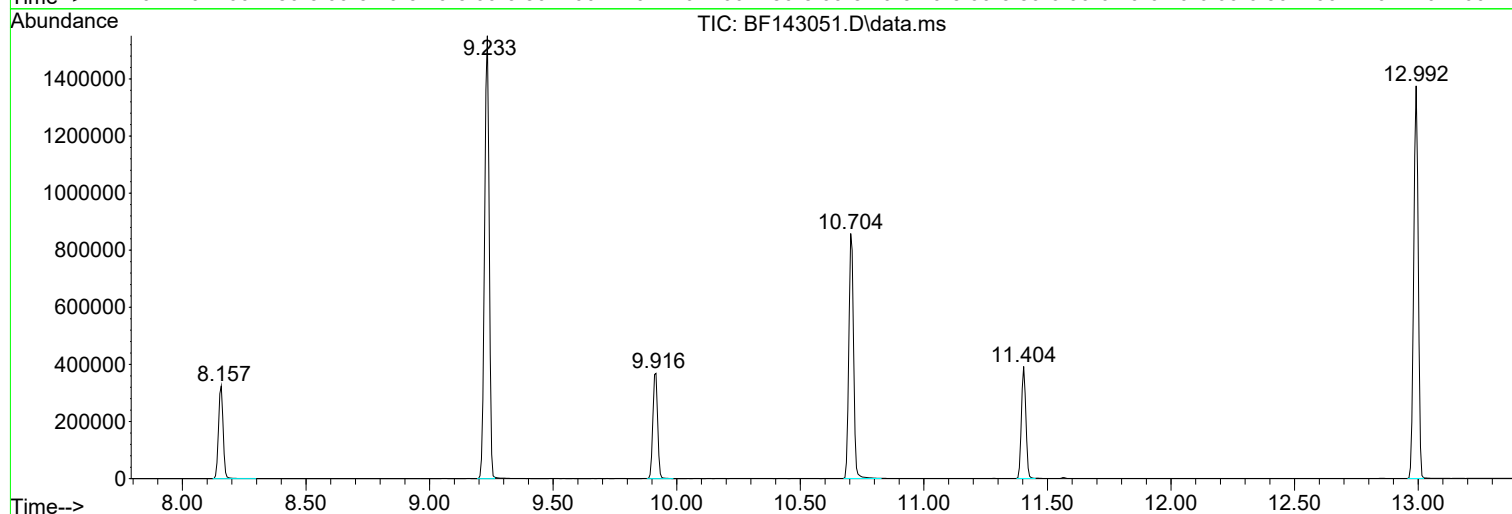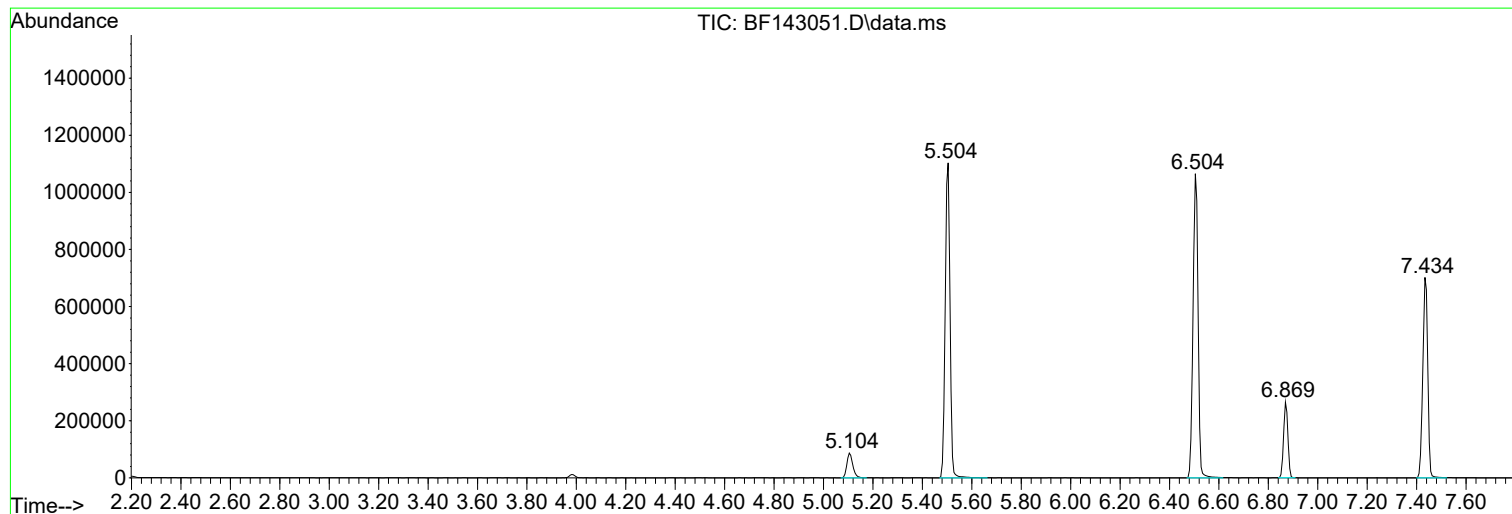

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
Data File : BF143051.D
Acq On : 09 Jul 2025 12:24
Operator : RC/JU
Sample : PB168750BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168750BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070925\
Data File : BF143051.D
Acq On : 09 Jul 2025 12:24
Operator : RC/JU
Sample : PB168750BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB168750BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------