



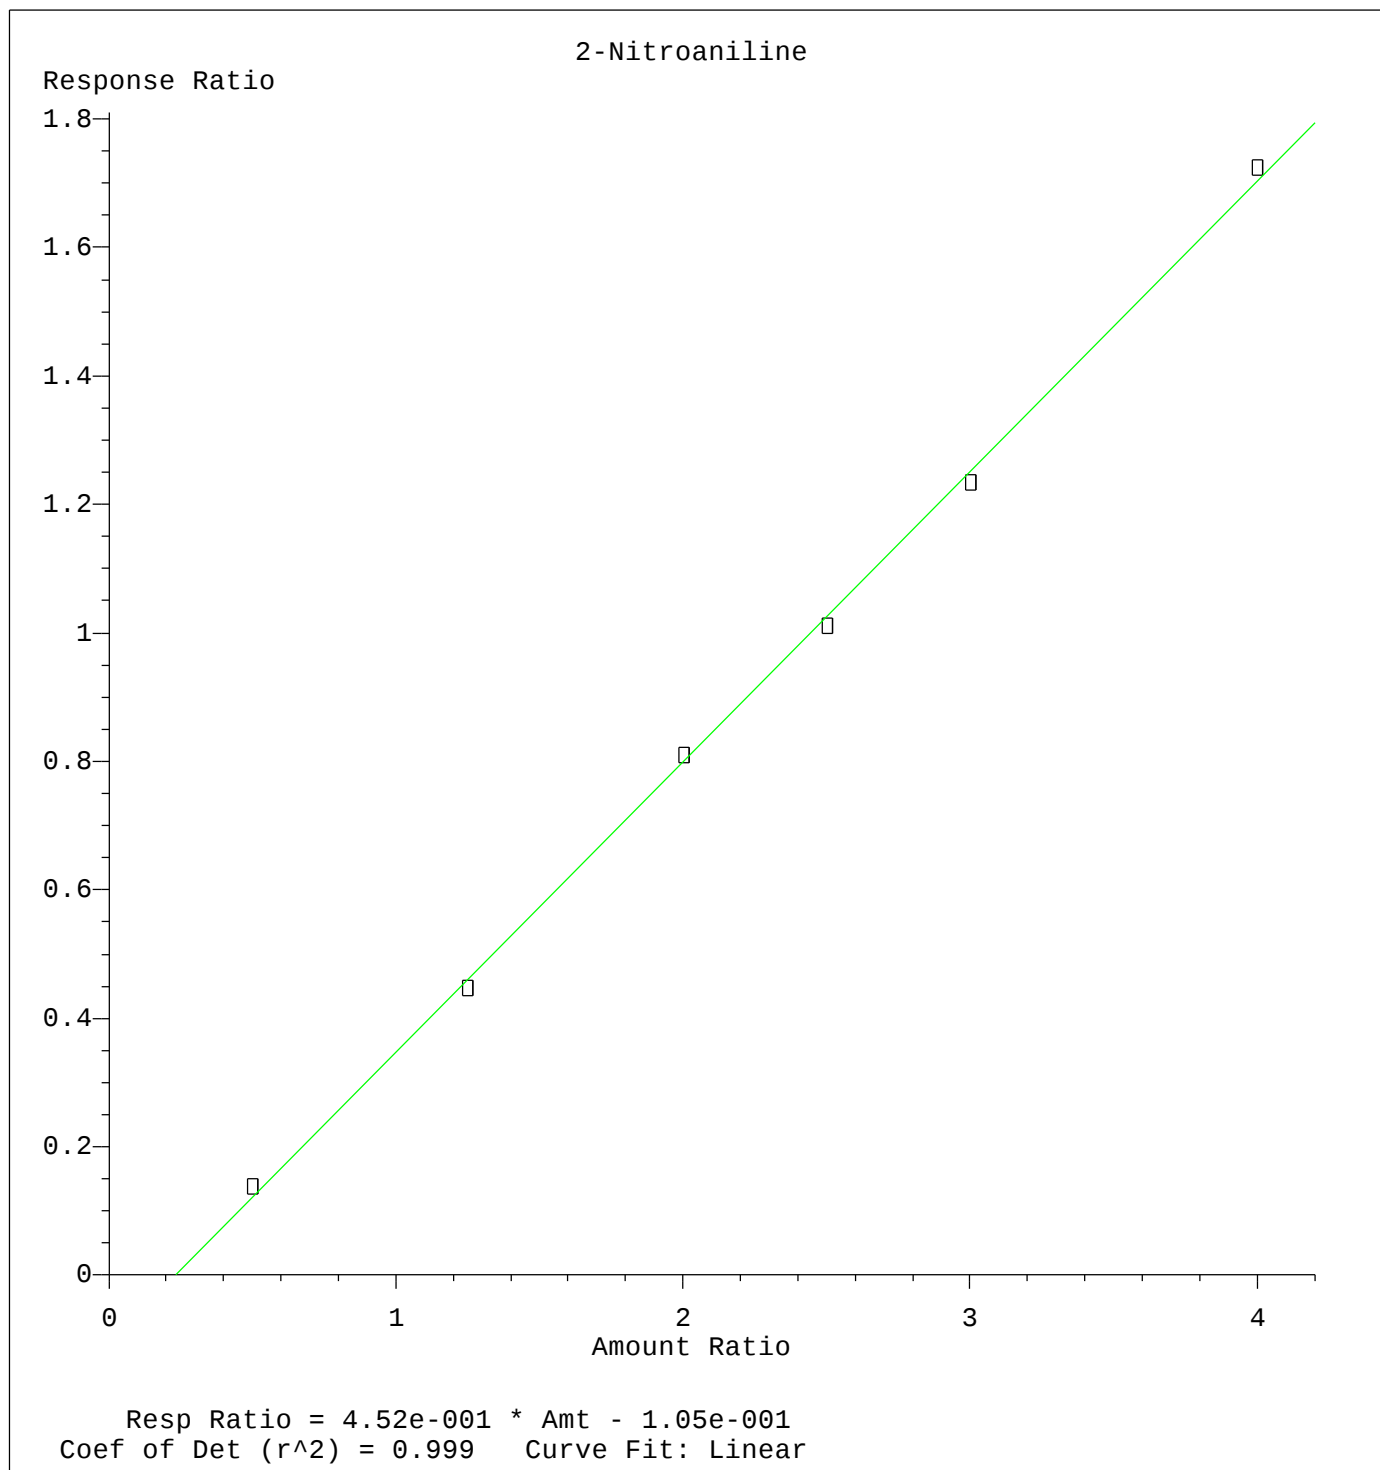

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
Calibration Table Last Updated: Sat Jul 11 05:35:30 2015


2,4-Dinitrophenol

Response Ratio

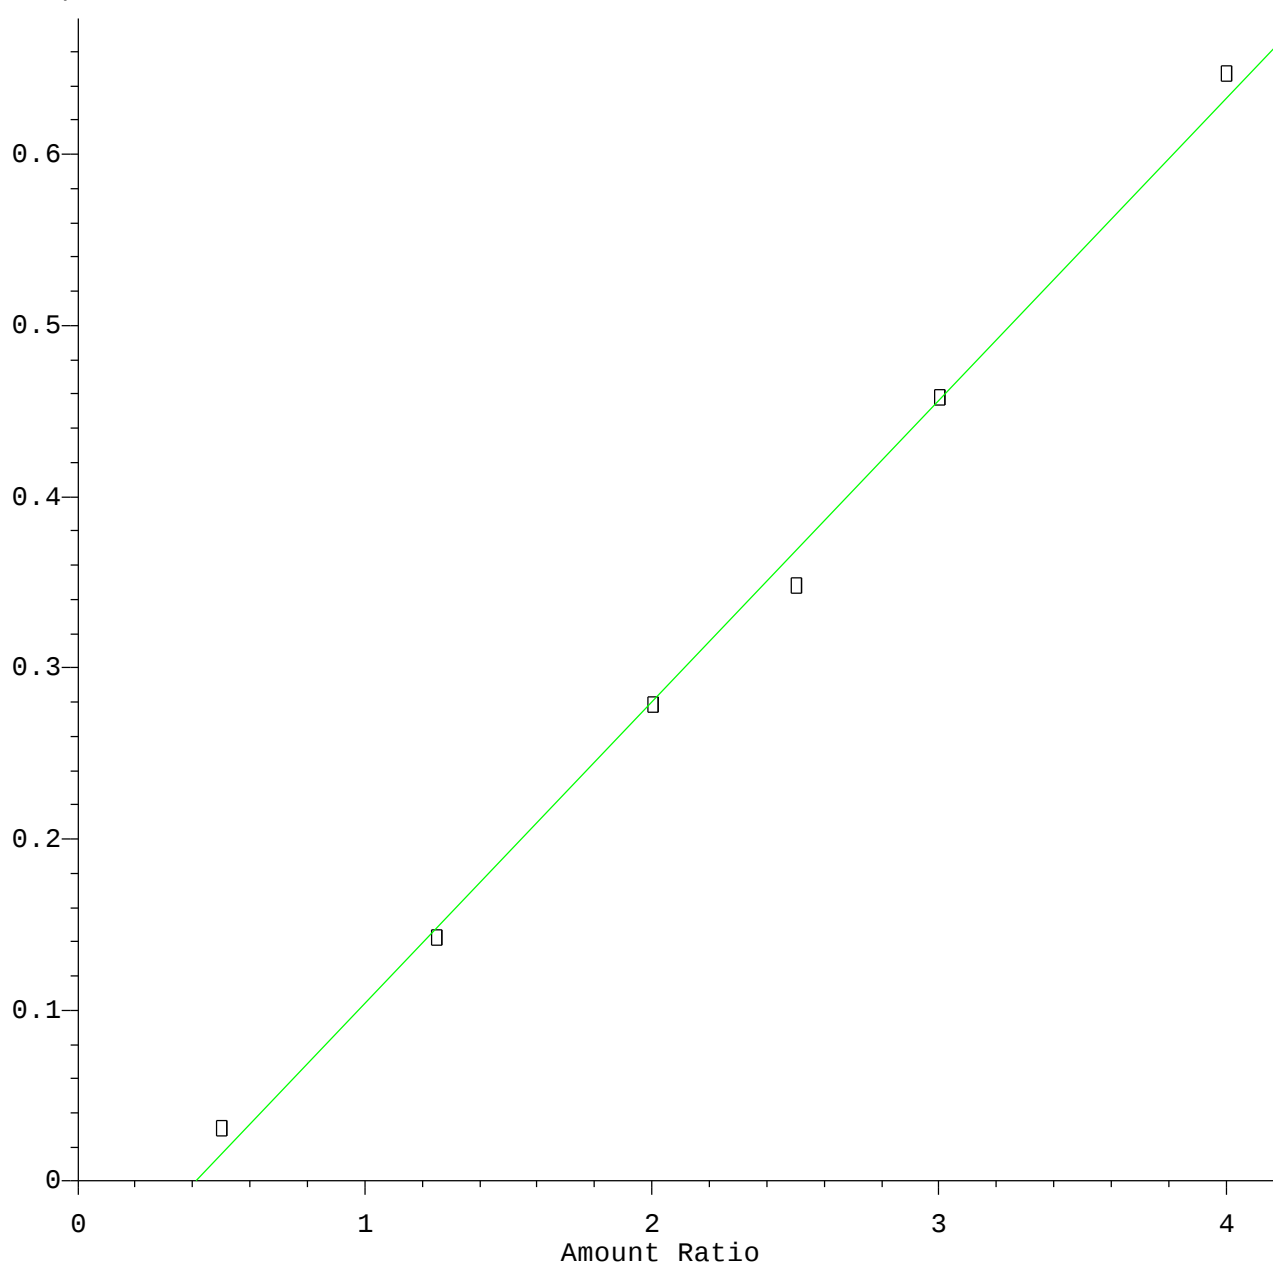

Resp Ratio = $1.76 \times 10^{-1} \times \text{Amt} - 7.20 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
Calibration Table Last Updated: Sat Jul 11 05:35:30 2015

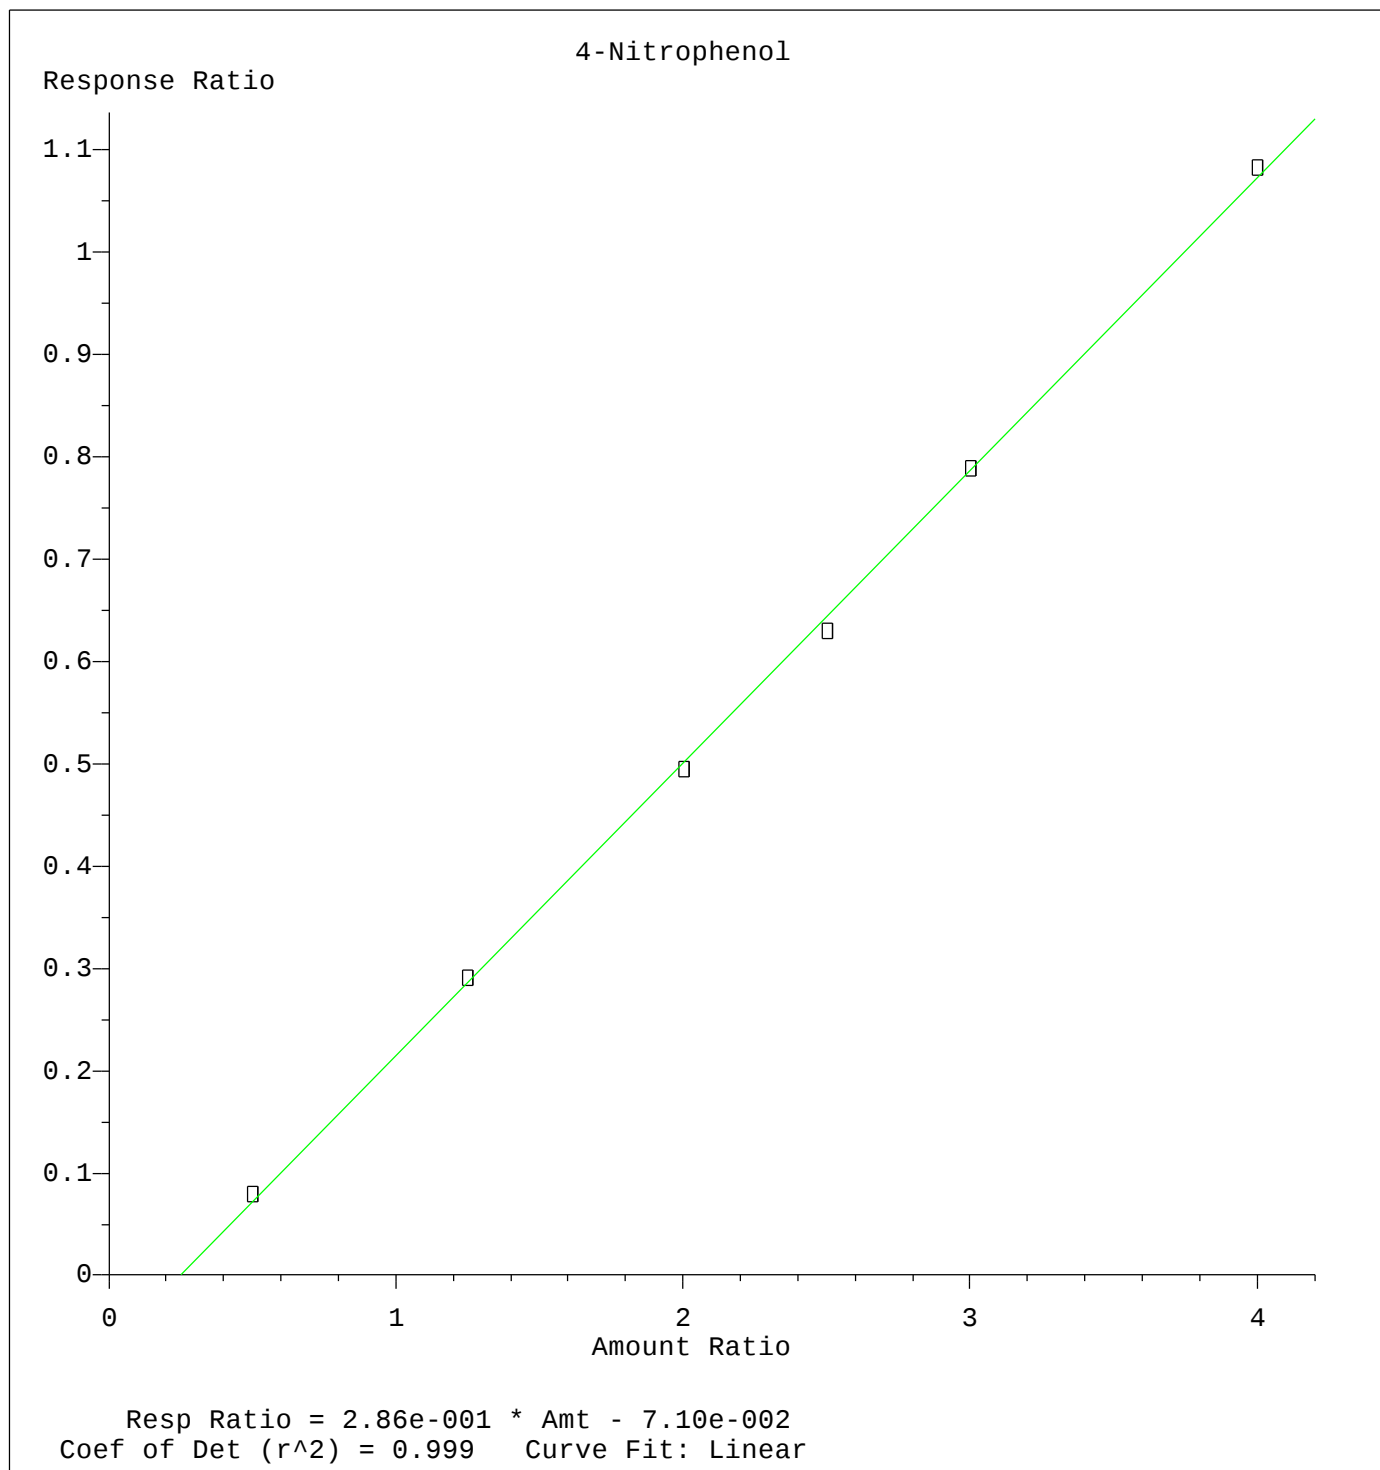

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
Calibration Table Last Updated: Sat Jul 11 05:35:30 2015

4-Nitroaniline


Response Ratio

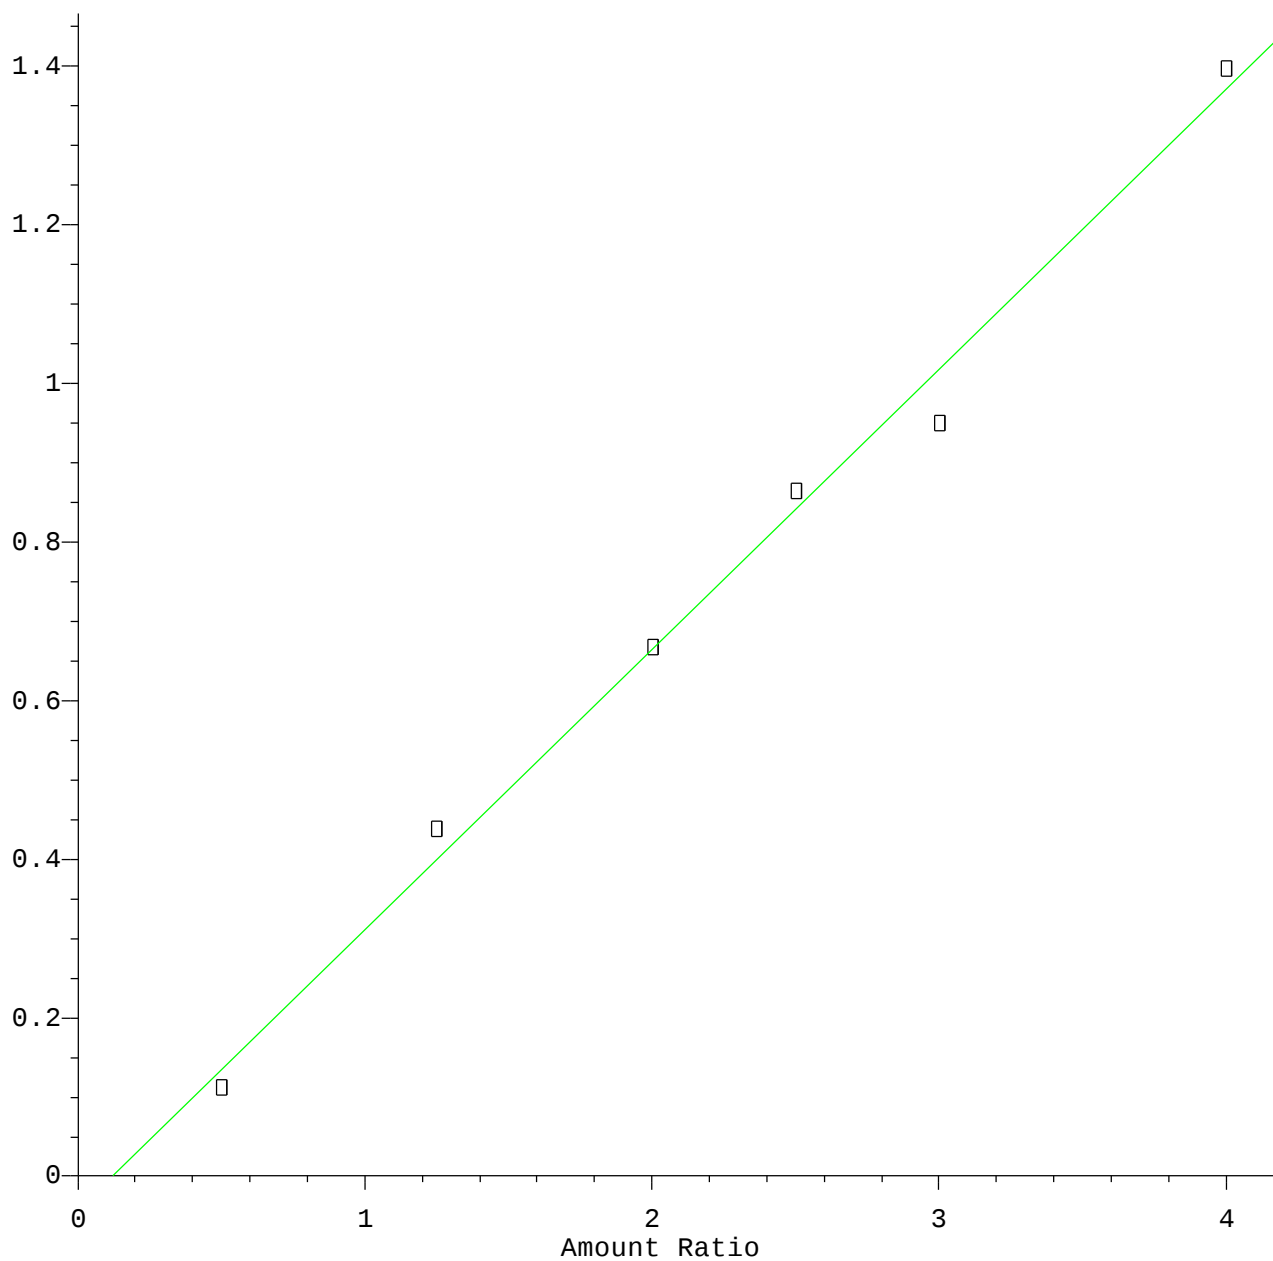

Resp Ratio = $3.53 \times 10^{-1} \times \text{Amt} - 4.25 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
Calibration Table Last Updated: Sat Jul 11 05:35:30 2015

4,6-Dinitro-2-methylphenol

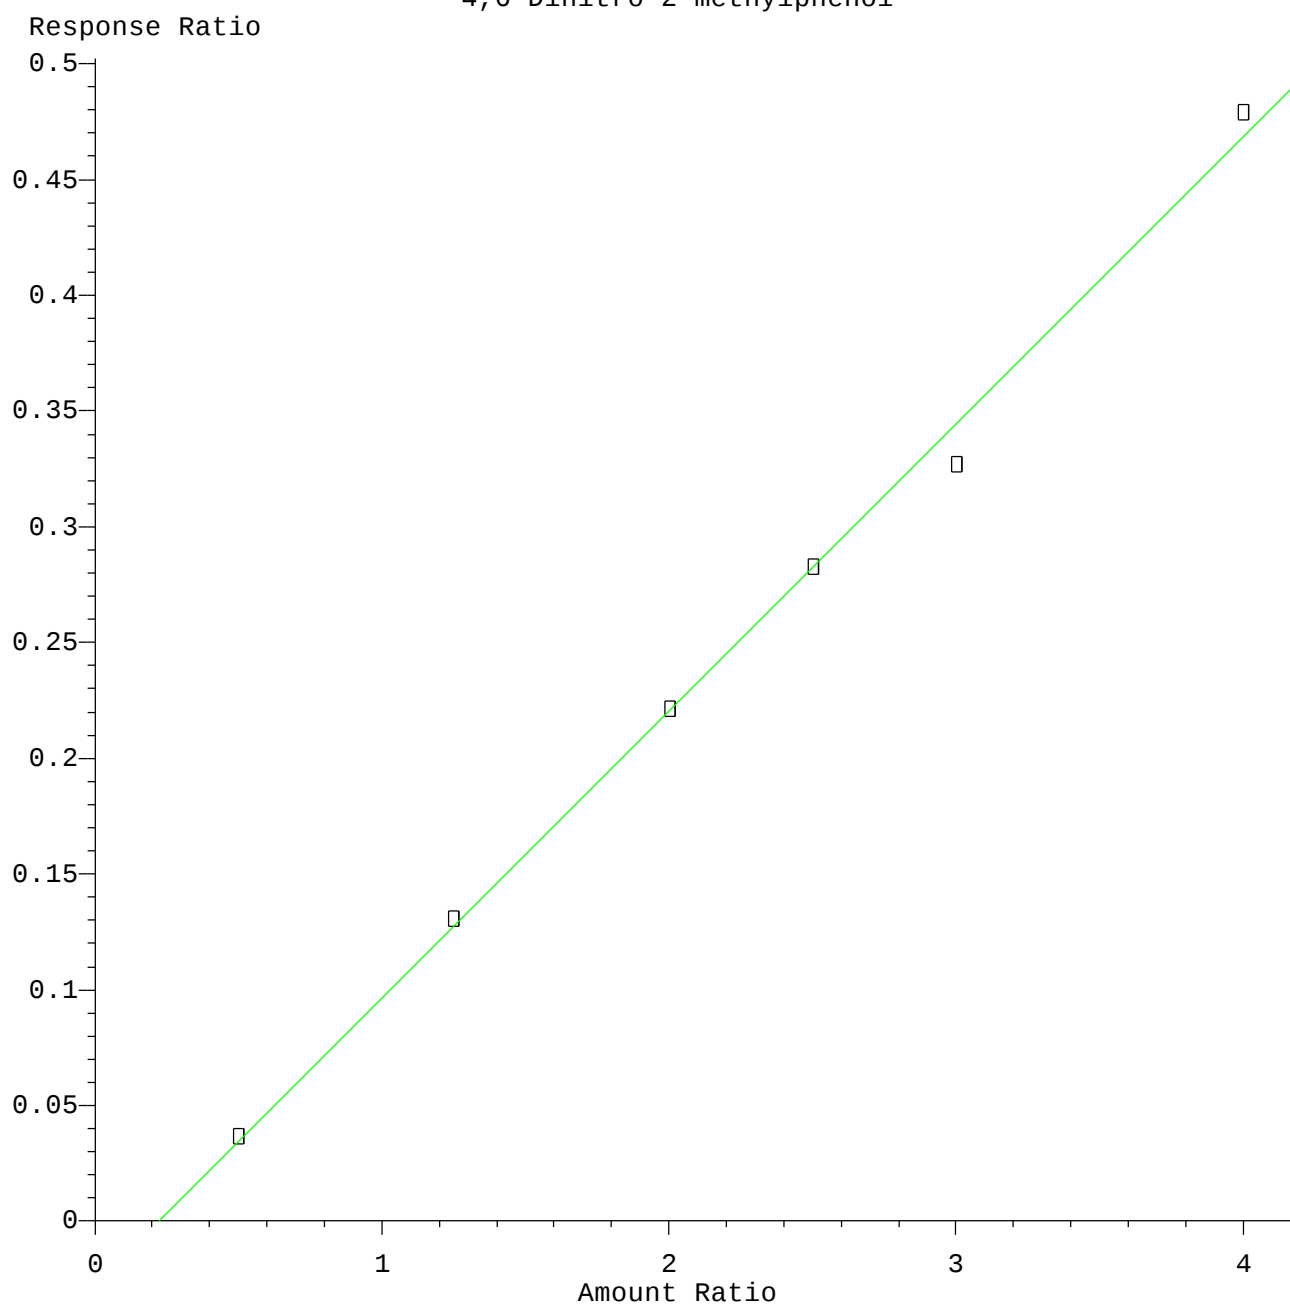

Resp Ratio = $1.24 \times 10^{-1} \times \text{Amt} - 2.74 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
Calibration Table Last Updated: Sat Jul 11 05:35:30 2015