
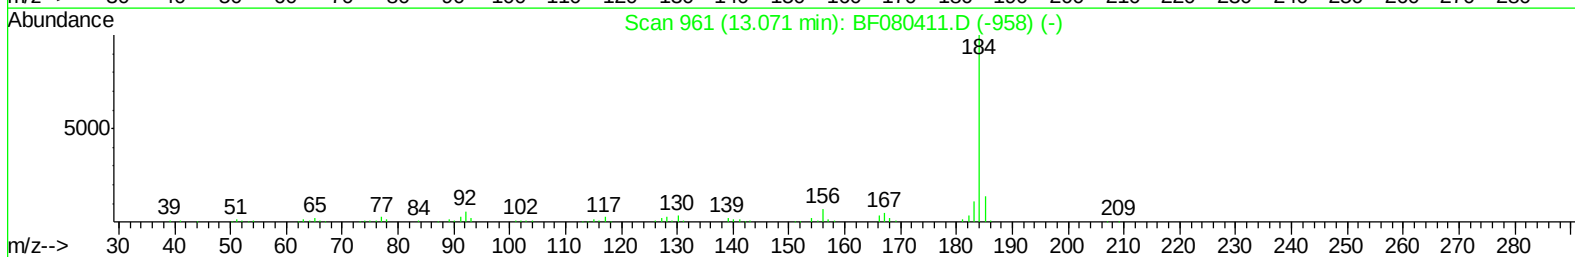
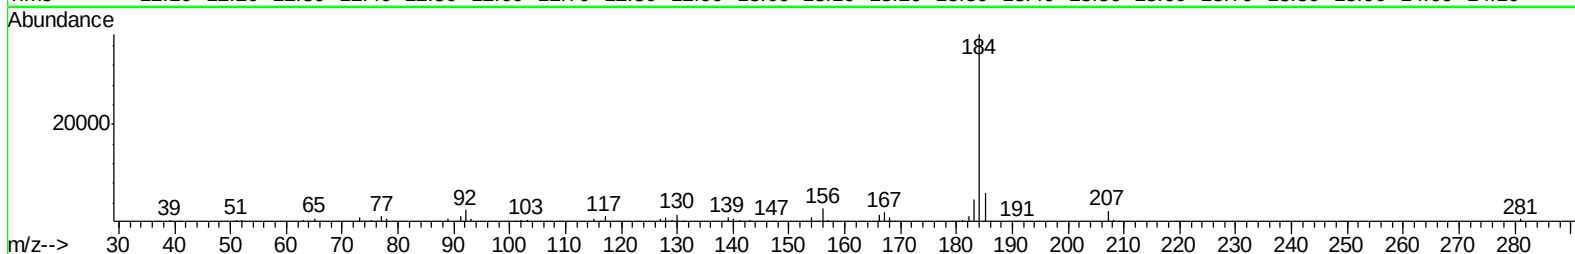


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071015\
 Data File : BF080407.D
 Acq On : 11 Jul 2015 00:44
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 02:21:06 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF071015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 11 05:35:30 2015
 Response via : Initial Calibration

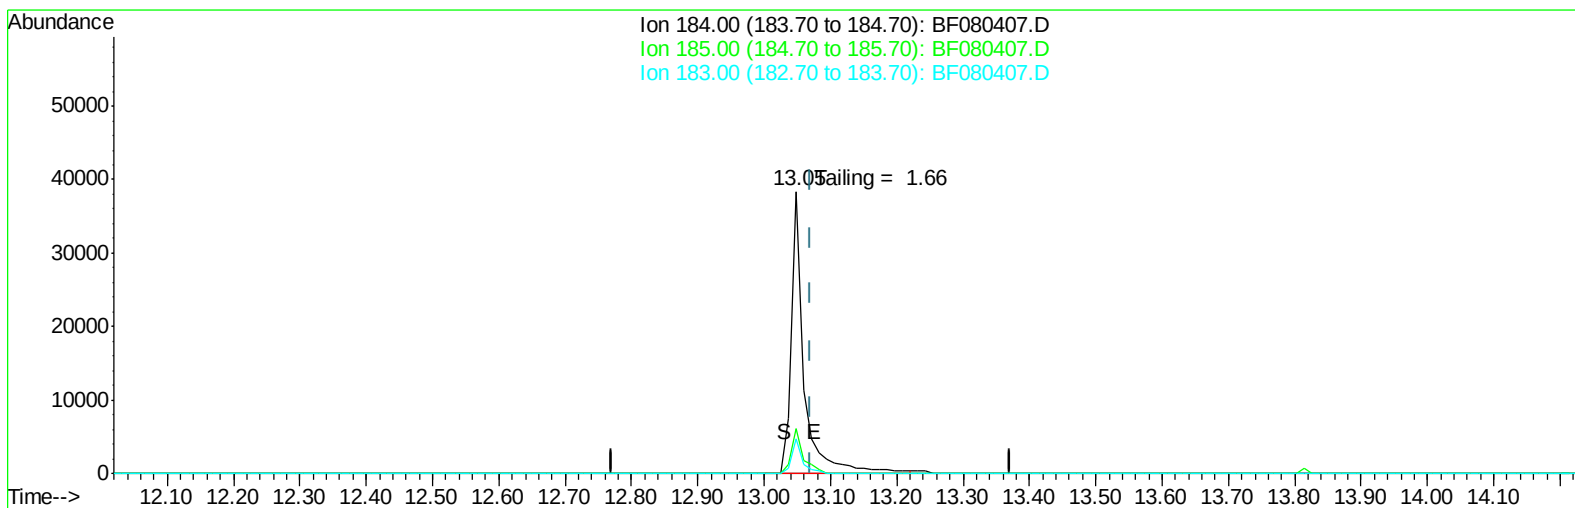

TIC: BF080407.D

(76) Benzidine

13.048min (-0.023) 11597.41ng

response 51209

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	15.81
183.00	11.30	12.50
0.00	0.00	0.00