


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071017\
 Data File : BF096629.D
 Acq On : 11 Jul 2017 4:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 13:02:33 2017

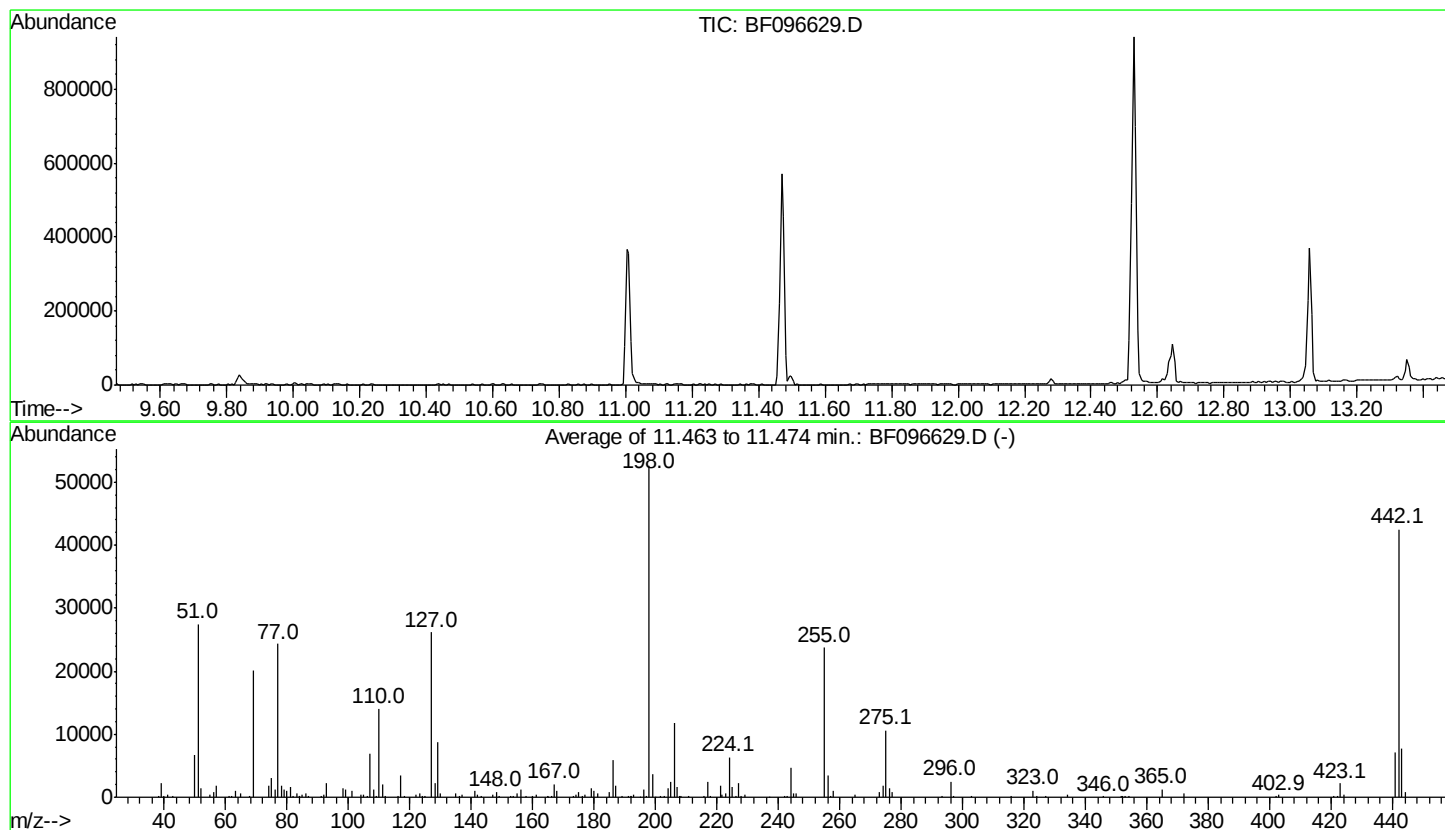

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	27504	PASS
68	69	0.00	2	1.5	300	PASS
69	198	0.00	100	38.2	20075	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	26162	PASS
197	198	0.00	2	0.5	289	PASS
198	198	100	100	100.0	52608	PASS
199	198	5	9	6.8	3603	PASS
275	198	10	60	20.2	10647	PASS
365	198	1	100	2.3	1220	PASS
441	442	0.01	24	16.7	7102	PASS
442	198	50	100	80.7	42461	PASS
443	442	15	24	18.3	7754	PASS