


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071019\
Data File : BF115482.D
Acq On : 11 Jul 2019 3:53
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jul 10 16:47:05 2019

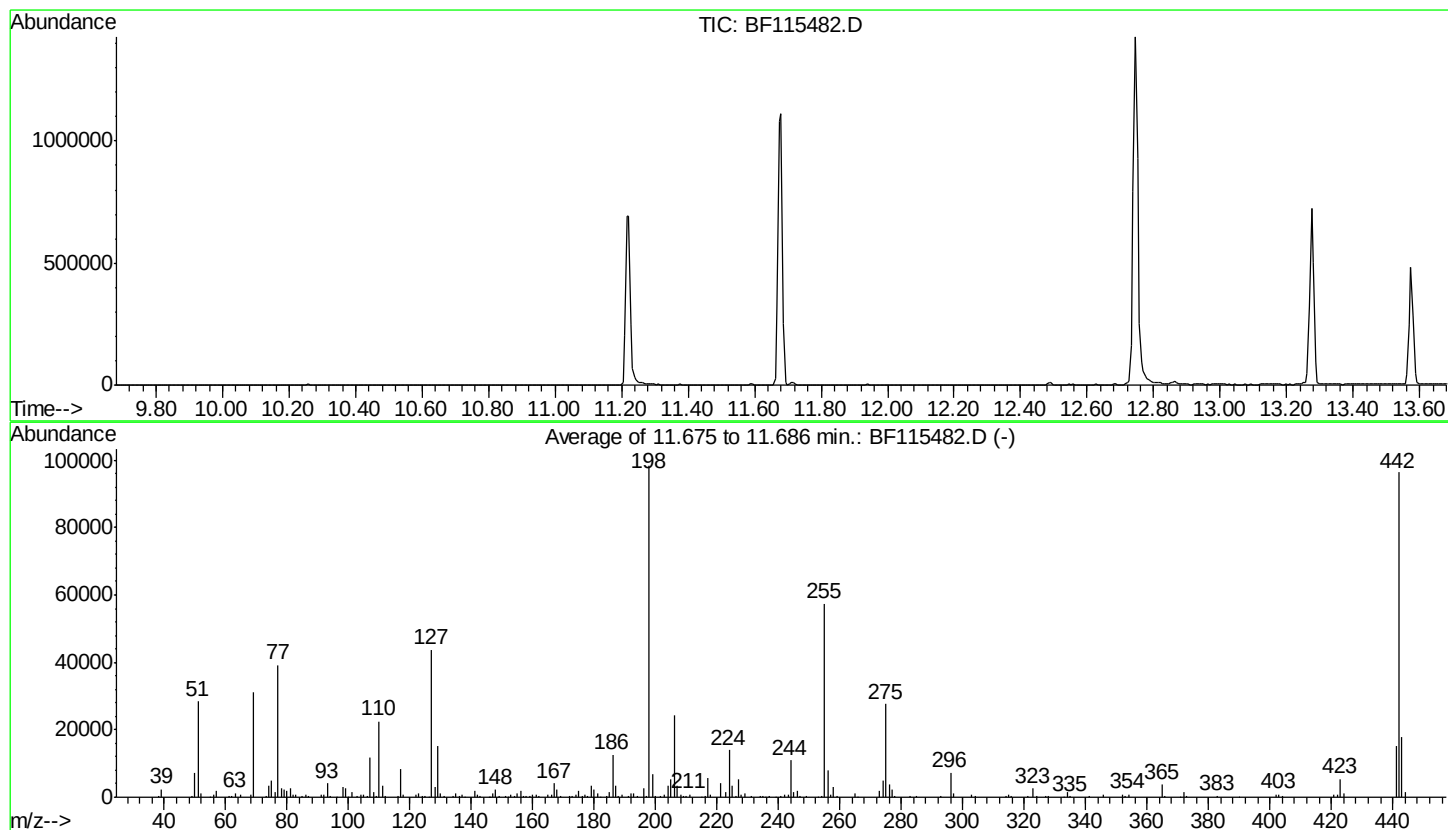

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	28368	PASS
68	69	0.00	2	1.9	588	PASS
69	198	0.00	100	31.8	31313	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.6	43822	PASS
197	198	0.00	2	0.2	240	PASS
198	198	100	100	100.0	98365	PASS
199	198	5	9	6.8	6736	PASS
275	198	10	60	28.2	27714	PASS
365	198	1	100	3.7	3673	PASS
441	198	0.01	100	15.3	15048	PASS
442	198	50	100	97.9	96272	PASS
443	442	15	24	18.6	17924	PASS