
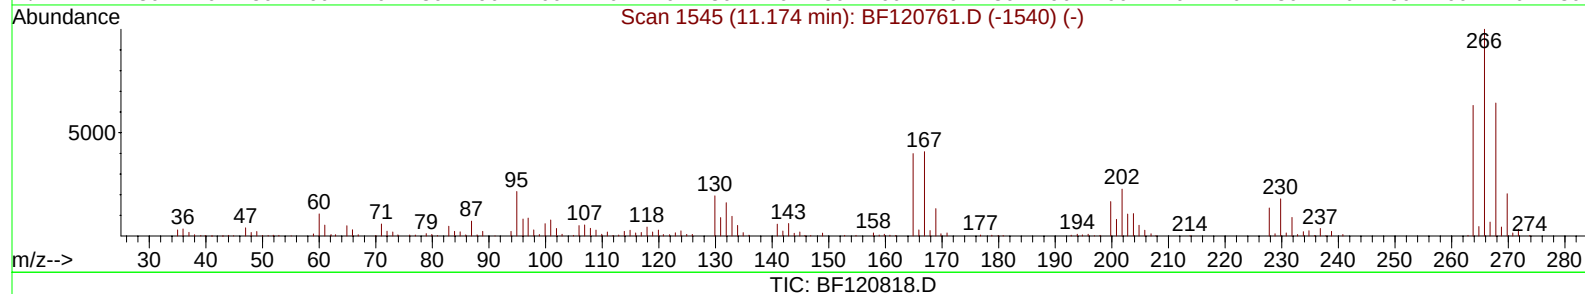
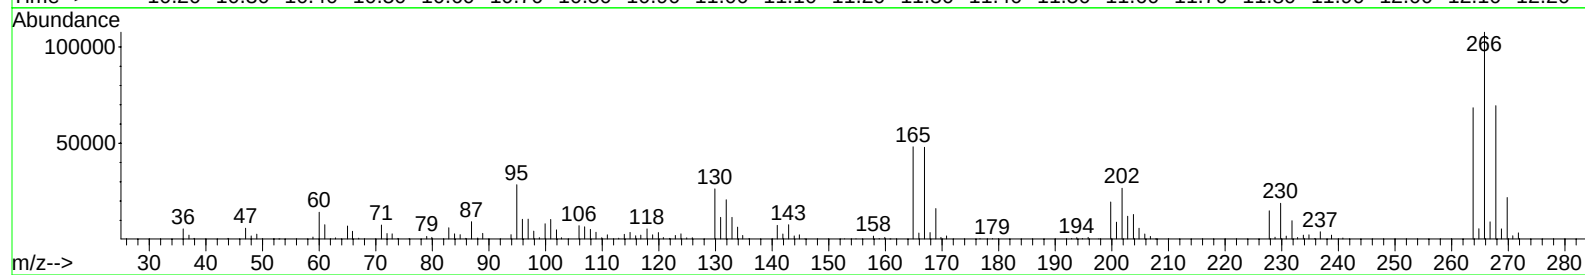


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
Data File : BF120818.D
Acq On : 10 Jul 2020 8:22
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 19:07:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 18:51:52 2020
Response via : Initial Calibration

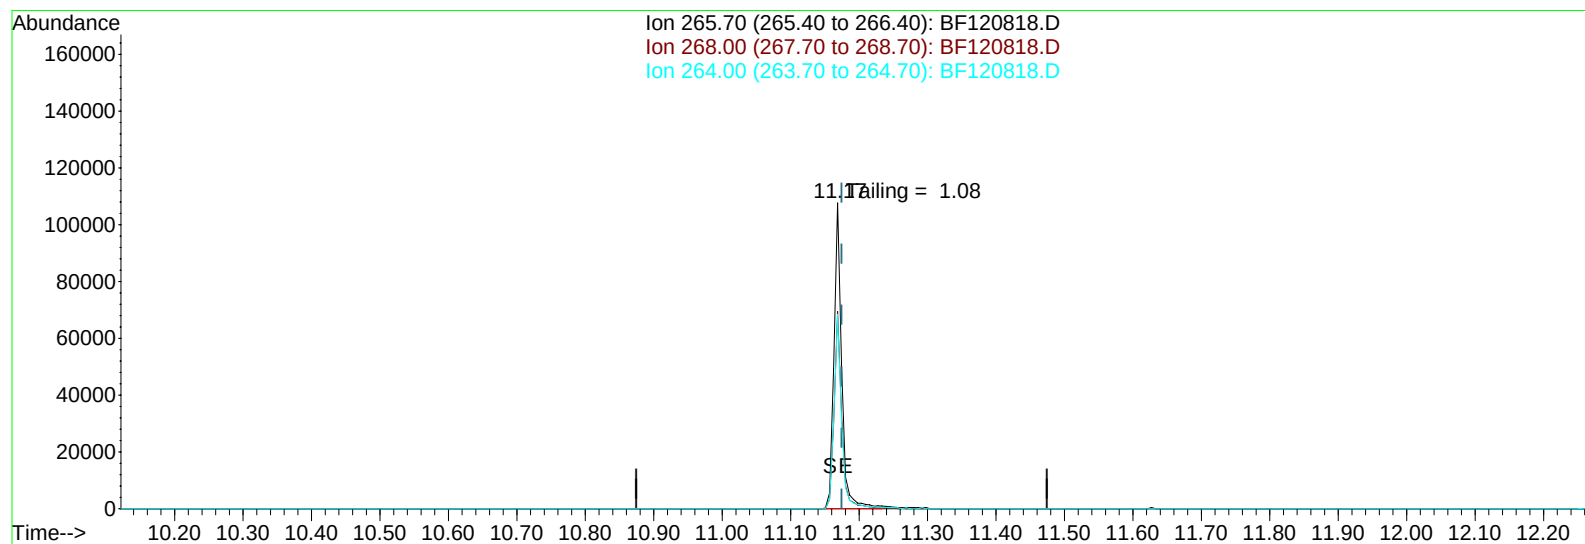

(70) Pentachlorophenol (C)




11.169min (-0.006) 115953.90ng

response 86245

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	64.55
264.00	63.20	63.55
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
 Data File : BF120818.D
 Acq On : 10 Jul 2020 8:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 19:07:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 02 18:51:52 2020
 Response via : Initial Calibration

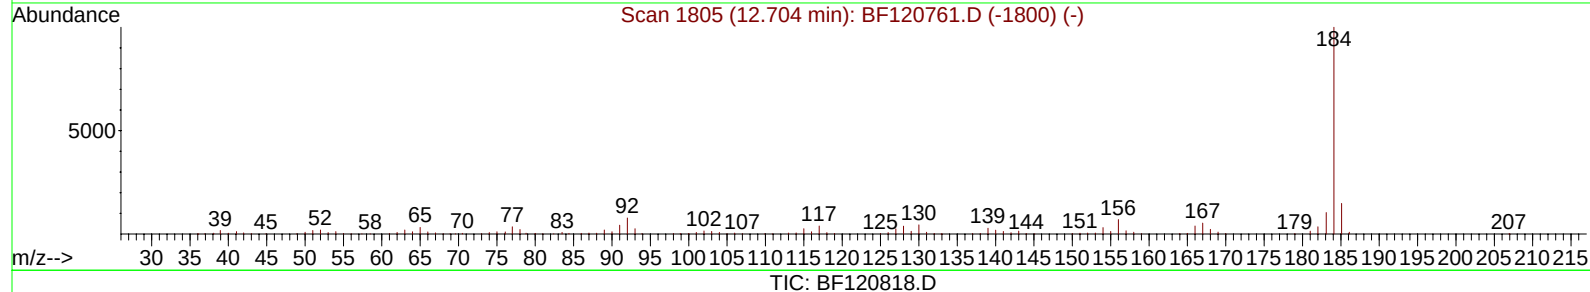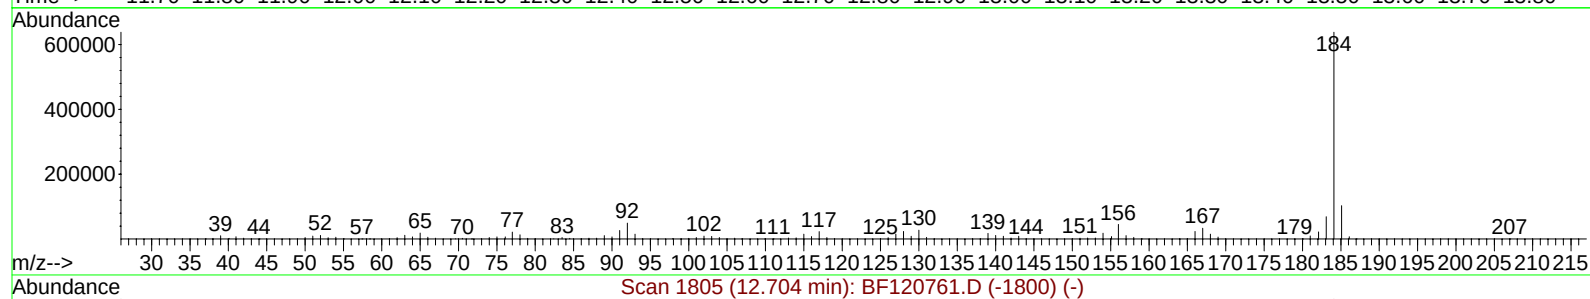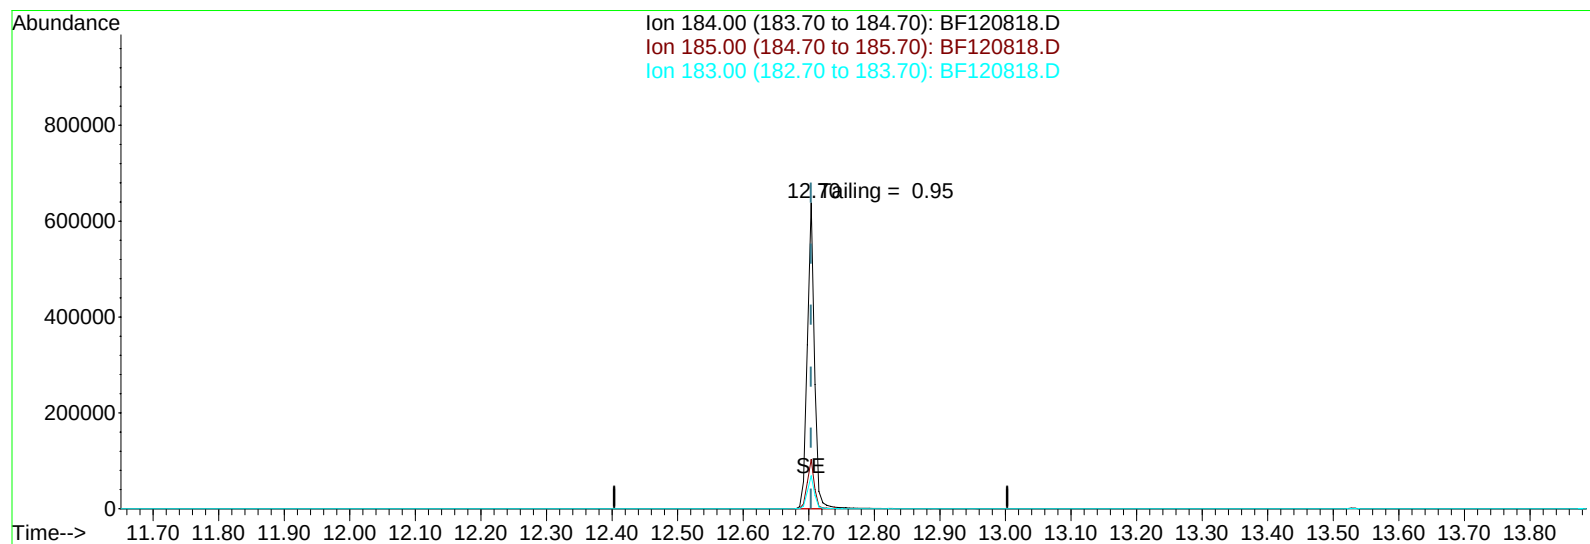

(77) Benzidine

12.704min (+0.001) 12342.06ng

response 489105

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	16.12
183.00	10.40	10.78
0.00	0.00	0.00