
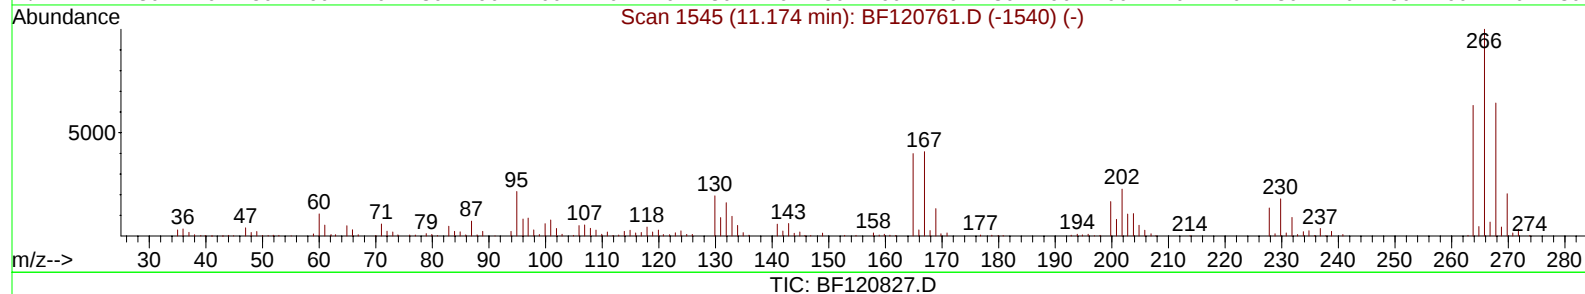
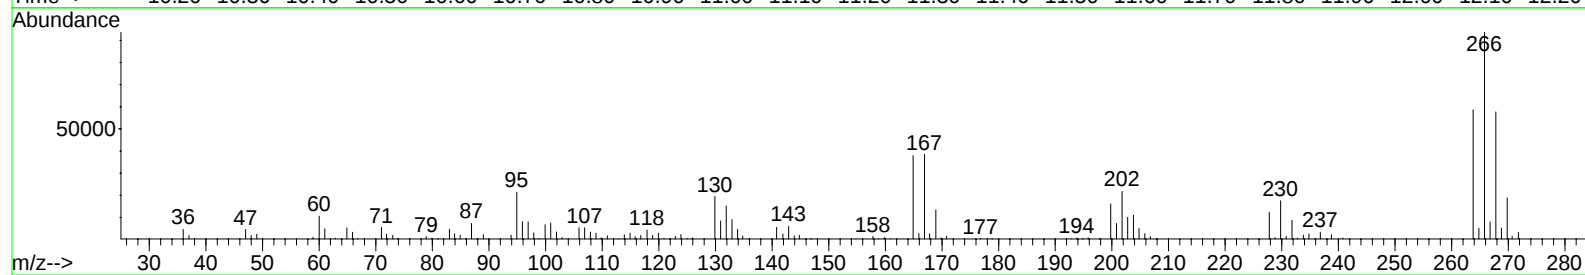


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
Data File : BF120827.D
Acq On : 10 Jul 2020 13:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 19:05:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 18:51:52 2020
Response via : Initial Calibration

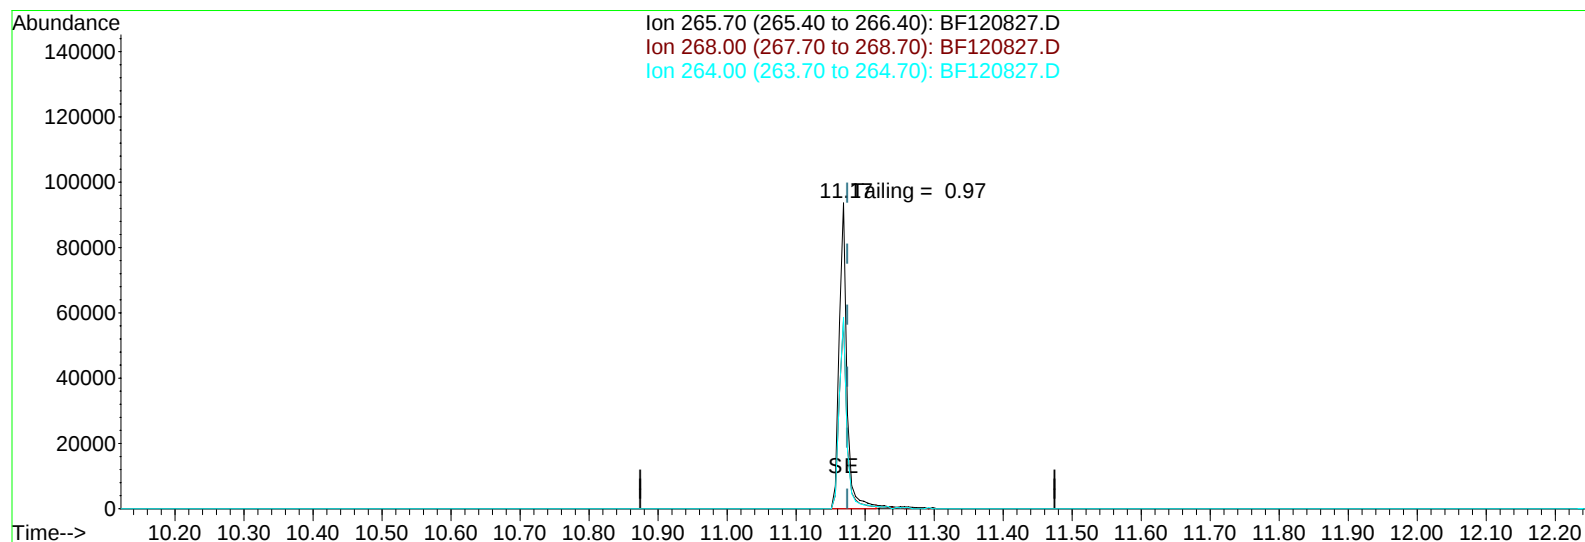

(70) Pentachlorophenol (C)




11.169min (-0.006) 36318.87ng

response 74037

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.55
264.00	63.20	62.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
Data File : BF120827.D
Acq On : 10 Jul 2020 13:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 19:05:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 18:51:52 2020
Response via : Initial Calibration

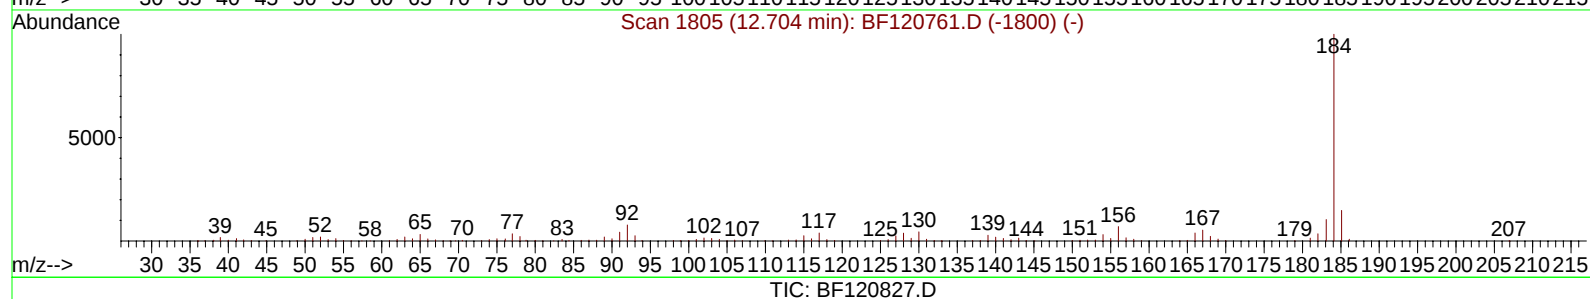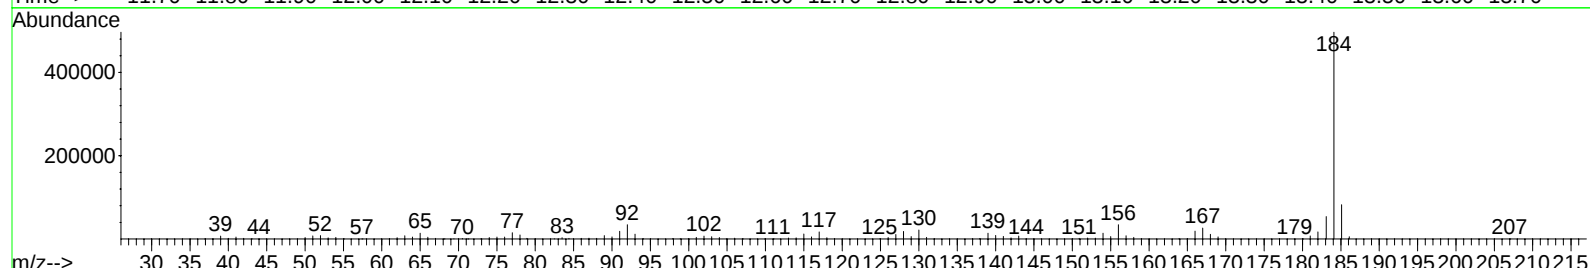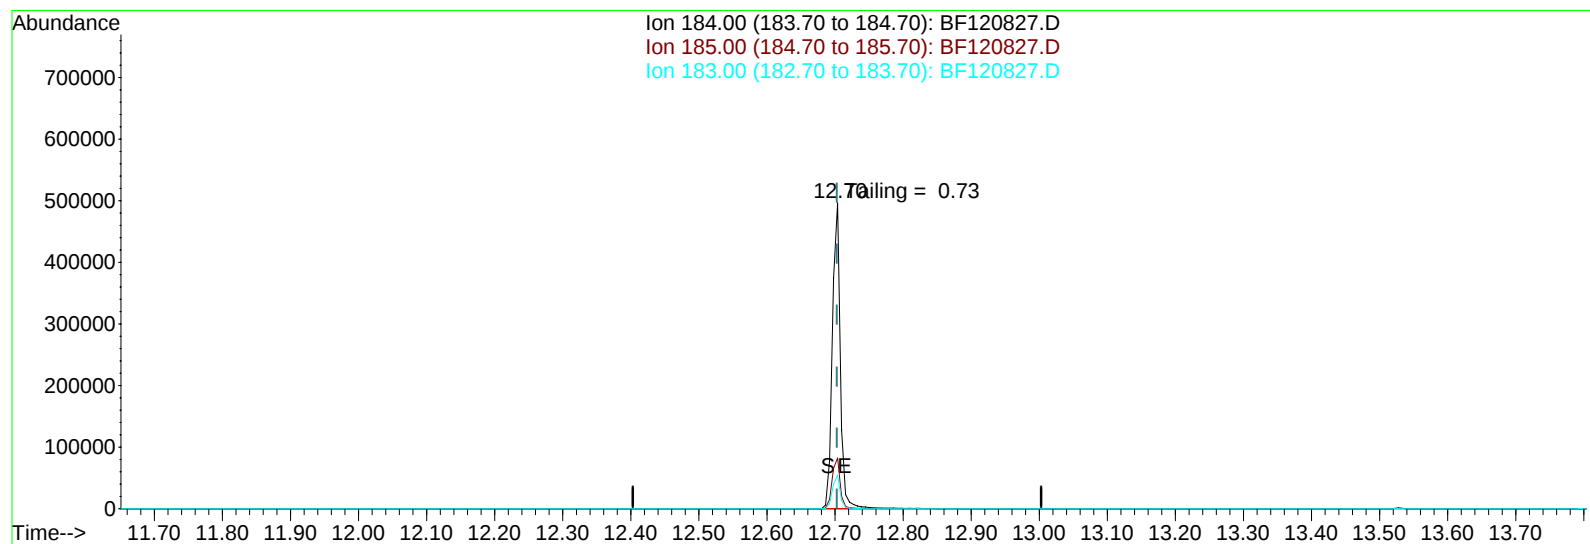

(77) Benzidine

12.704min (+0.001) 0.00ng

response 404145

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	16.59
183.00	10.40	10.93
0.00	0.00	0.00