

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
 Data File : BF120833.D
 Acq On : 10 Jul 2020 16:00
 Operator : JU/CG
 Sample : PB130117BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130117BL

Quant Time: Jul 11 06:22:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 02 18:51:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	142938	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	522835	20.00	ng	0.00
39) Acenaphthene-d10	9.88	164	249999	20.00	ng	0.00
64) Phenanthrene-d10	11.36	188	446121	20.00	ng	-0.01
76) Chrysene-d12	14.00	240	286596	20.00	ng	0.00
86) Perylene-d12	15.46	264	233638	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	1252059	135.22	ng	0.00
7) Phenol-d6	6.47	99	1506140	127.37	ng	0.00
23) Nitrobenzene-d5	7.41	82	932077	103.29	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	369224	147.01	ng	0.00
45) 2-Fluorobiphenyl	9.21	172	1533426	92.80	ng	0.00
79) Terphenyl-d14	12.96	244	1658518	113.30	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
Data File : BF120833.D
Acq On : 10 Jul 2020 16:00
Operator : JU/CG
Sample : PB130117BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130117BL

Quant Time: Jul 11 06:22:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 02 18:51:52 2020
Response via : Initial Calibration

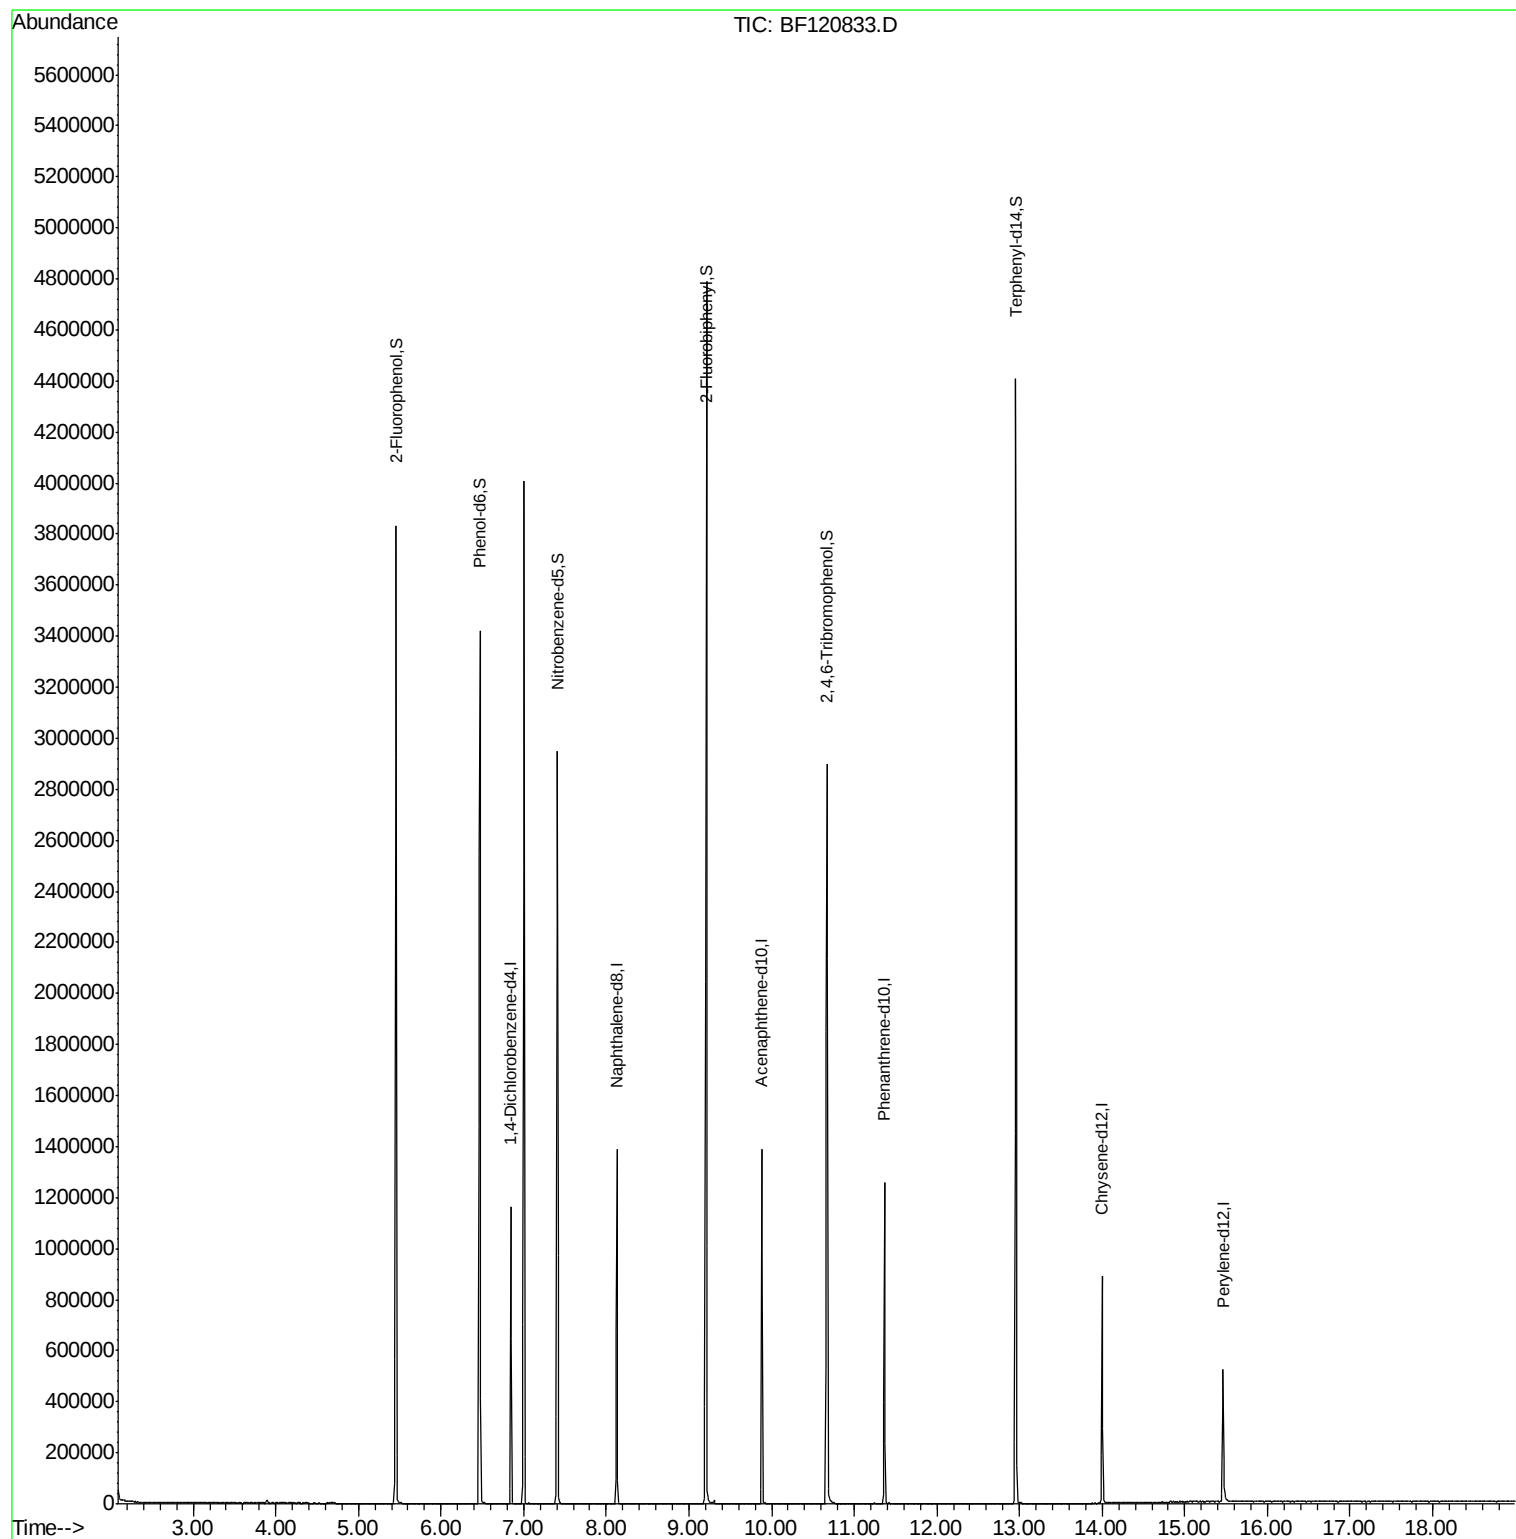




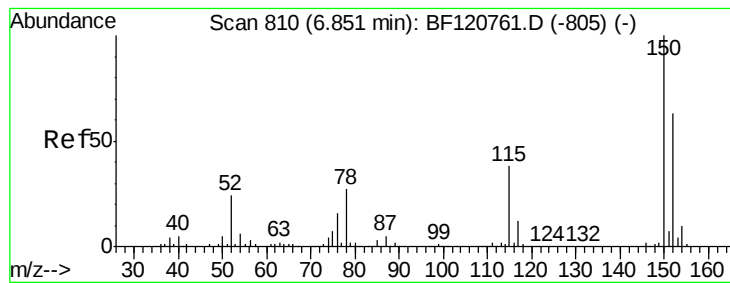


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.85 min Scan# 809
Delta R.T. -0.01 min
Lab File: BF120833.D
Acq: 10 Jul 2020 16:00

Instrument :
BNA_F
ClientSampleId :
PB130117BL




Tot Ion:152 Resp: 142938
Ion Ratio Lower Upper
152 100
150 155.1 126.1 189.1
115 62.2 48.5 72.7

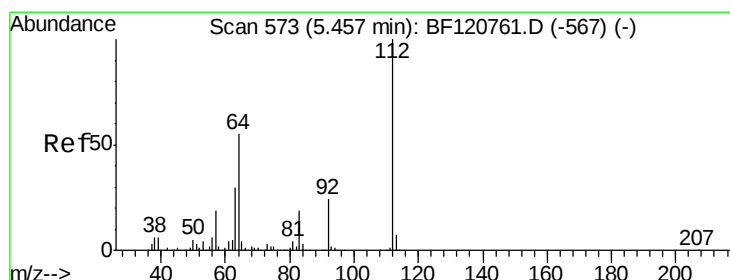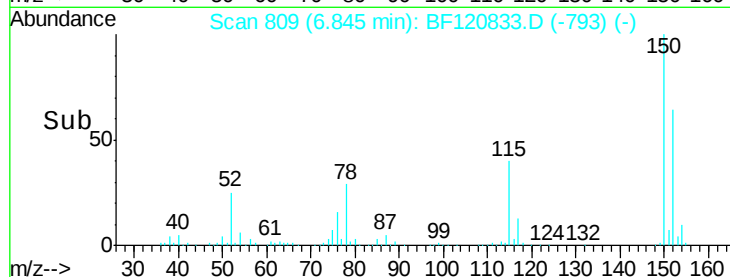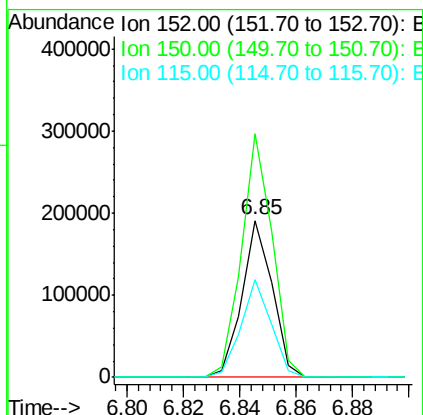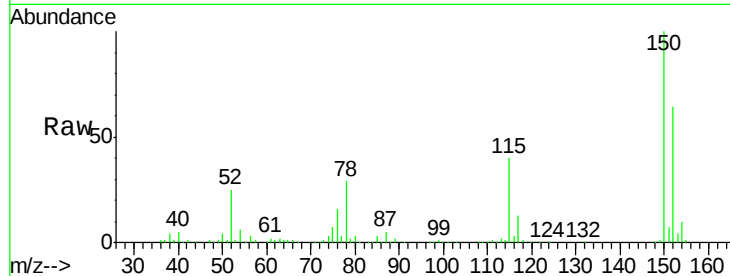


#5

2-Fluorophenol
Concen: 135.215 ng
RT: 5.46 min Scan# 573
Delta R.T. 0.00 min
Lab File: BF120833.D
Acq: 10 Jul 2020 16:00

Tgt Ion:112 Resp: 1252059
Ion Ratio Lower Upper
112 100
64 55.3 43.8 65.6
63 29.6 23.6 35.4

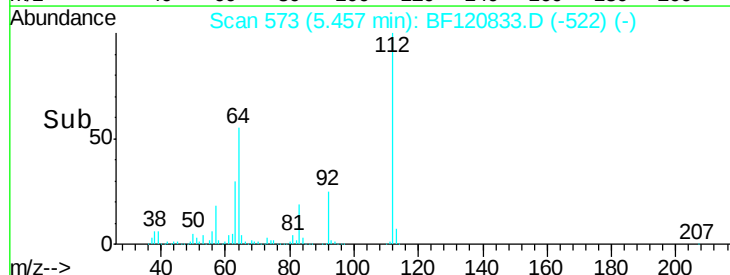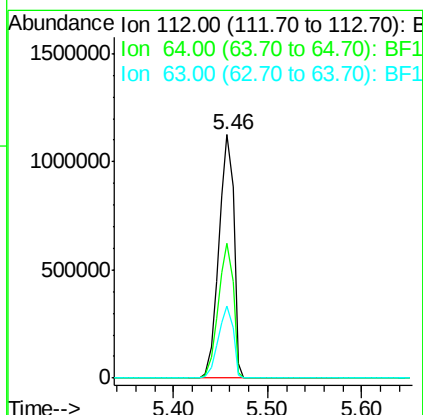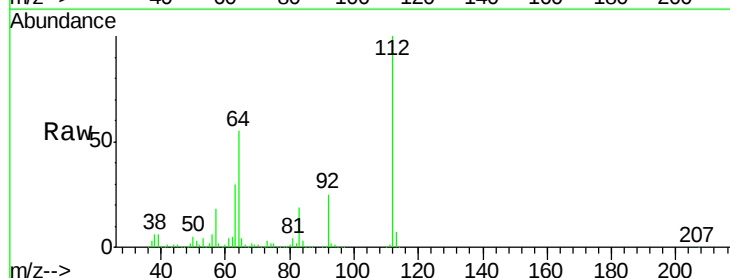

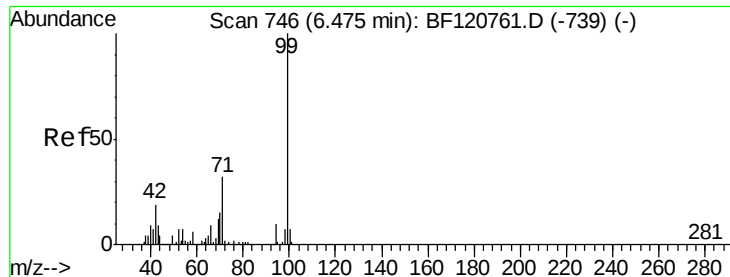

#7

Phenol-d6

Concen: 127.368 ng

RT: 6.47 min Scan# 746

Delta R.T. 0.00 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00

Instrument :

BNA_F

ClientSampleId :

PB130117BL


Tot Ion: 99 Resp: 1506140

Ion Ratio Lower Upper

99 100

42 17.6 15.4 23.0




71 31.7 25.9 38.9

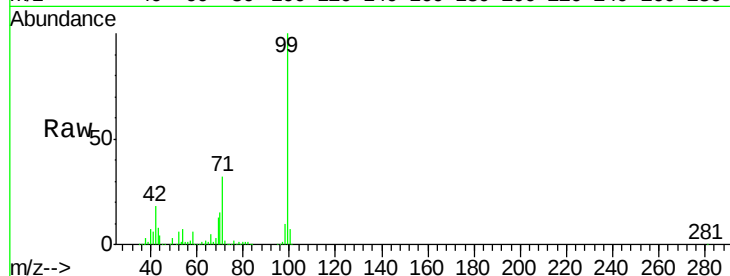

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

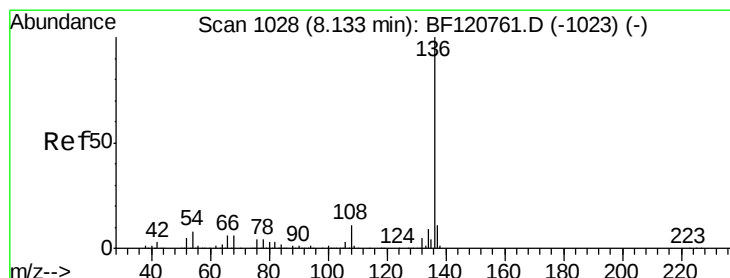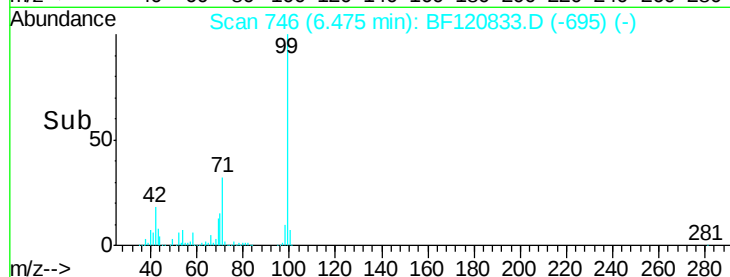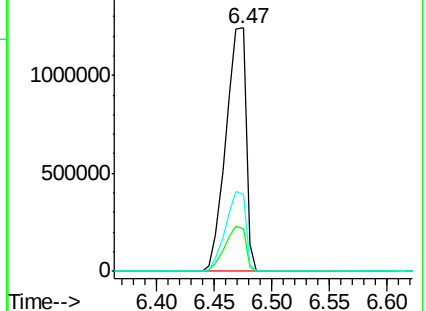

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.13 min Scan# 1027

Delta R.T. -0.01 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00

Tgt Ion: 136 Resp: 522835


Ion Ratio Lower Upper

136 100

137 11.5 9.0 13.6

54 8.0 6.2 9.4

68 5.8 4.7 7.1


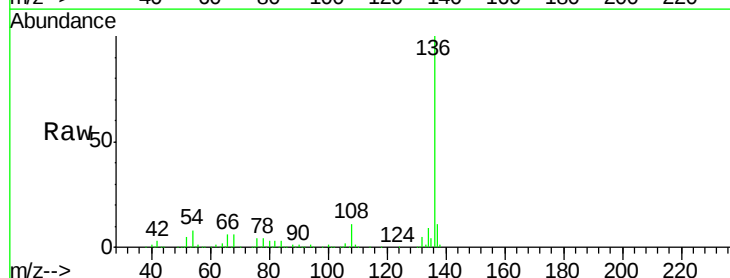


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



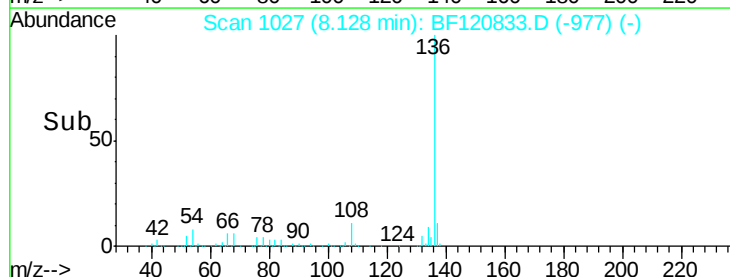
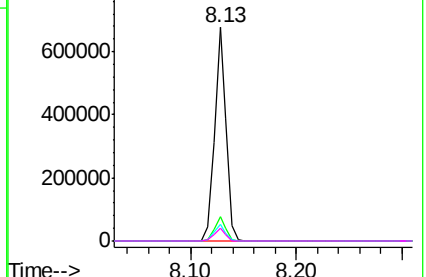




#23
 Nitrobenzene-d5
 Concen: 103.288 ng
 RT: 7.41 min Scan# 905
 Delta R.T. -0.01 min
 Lab File: BF120833.D
 Acq: 10 Jul 2020 16:00




Instrument :
 BNA_F
 ClientSampleId :
 PB130117BL


Tot Ion	82	Resp	932077
Ion Ratio	100	Lower	Upper
128	46.2	35.7	53.5
54	49.5	40.9	61.3

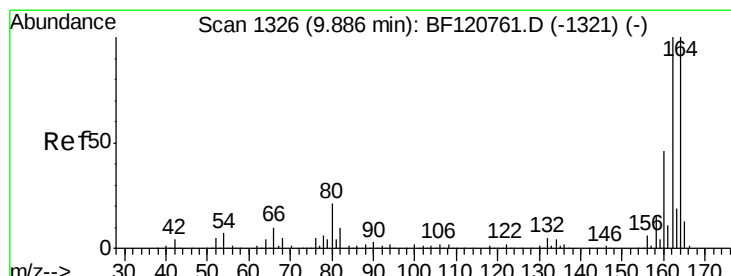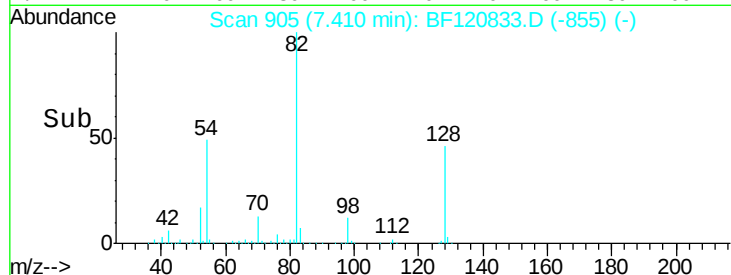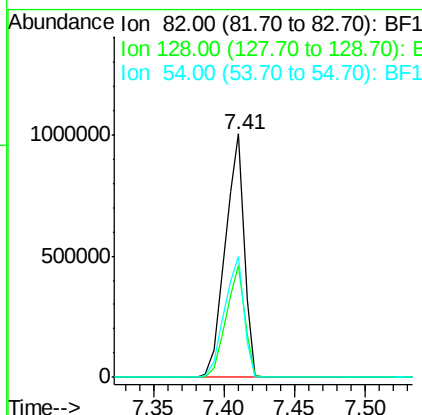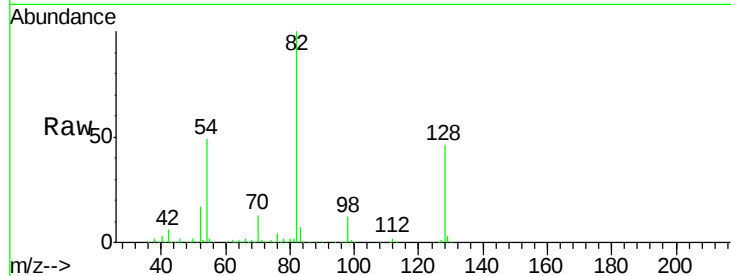

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.88 min Scan# 1325
 Delta R.T. -0.01 min
 Lab File: BF120833.D
 Acq: 10 Jul 2020 16:00

Tgt Ion	164	Resp	249999
Ion Ratio	100	Lower	Upper
162	100.0	80.2	120.2
160	45.6	36.9	55.3

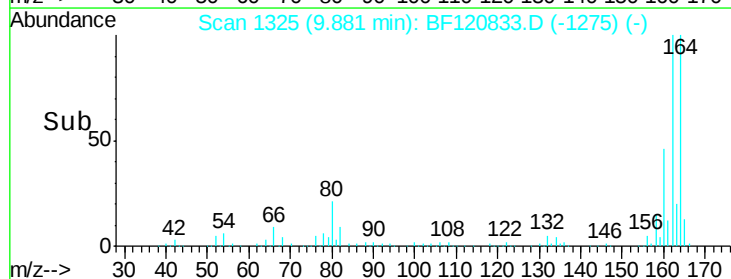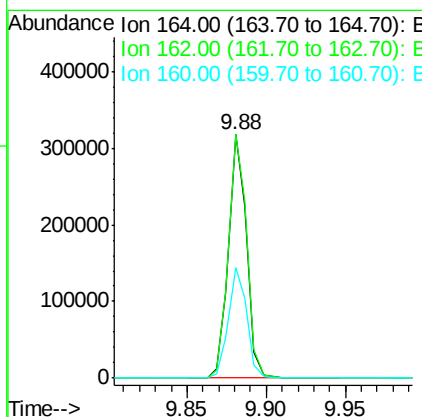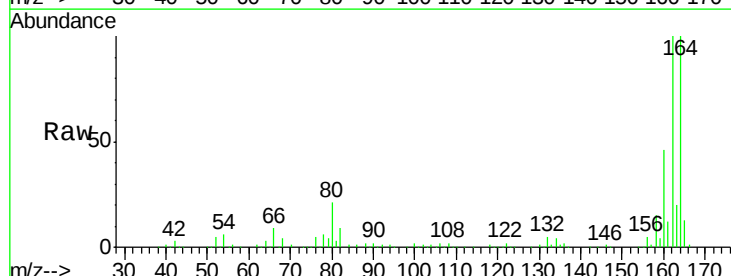

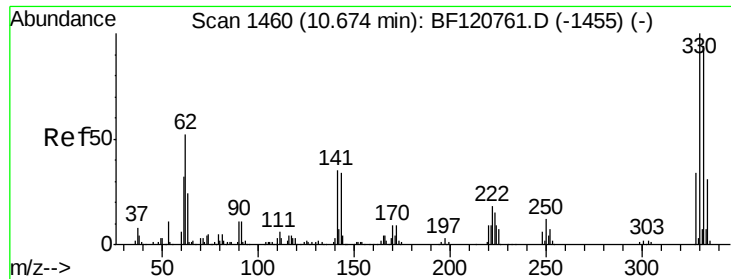

#42

2,4,6-Tribromophenol

Concen: 147.007 ng

RT: 10.67 min Scan# 1459

Delta R.T. -0.01 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00

Instrument :

BNA_F

ClientSampleId :

PB130117BL


Tot Ion:330 Resp: 369224

Ion Ratio Lower Upper

330 100

332 94.6 75.8 113.6




141 33.4 29.7 44.5

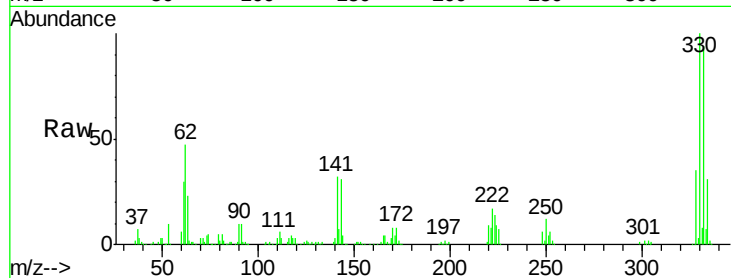

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

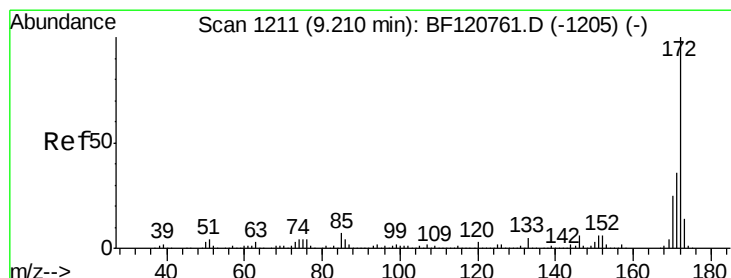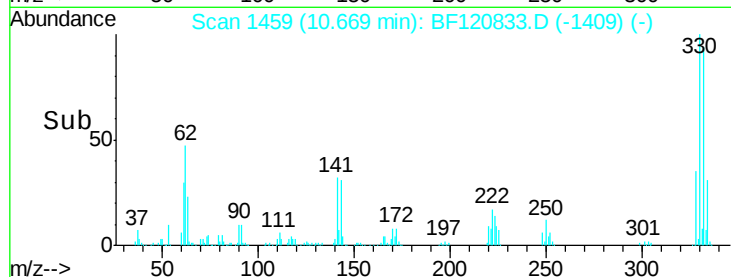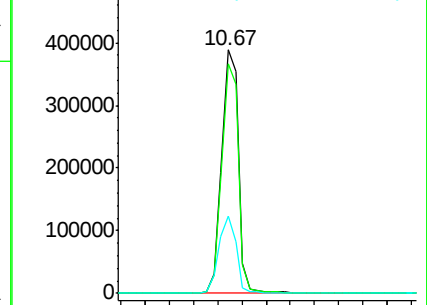

#45

2-Fluorobiphenyl

Concen: 92.800 ng

RT: 9.21 min Scan# 1211

Delta R.T. 0.00 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00


Tgt Ion:172 Resp: 1533426

Ion Ratio Lower Upper

172 100

171 36.3 29.1 43.7



170 24.8 19.8 29.6

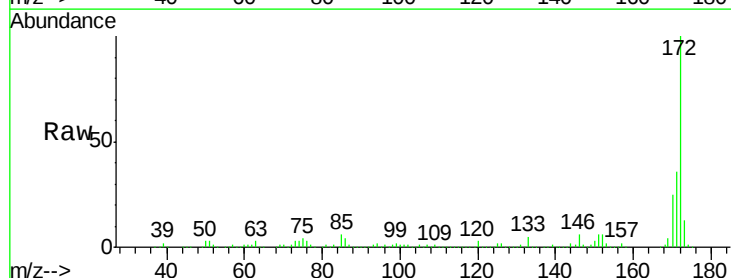


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

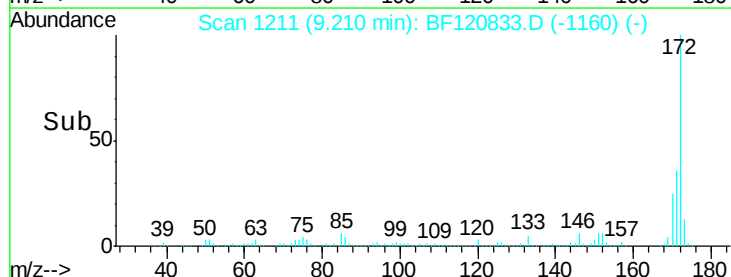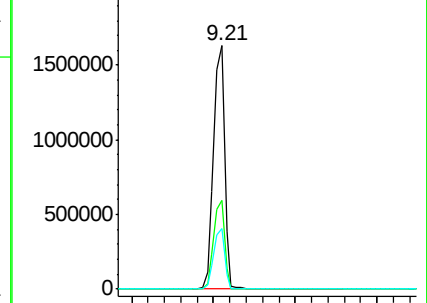

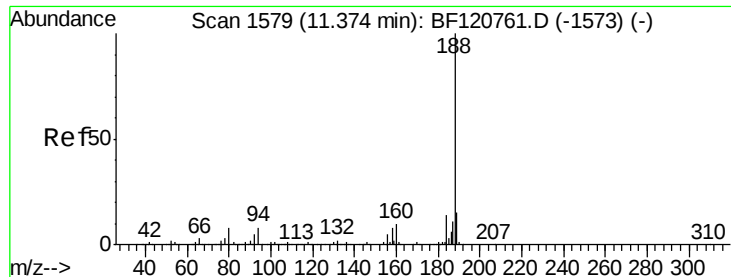

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.36 min Scan# 1577

Delta R.T. -0.01 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00

Instrument :

BNA_F

ClientSampleId :

PB130117BL


Tot Ion:188 Resp: 446121

Ion Ratio Lower Upper

188 100

94 9.7 6.6 9.8




80 10.5 6.6 10.0#

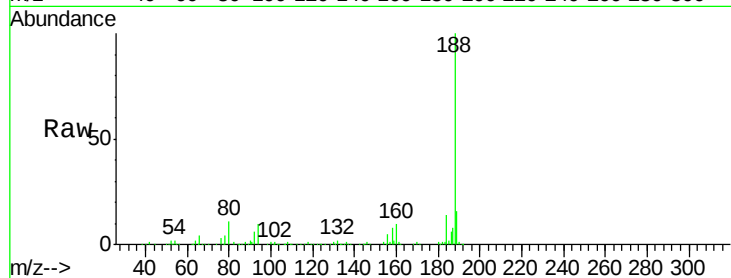

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

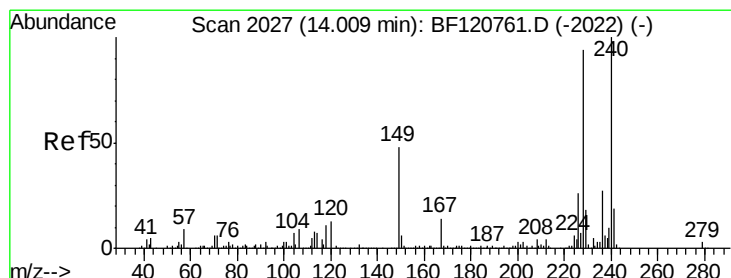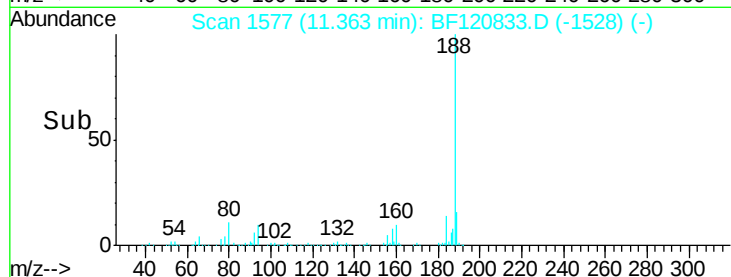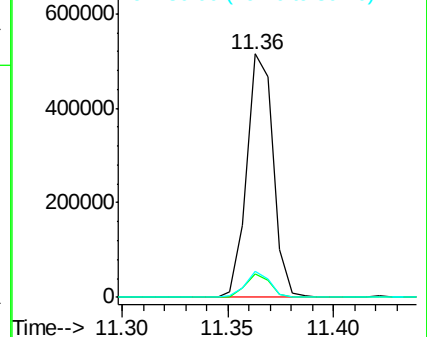

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.00 min Scan# 2026

Delta R.T. -0.01 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00


Tgt Ion:240 Resp: 286596

Ion Ratio Lower Upper

240 100

120 10.1 10.3 15.5#



236 26.4 21.4 32.2

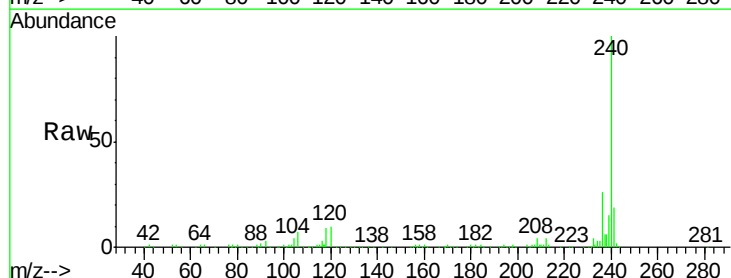


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

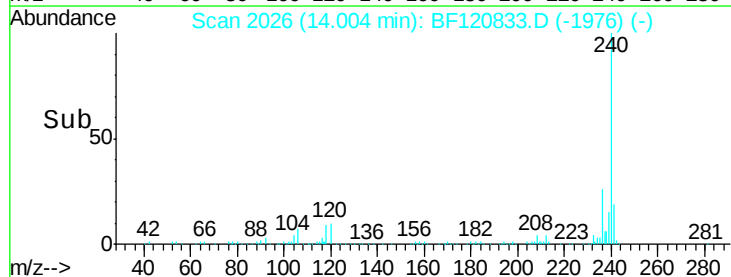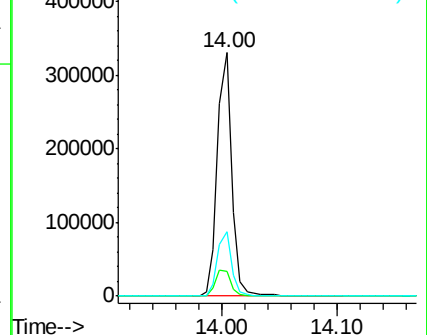

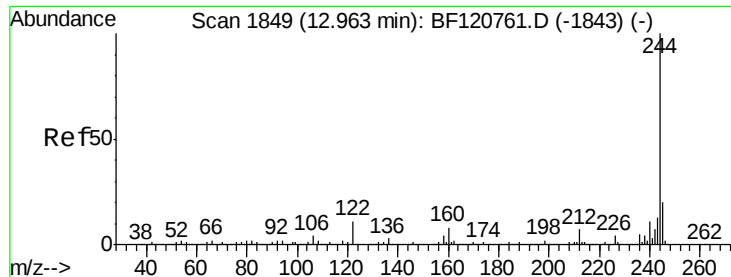

#79

Terphenyl-d14

Concen: 113.302 ng

RT: 12.96 min Scan# 1848

Delta R.T. -0.01 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00

Instrument :


BNA_F

ClientSampleId :

PB130117BL

Tot Ion:244 Resp: 1658518


Ion	Ratio	Lower	Upper
244	100		
212	7.1	5.6	8.4
122	11.1	9.0	13.4

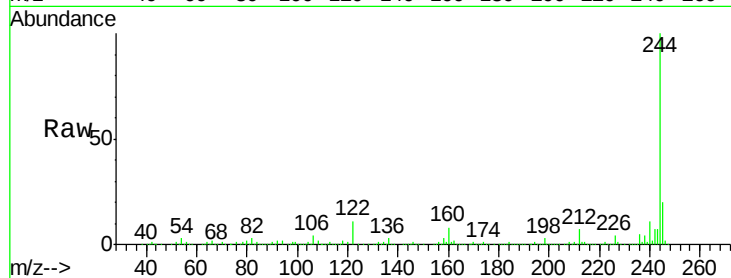


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

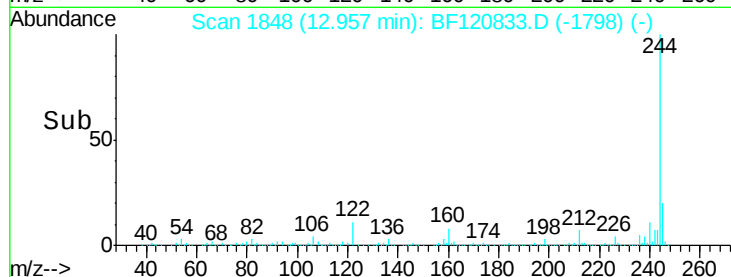

Time-->

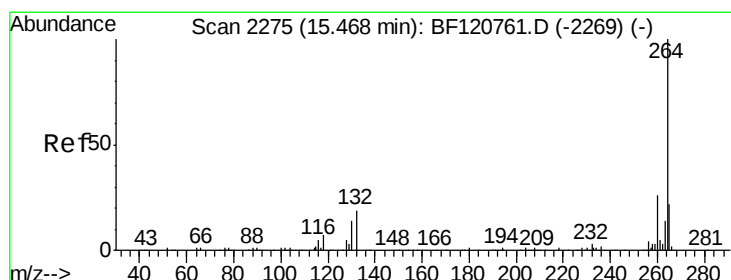

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2274


Delta R.T. -0.01 min

Lab File: BF120833.D

Acq: 10 Jul 2020 16:00

Tgt Ion:264 Resp: 233638



Ion	Ratio	Lower	Upper
264	100		
260	25.4	20.6	30.8
265	21.8	17.6	26.4

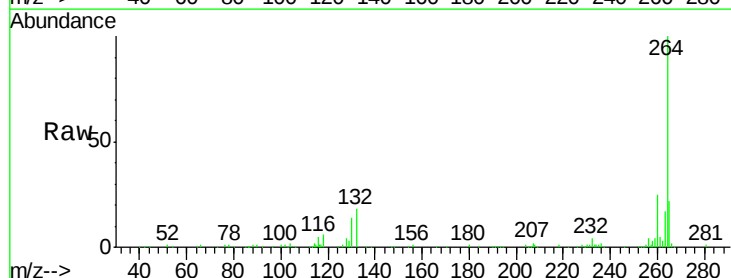

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

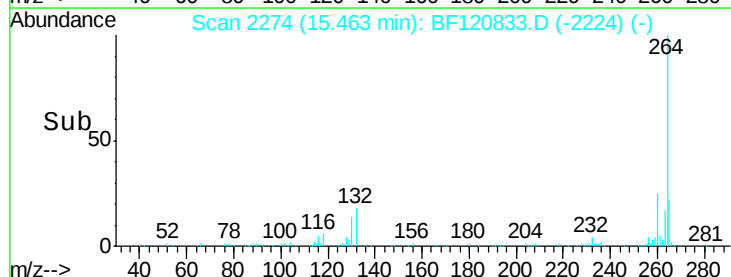

Time-->