

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071020\
Data File : BF120830.D
Acq On : 10 Jul 2020 14:34
Operator : JU/CG
Sample : PB130090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130090BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	567	573	576	rBV	3775092	4050848	89.60%	13.003%
2	6.469	739	745	748	rBV	3343856	4055978	89.72%	13.019%
3	6.845	806	809	813	rBV	1119259	850642	18.82%	2.730%
4	7.004	832	836	839	rBV	3875323	3468571	76.72%	11.134%
5	7.410	900	905	908	rBV	2859092	2657622	58.79%	8.531%
6	8.128	1023	1027	1030	rBV	1407354	1050103	23.23%	3.371%
7	9.210	1206	1211	1214	rBV	4462556	4520810	100.00%	14.511%
8	9.880	1322	1325	1329	rBV	1376815	1095359	24.23%	3.516%
9	10.669	1455	1459	1462	rBV	2890092	2670836	59.08%	8.573%
10	11.369	1574	1578	1581	rBV	1185939	1064809	23.55%	3.418%
11	12.957	1843	1848	1851	rBV	4339772	4310474	95.35%	13.836%
12	14.004	2022	2026	2035	rBV	859187	760542	16.82%	2.441%
13	15.462	2269	2274	2291	rBV	504913	597530	13.22%	1.918%


Sum of corrected areas: 31154124

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
Data File : BF120830.D
Acq On : 10 Jul 2020 14:34
Operator : JU/CG
Sample : PB130090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130090BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

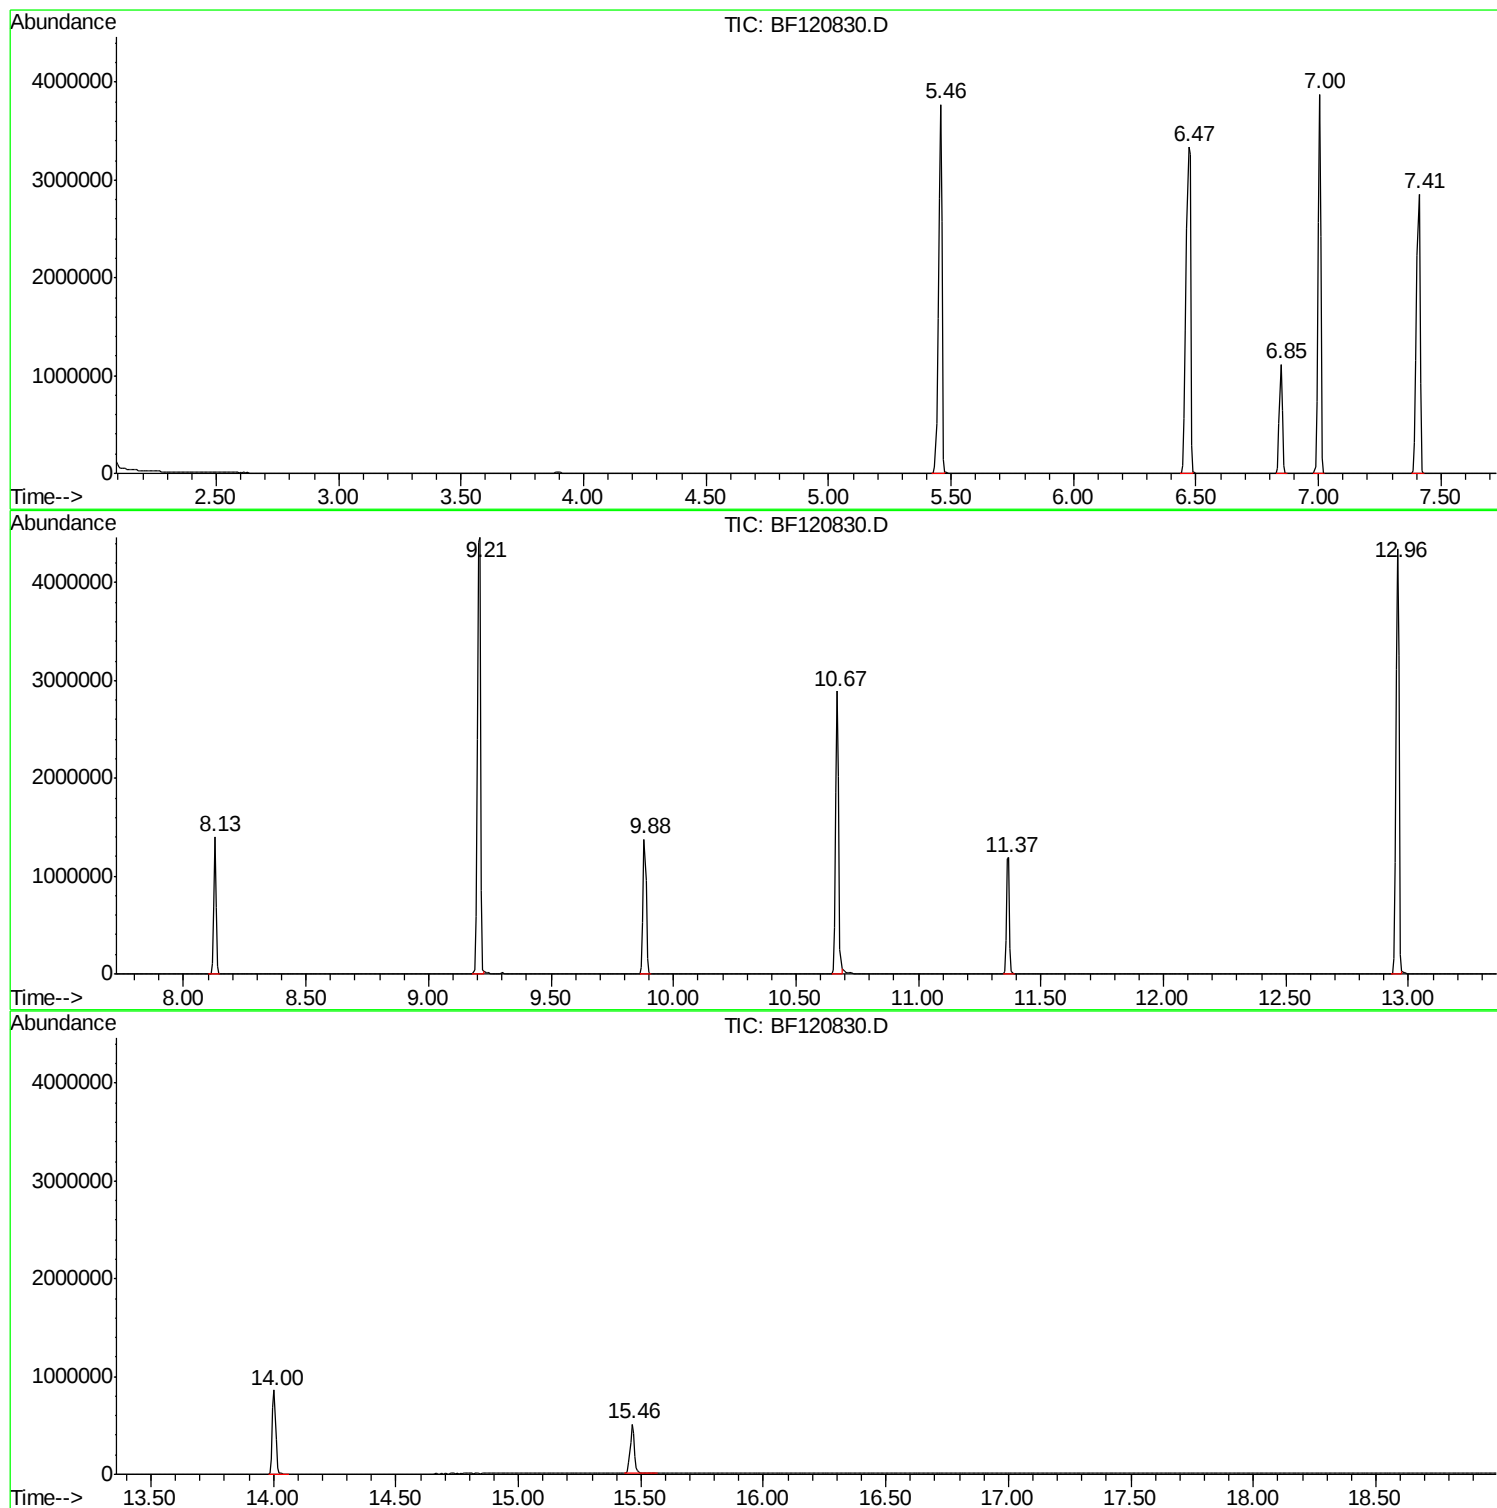

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071020\
Data File : BF120830.D
Acq On : 10 Jul 2020 14:34
Operator : JU/CG
Sample : PB130090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130090BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071020\
Data File : BF120830.D
Acq On : 10 Jul 2020 14:34
Operator : JU/CG
Sample : PB130090BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130090BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc