

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071020\
 Data File : BF120833.D
 Acq On : 10 Jul 2020 16:00
 Operator : JU/CG
 Sample : PB130117BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130117BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	567	573	576	rBV	3832003	4244461	94.41%	13.280%
2	6.475	739	746	748	rBV	3421372	4208163	93.61%	13.166%
3	6.845	806	809	812	rBV	1162996	870124	19.36%	2.722%
4	7.004	832	836	839	rBV	4005911	3574662	79.52%	11.184%
5	7.410	900	905	908	rBV	2947038	2757475	61.34%	8.627%
6	8.128	1023	1027	1030	rBV	1389723	1065790	23.71%	3.335%
7	9.210	1206	1211	1214	rBV	4789249	4495549	100.00%	14.065%
8	9.881	1322	1325	1329	rBV	1390136	1108212	24.65%	3.467%
9	10.669	1455	1459	1462	rBV	2897477	2742807	61.01%	8.581%
10	11.363	1574	1577	1581	rBV	1256596	1076186	23.94%	3.367%
11	12.957	1843	1848	1851	rBV	4407572	4408143	98.06%	13.792%
12	14.004	2022	2026	2036	rBV	891039	779694	17.34%	2.439%
13	15.463	2269	2274	2291	rBV	516446	630775	14.03%	1.974%


Sum of corrected areas: 31962041

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071020\
Data File : BF120833.D
Acq On : 10 Jul 2020 16:00
Operator : JU/CG
Sample : PB130117BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130117BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

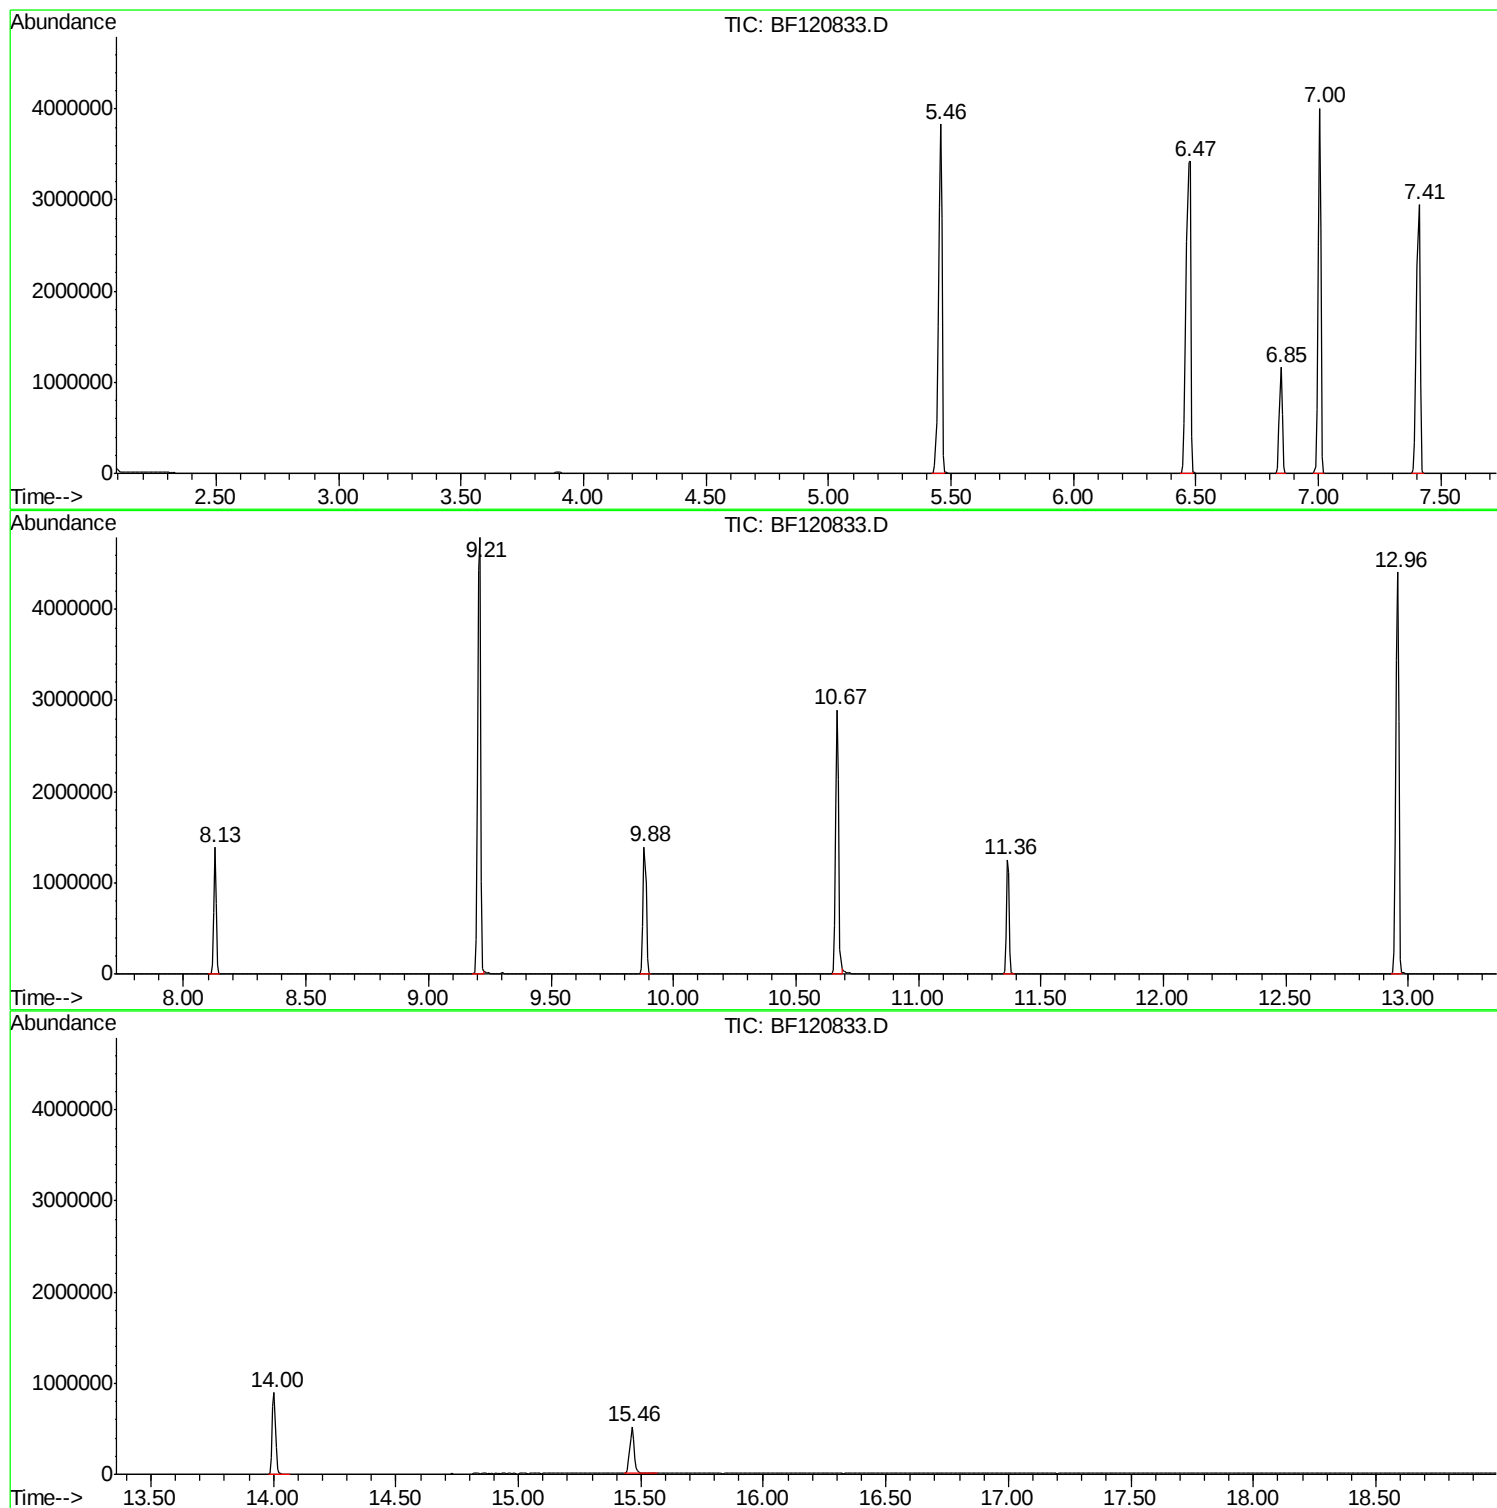

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071020\
Data File : BF120833.D
Acq On : 10 Jul 2020 16:00
Operator : JU/CG
Sample : PB130117BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130117BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF071020\
Data File : BF120833.D
Acq On : 10 Jul 2020 16:00
Operator : JU/CG
Sample : PB130117BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130117BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc