


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071020\
 Data File : BF120827.D
 Acq On : 10 Jul 2020 13:08
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 18:51:52 2020

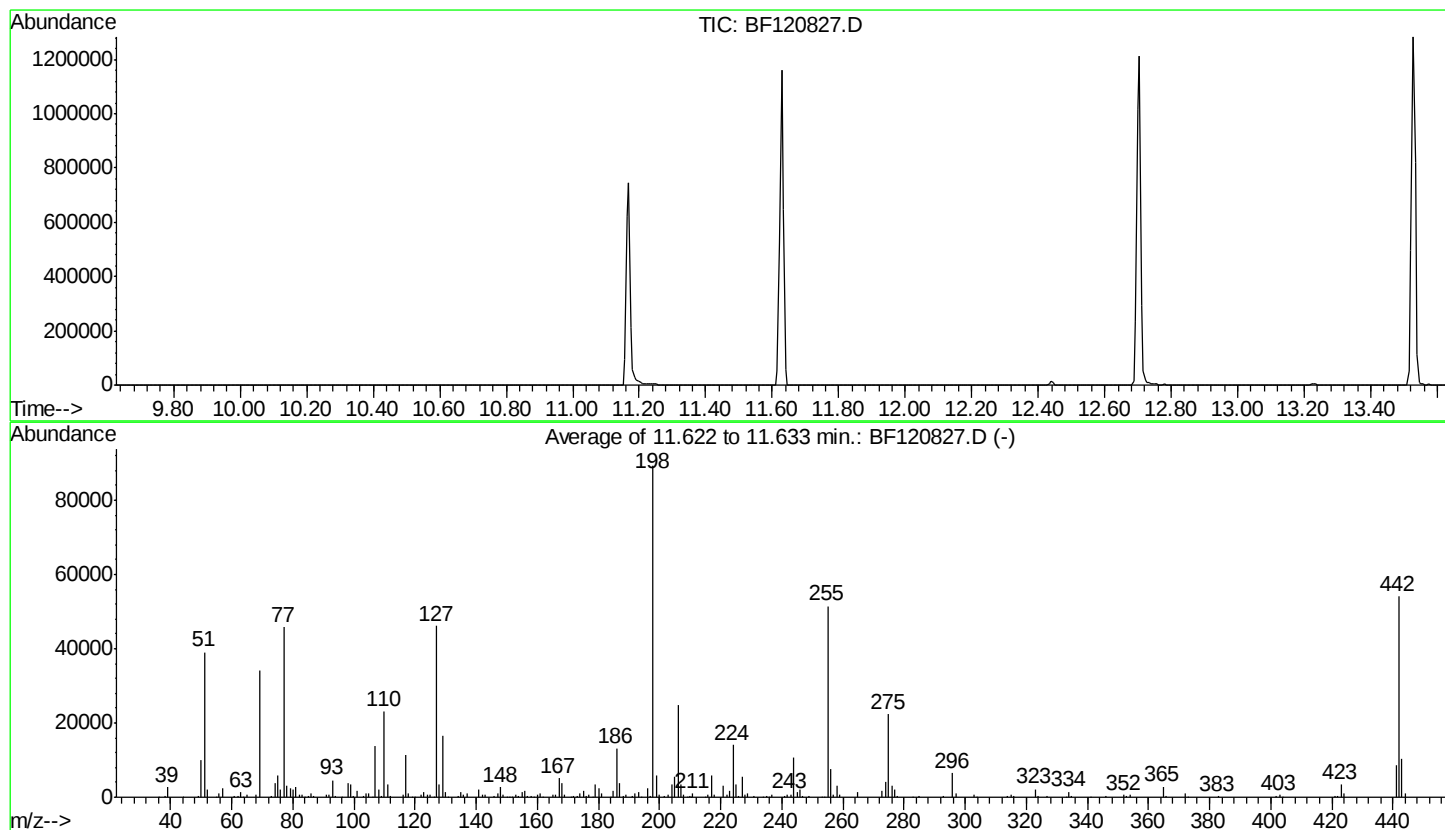

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	39040	PASS
68	69	0.00	2	1.8	602	PASS
69	198	0.00	100	38.3	34213	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	46181	PASS
197	198	0.00	2	0.4	367	PASS
198	198	100	100	100.0	89341	PASS
199	198	5	9	6.8	6046	PASS
275	198	10	60	24.9	22265	PASS
365	198	1	100	3.2	2851	PASS
441	198	0.01	100	9.6	8616	PASS
442	198	50	100	60.4	53995	PASS
443	442	15	24	19.1	10300	PASS