
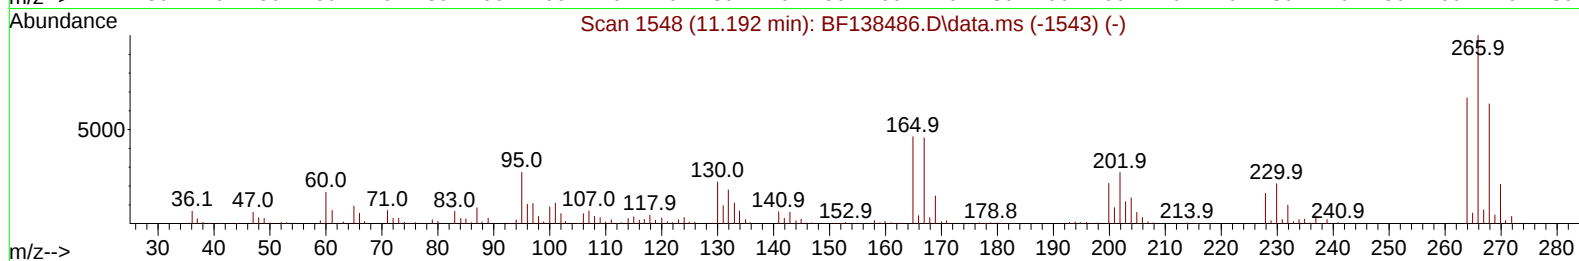
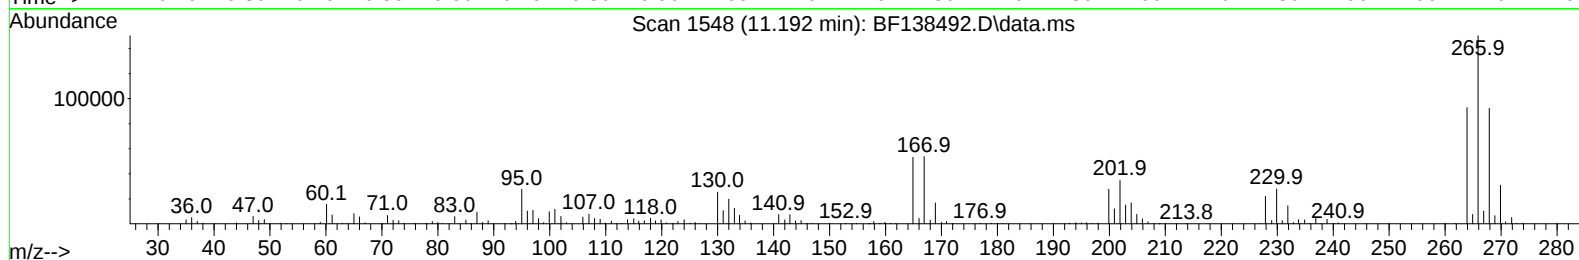


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071024\
Data File : BF138492.D
Acq On : 10 Jul 2024 10:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 12:49:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

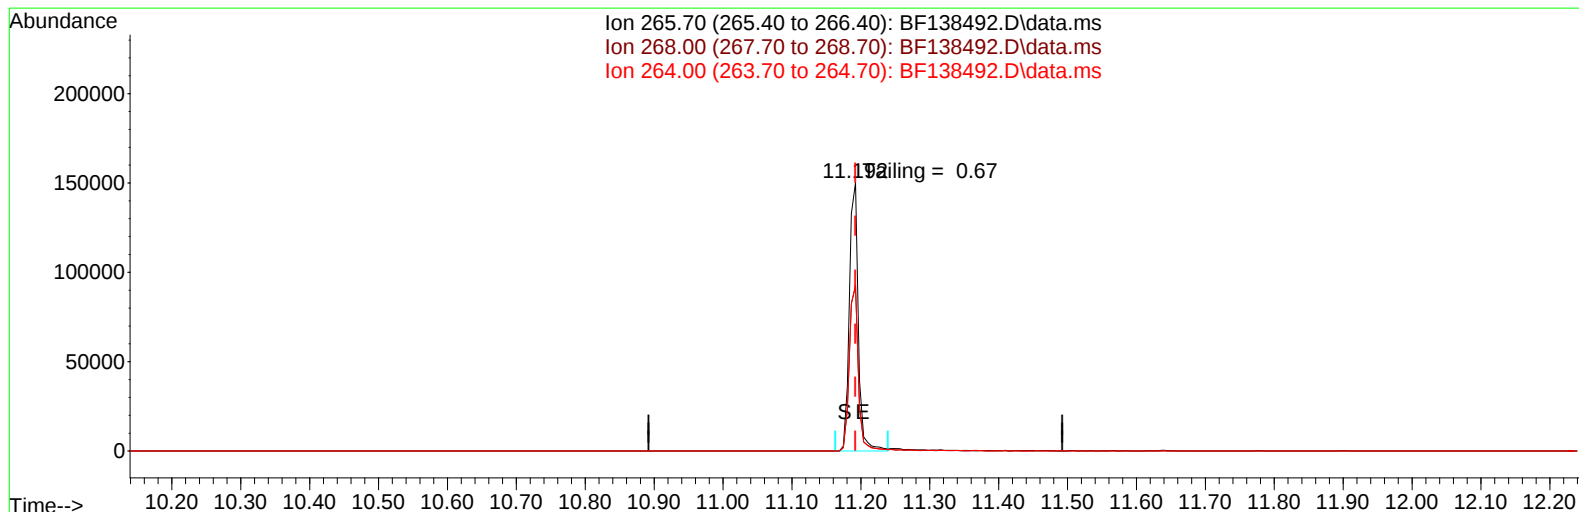

TIC: BF138492.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.000) 345859.61 ng

response 135534

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	61.39
264.00	66.90	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071024\
Data File : BF138492.D
Acq On : 10 Jul 2024 10:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 12:49:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

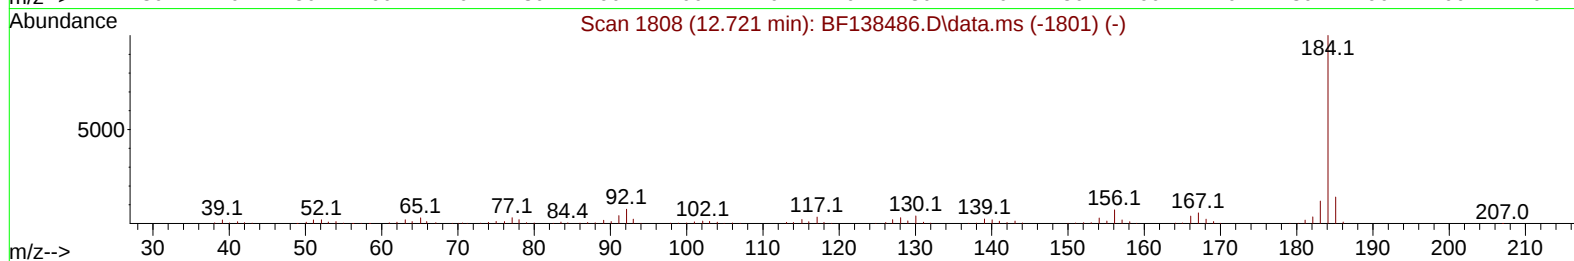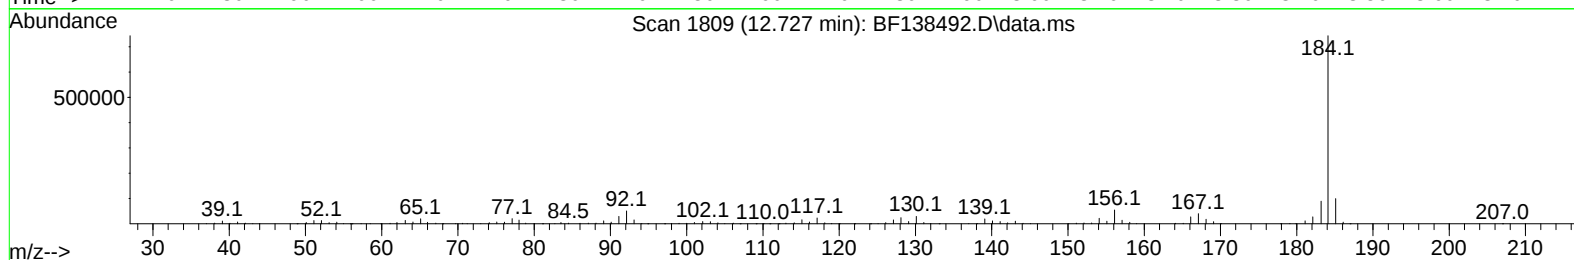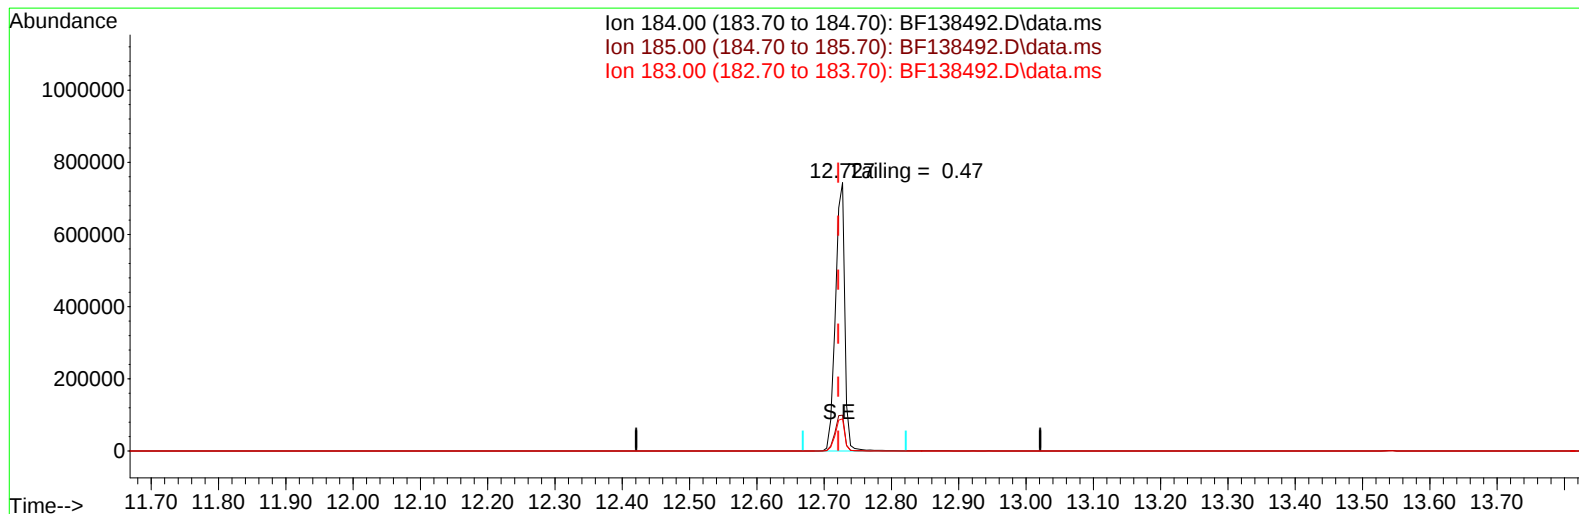

TIC: BF138492.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 345787.60 ng

response 715382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.39
183.00	11.90	12.02
0.00	0.00	0.00