


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071024\
Data File : BF138492.D
Acq On : 10 Jul 2024 10:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

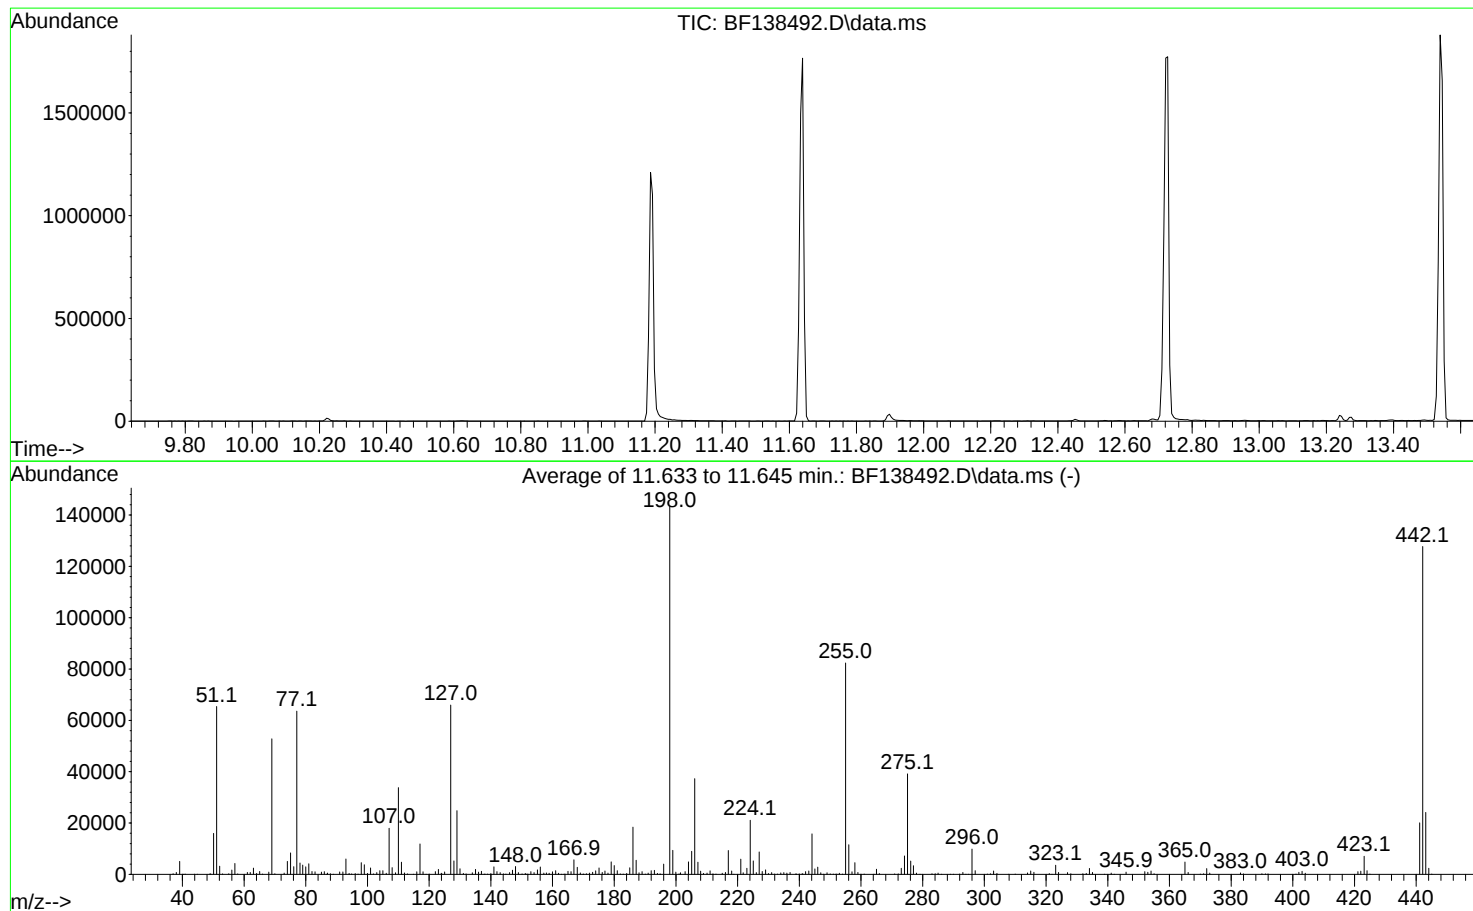

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	65372	PASS
68	69	0.00	2	1.6	849	PASS
69	198	0.00	100	36.8	52780	PASS
70	69	0.00	2	0.5	242	PASS
127	198	10	80	46.0	65968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143323	PASS
199	198	5	9	6.5	9344	PASS
275	198	10	60	27.3	39179	PASS
365	198	1	100	3.4	4833	PASS
441	198	0.01	100	14.0	20094	PASS
442	442	50	100	100.0	127736	PASS
443	442	15	24	18.9	24149	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/10/2024	BNA_F	<u>BF138492.D</u>
Compound Name	Response	Retention Time
DDT	324236	13.539
DDD	7711	13.245
DDE	311	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8022	332258	2.41

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071024\
Data File : BF138492.D
Acq On : 10 Jul 2024 10:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 10 12:49:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

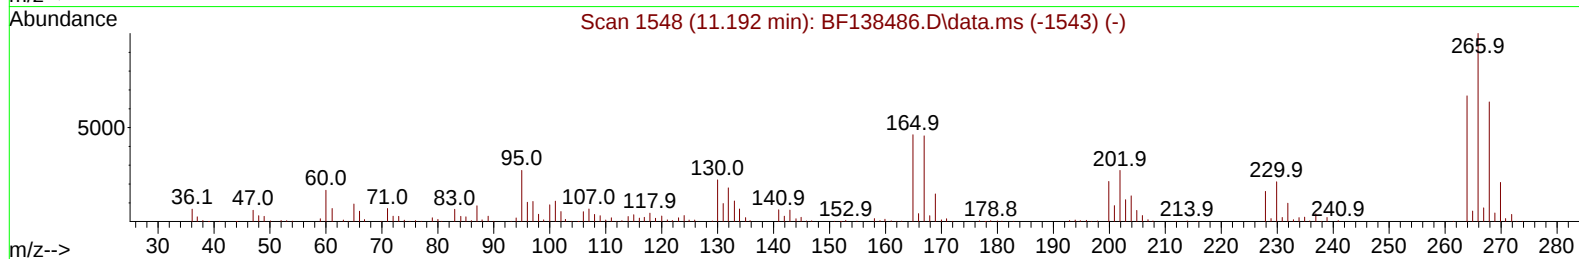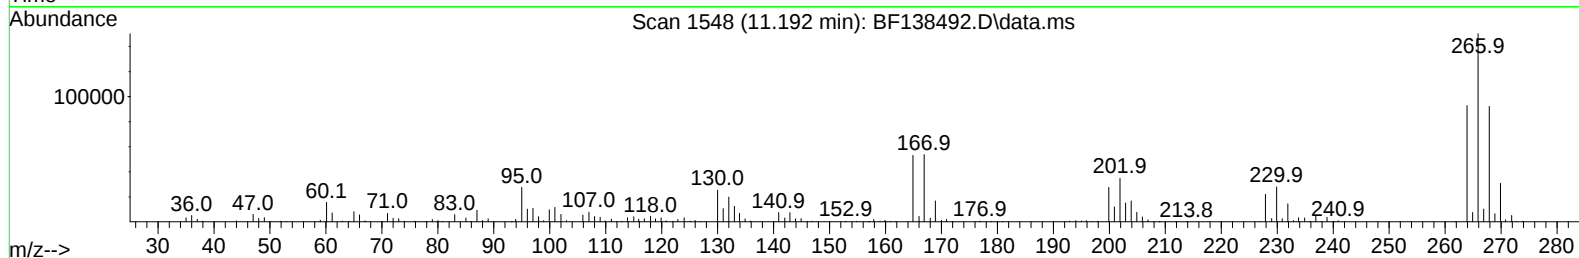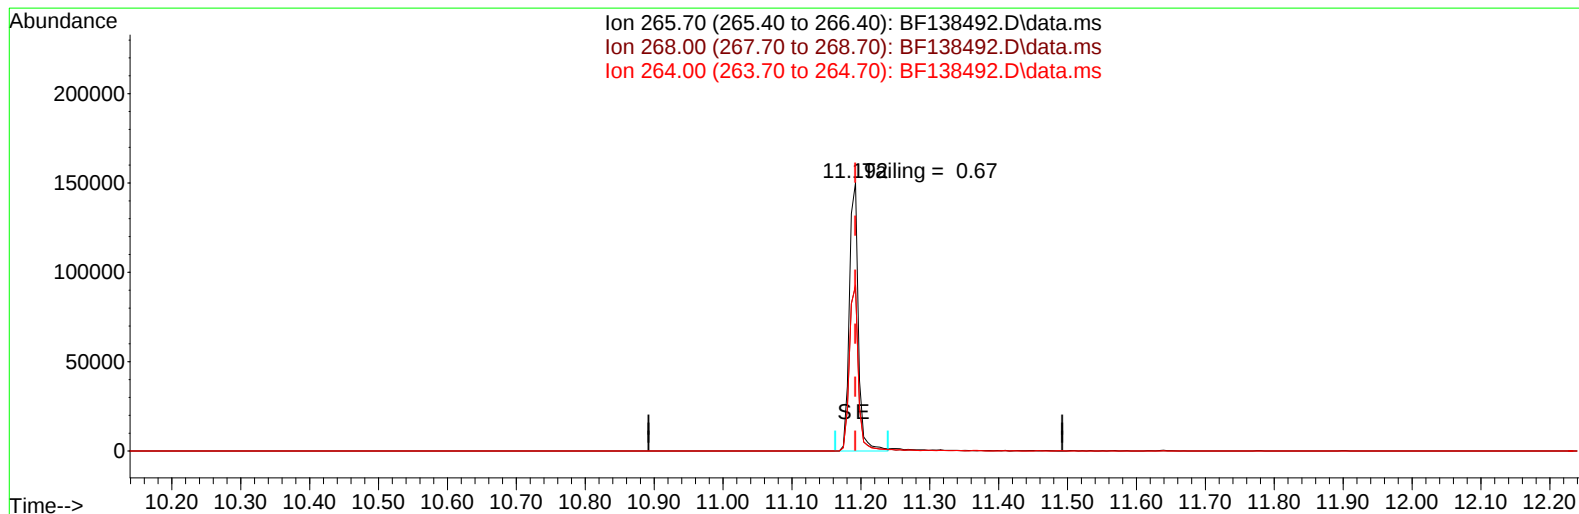

TIC: BF138492.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 345859.61 ng




response 135534

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	61.39
264.00	66.90	61.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071024\
Data File : BF138492.D
Acq On : 10 Jul 2024 10:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 10 12:49:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

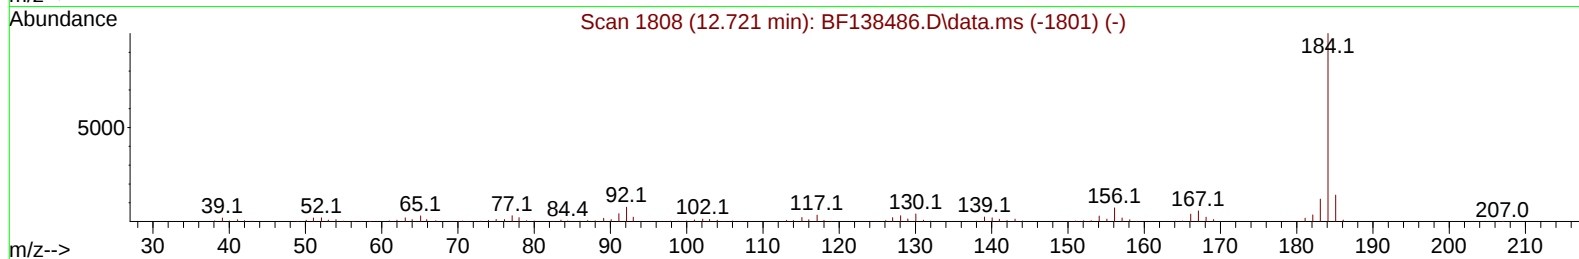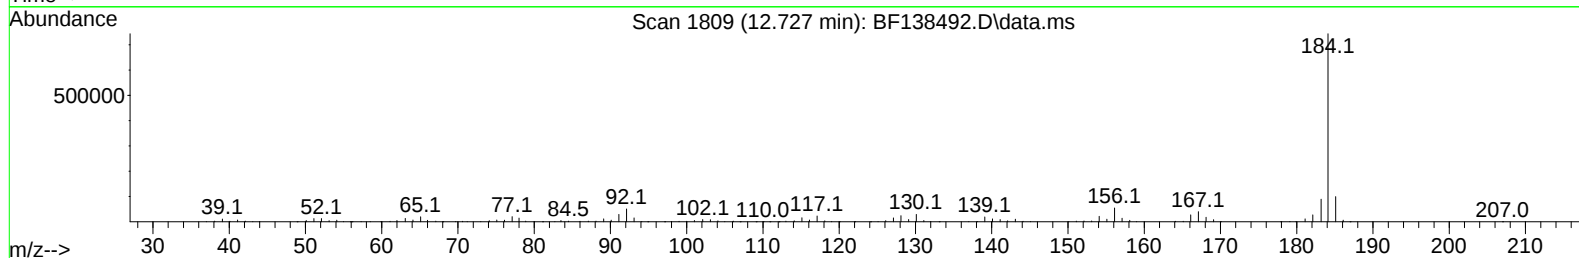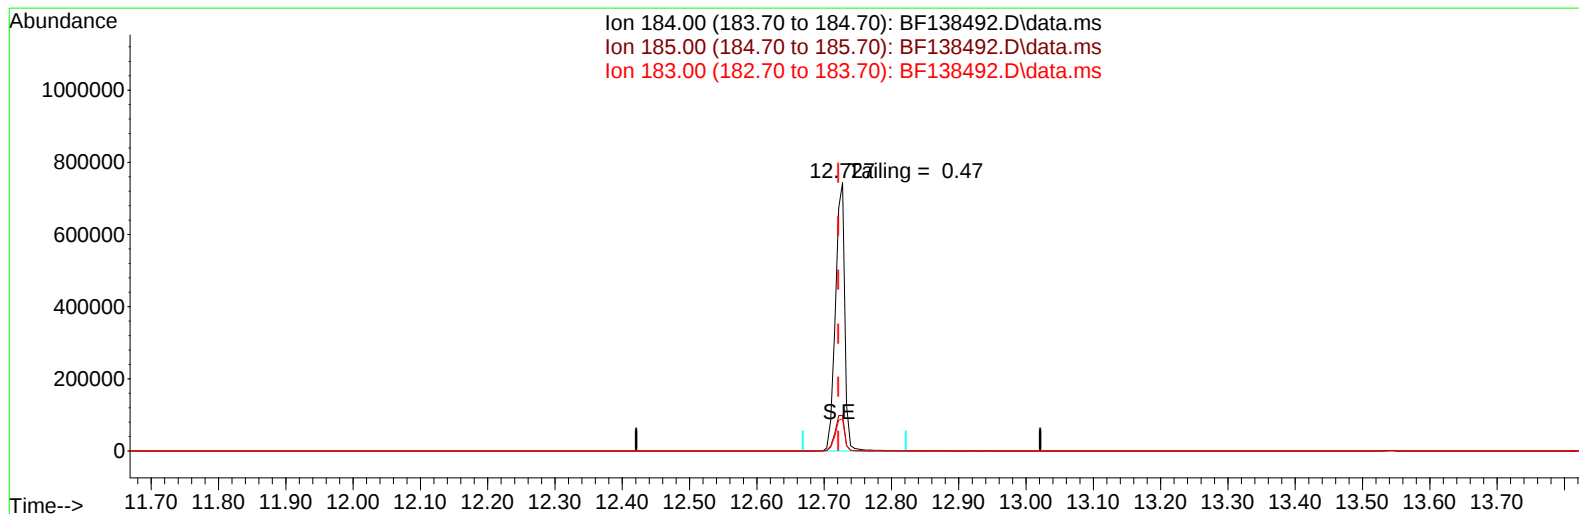

TIC: BF138492.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 345787.60 ng

response 715382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.39
183.00	11.90	12.02
0.00	0.00	0.00