


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF071116\
 Data File : BF088897.D
 Acq On : 11 Jul 2016 12:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 11 18:13:32 2016

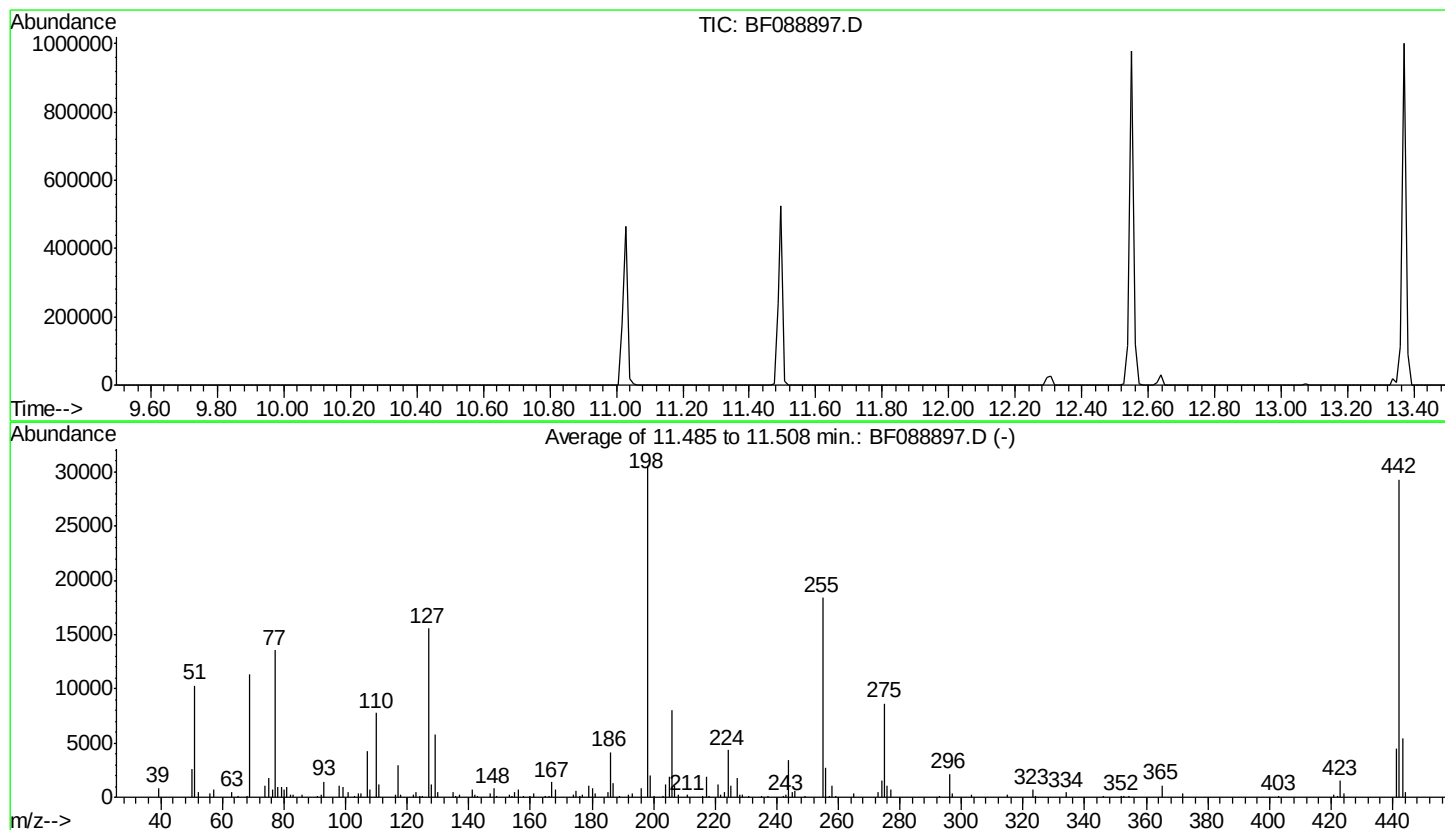

AutoFind: Scans 866, 867, 868; Background Corrected with Scan 862

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	10289	PASS
68	69	0.00	2	1.1	126	PASS
69	198	0.00	100	37.1	11329	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	15536	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	30565	PASS
199	198	5	9	6.6	2004	PASS
275	198	10	60	28.2	8626	PASS
365	198	1	100	3.5	1076	PASS
441	442	0.01	24	15.3	4486	PASS
442	198	50	100	95.7	29262	PASS
443	442	15	24	18.8	5490	PASS