


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071117\
Data File : BF096634.D
Acq On : 11 Jul 2017 10:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 07 13:02:33 2017

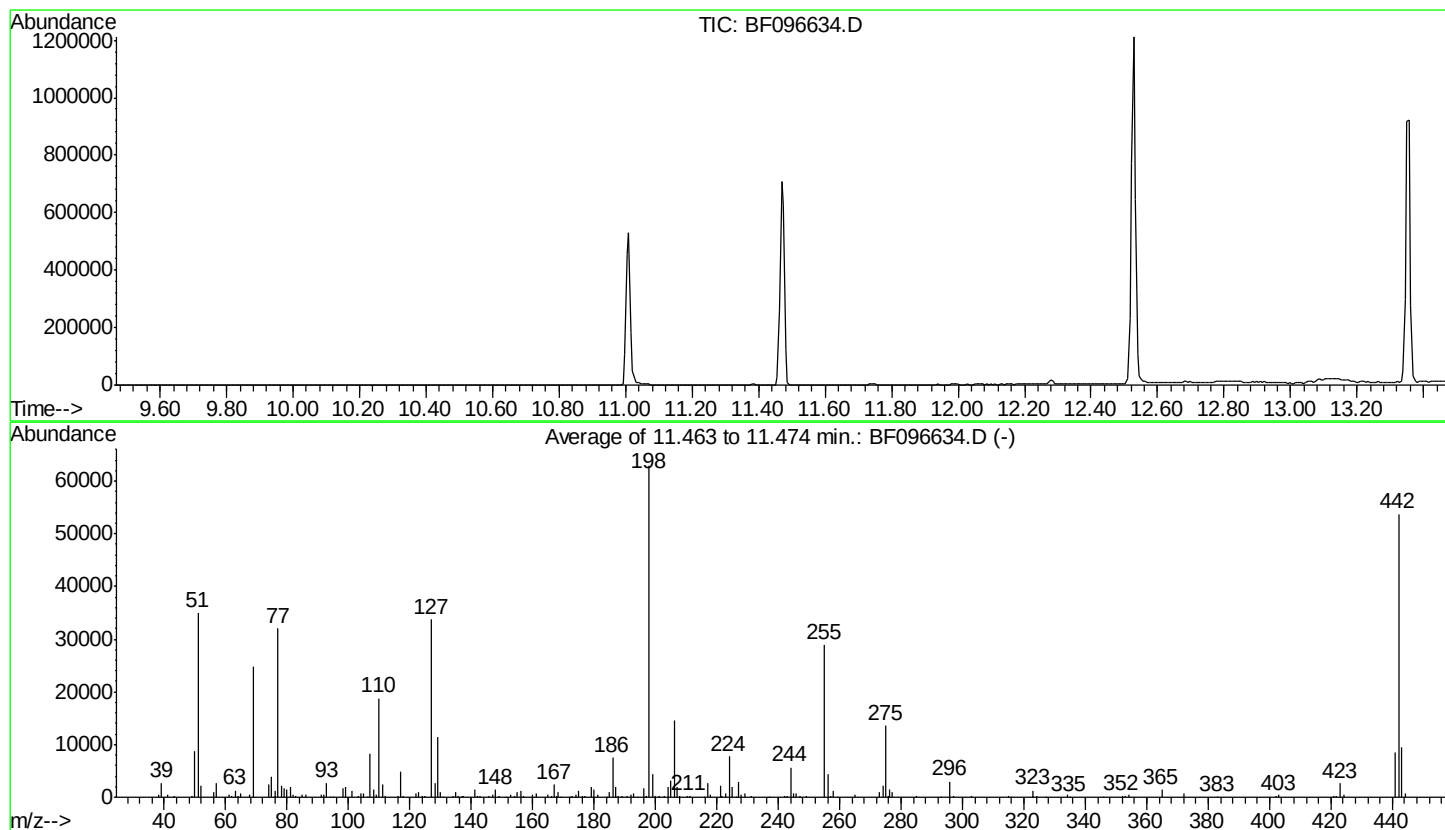

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.8	35088	PASS
68	69	0.00	2	2.0	486	PASS
69	198	0.00	100	39.6	24897	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	33658	PASS
197	198	0.00	2	0.4	223	PASS
198	198	100	100	100.0	62933	PASS
199	198	5	9	7.0	4416	PASS
275	198	10	60	21.5	13539	PASS
365	198	1	100	2.2	1355	PASS
441	442	0.01	24	15.7	8411	PASS
442	198	50	100	85.4	53721	PASS
443	442	15	24	17.9	9599	PASS