


Data Path : Z:\HPCHEM1\BNA_F\Data\BF071117\
 Data File : BF096660.D
 Acq On : 11 Jul 2017 23:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 07 13:02:33 2017

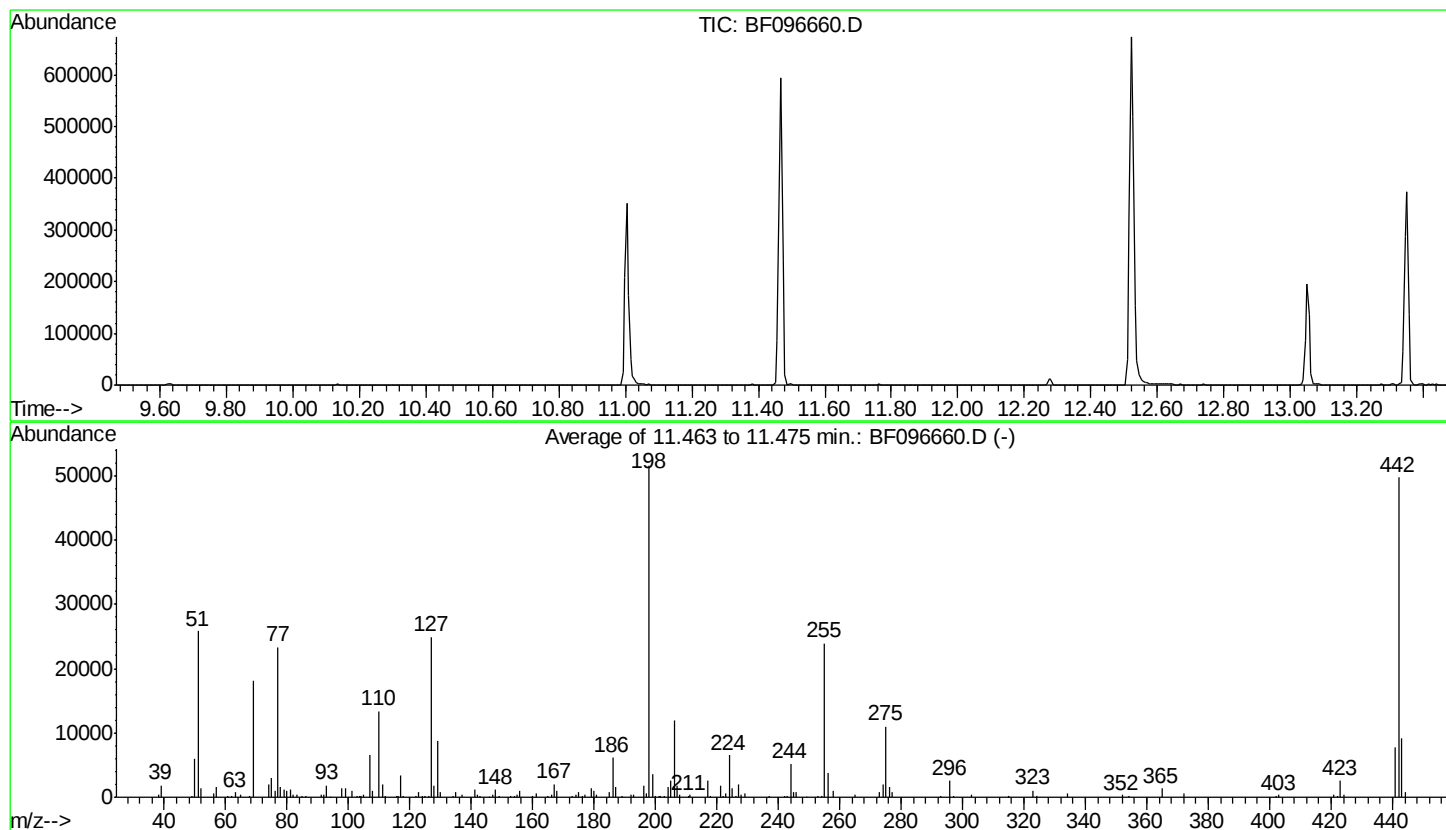

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.0	25780	PASS
68	69	0.00	2	1.0	181	PASS
69	198	0.00	100	35.2	18143	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	24945	PASS
197	198	0.00	2	1.1	589	PASS
198	198	100	100	100.0	51557	PASS
199	198	5	9	6.9	3542	PASS
275	198	10	60	21.4	11024	PASS
365	198	1	100	2.6	1315	PASS
441	442	0.01	24	15.8	7838	PASS
442	198	50	100	96.3	49672	PASS
443	442	15	24	18.6	9256	PASS