
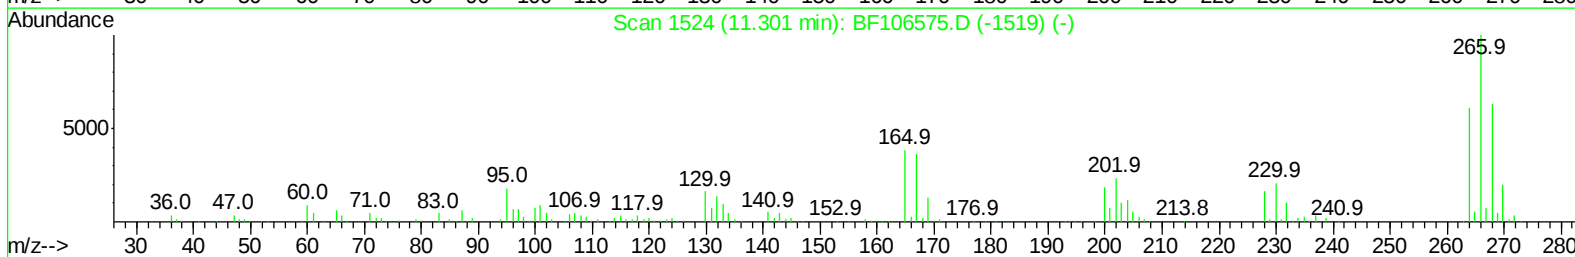
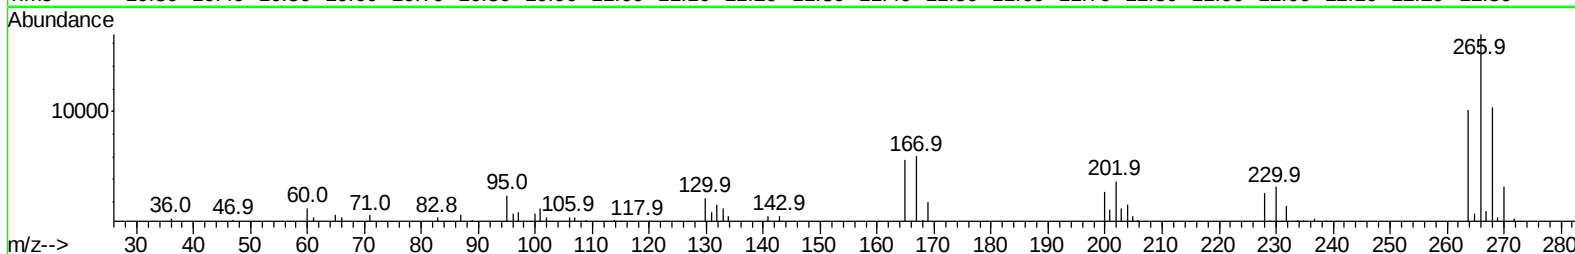


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071118\
Data File : BF107294.D
Acq On : 11 Jul 2018 11:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 09:35:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 11 16:39:37 2018
Response via : Initial Calibration

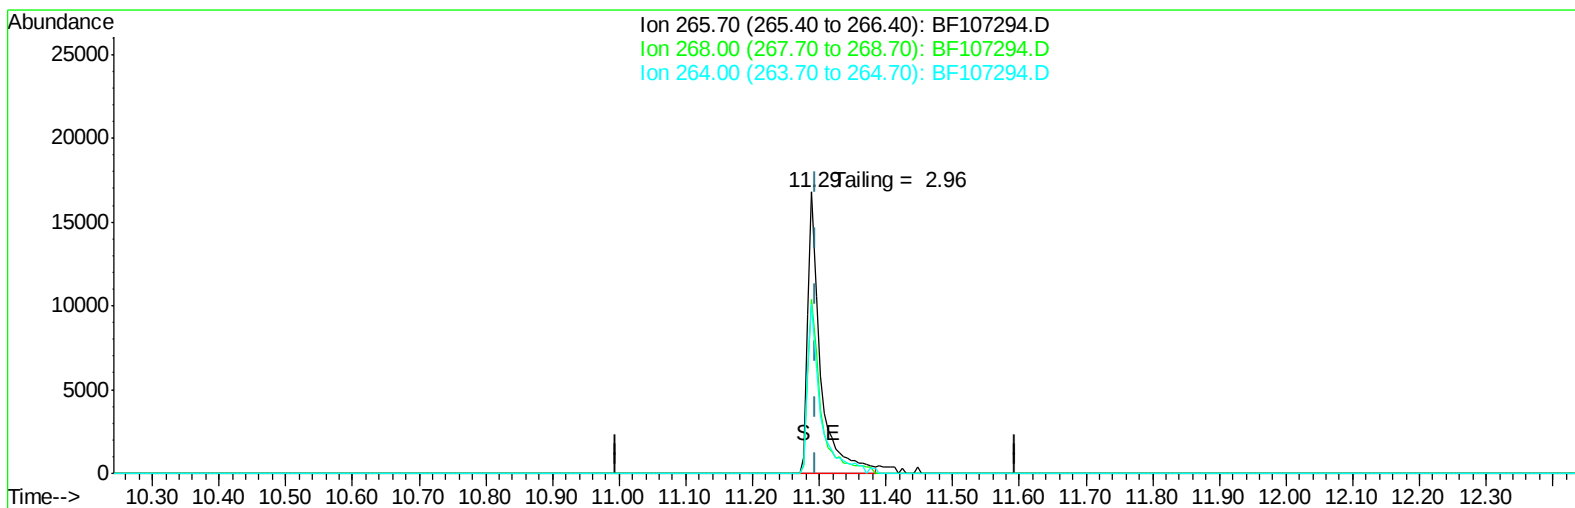

TIC: BF107294.D

(69) Pentachlorophenol (C)




11.289min (-0.006) 29696.18ng

response 22210

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.72
264.00	61.90	60.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071118\
 Data File : BF107294.D
 Acq On : 11 Jul 2018 11:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 09:35:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 11 16:39:37 2018
 Response via : Initial Calibration

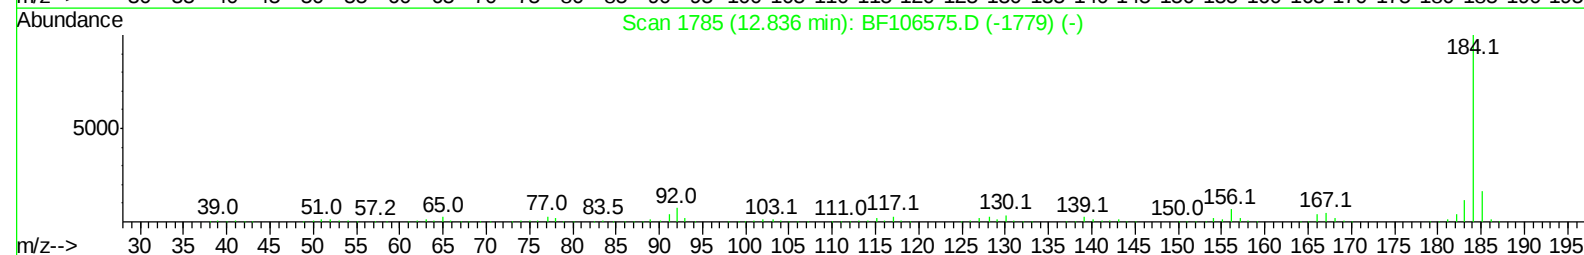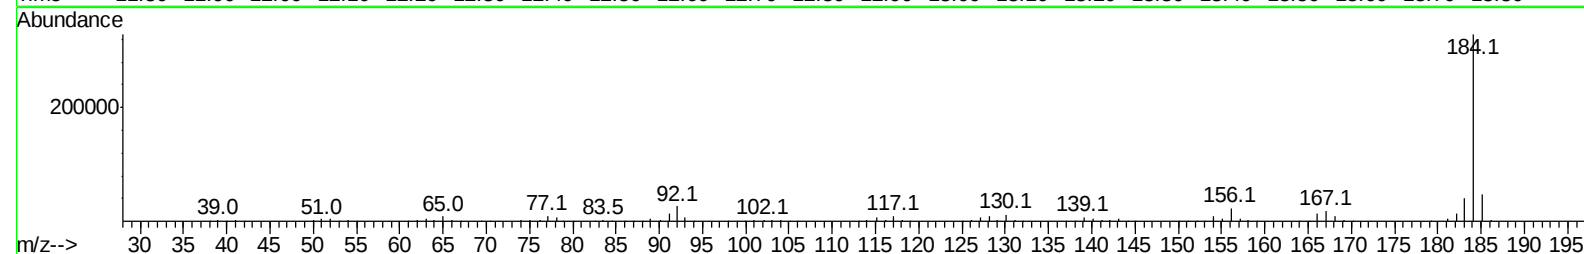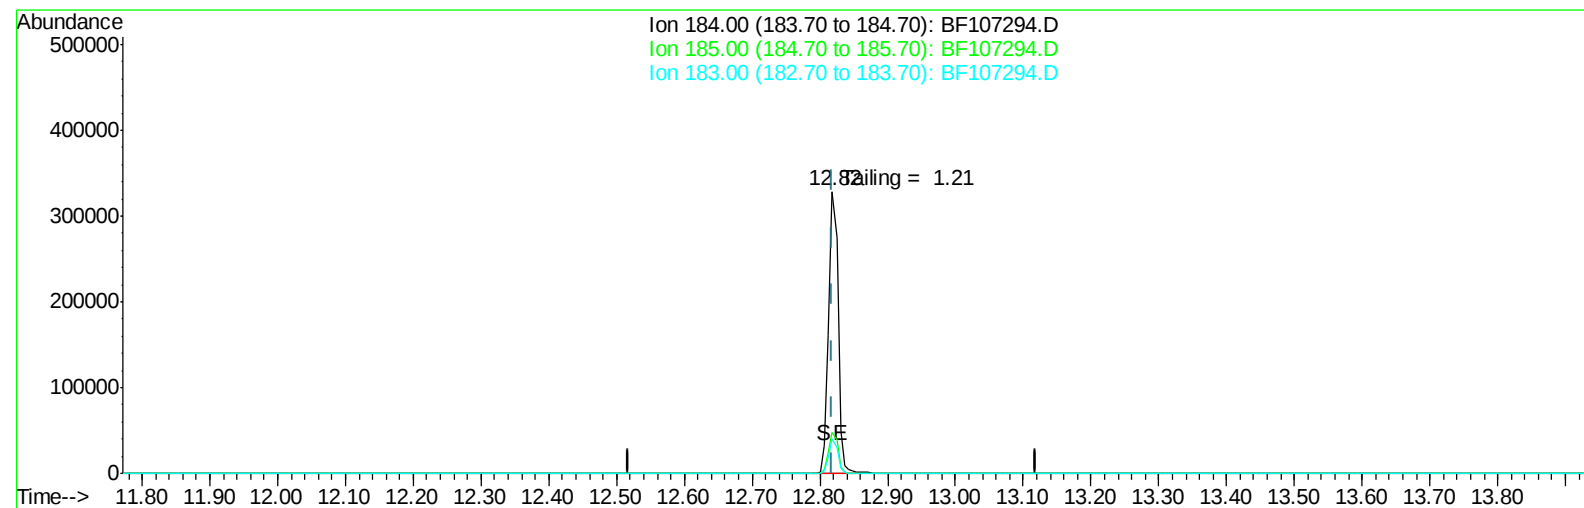

TIC: BF107294.D

(76) Benzidine

12.819min (-0.000) 0.00ng

response 307784

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.63
183.00	11.60	12.18
0.00	0.00	0.00